

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059632.D
 Acq On : 28 Jun 2024 19:53
 Operator : MD/SY
 Sample : P3068-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCL20

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.387	24	30	40	rBV	11242	12602	2.50%	0.311%
2	1.596	86	95	111	rBV	47884	56988	11.32%	1.406%
3	1.907	184	192	212	rVB	51361	71204	14.14%	1.756%
4	2.560	380	395	410	rBV	88227	144789	28.76%	3.572%
5	2.785	451	465	489	rBV2	9407	34720	6.90%	0.856%
6	3.039	535	544	556	rVB6	3814	7392	1.47%	0.182%
7	4.618	1026	1035	1065	rBV2	72519	197208	39.17%	4.865%
8	4.814	1086	1096	1117	rVB4	4314	10515	2.09%	0.259%
9	5.055	1156	1171	1202	rBV	96177	223808	44.46%	5.521%
10	5.718	1358	1377	1407	rBV2	185542	484029	96.15%	11.940%
11	6.245	1528	1541	1567	rBV	154861	304766	60.54%	7.518%
12	6.544	1620	1634	1642	rBV5	3536	7272	1.44%	0.179%
13	6.685	1664	1678	1696	rBV	118880	232035	46.09%	5.724%
14	7.560	1940	1950	1970	rBV	46656	85346	16.95%	2.105%
15	7.894	2038	2054	2076	rBV	208620	367594	73.02%	9.068%
16	8.177	2132	2142	2159	rBV	28756	50076	9.95%	1.235%
17	8.627	2271	2282	2321	rBV	257078	503434	100.00%	12.419%
18	9.412	2512	2526	2551	rBV	240123	408869	81.22%	10.086%
19	10.750	2930	2942	2960	rBV	102940	168275	33.43%	4.151%
20	11.807	3260	3271	3295	rBV	209123	346087	68.75%	8.537%
21	12.187	3377	3389	3418	rBV	194945	336890	66.92%	8.310%




Sum of corrected areas: 4053899

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059632.D
Acq On : 28 Jun 2024 19:53
Operator : MD/SY
Sample : P3068-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCL20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

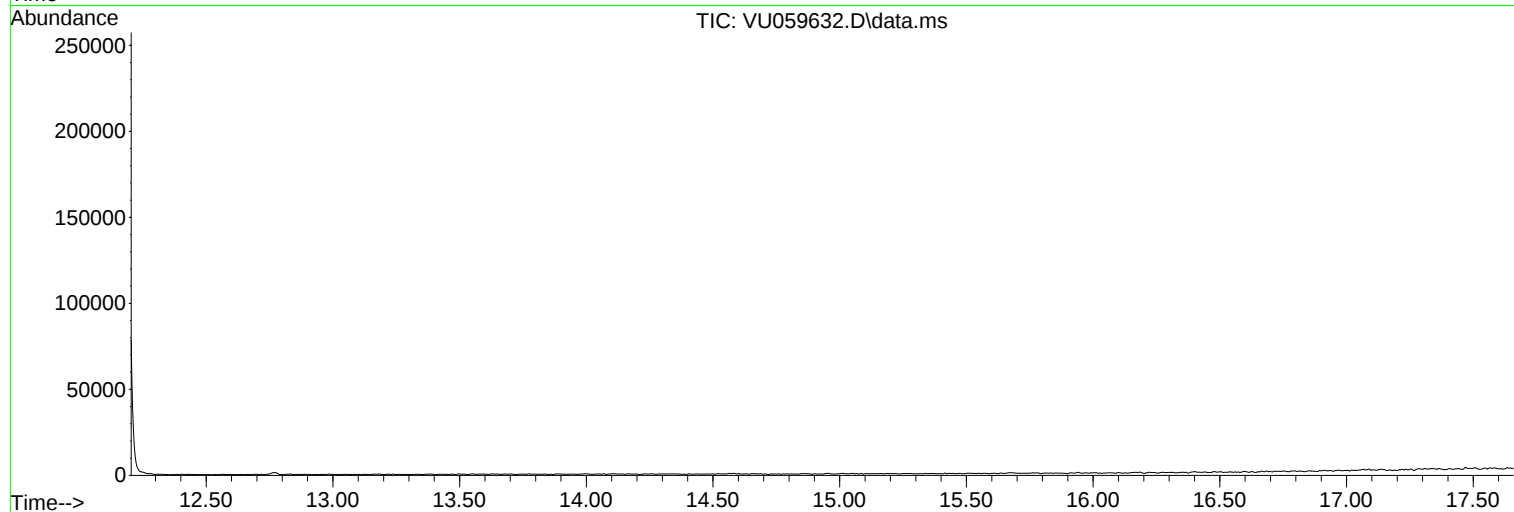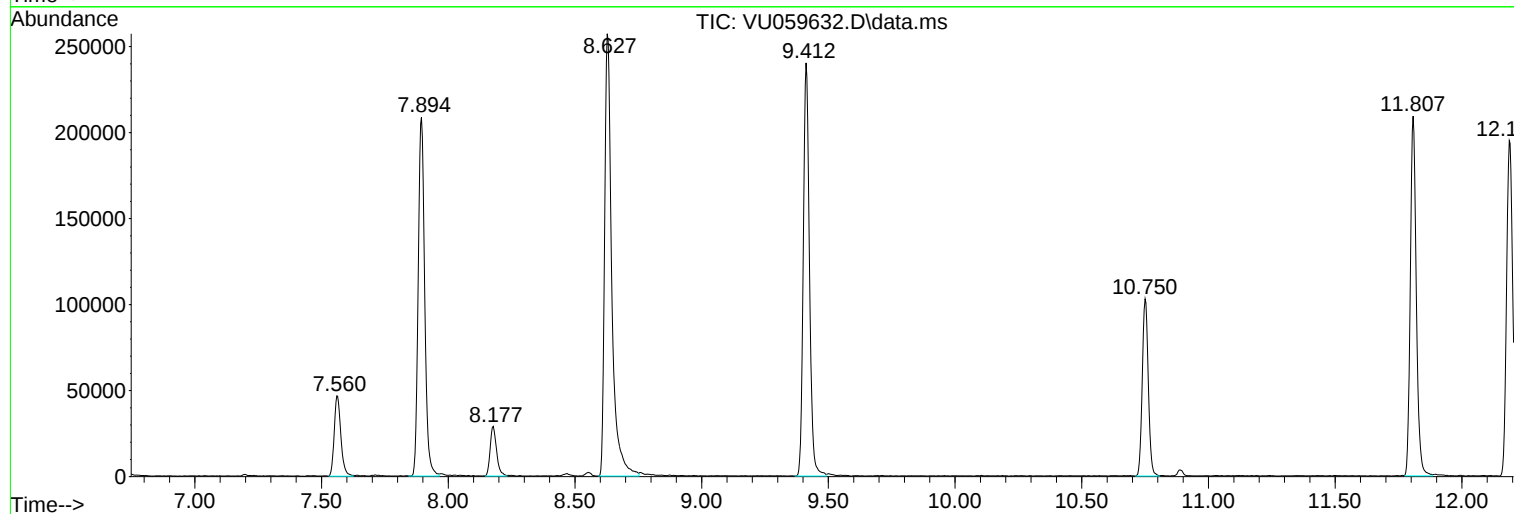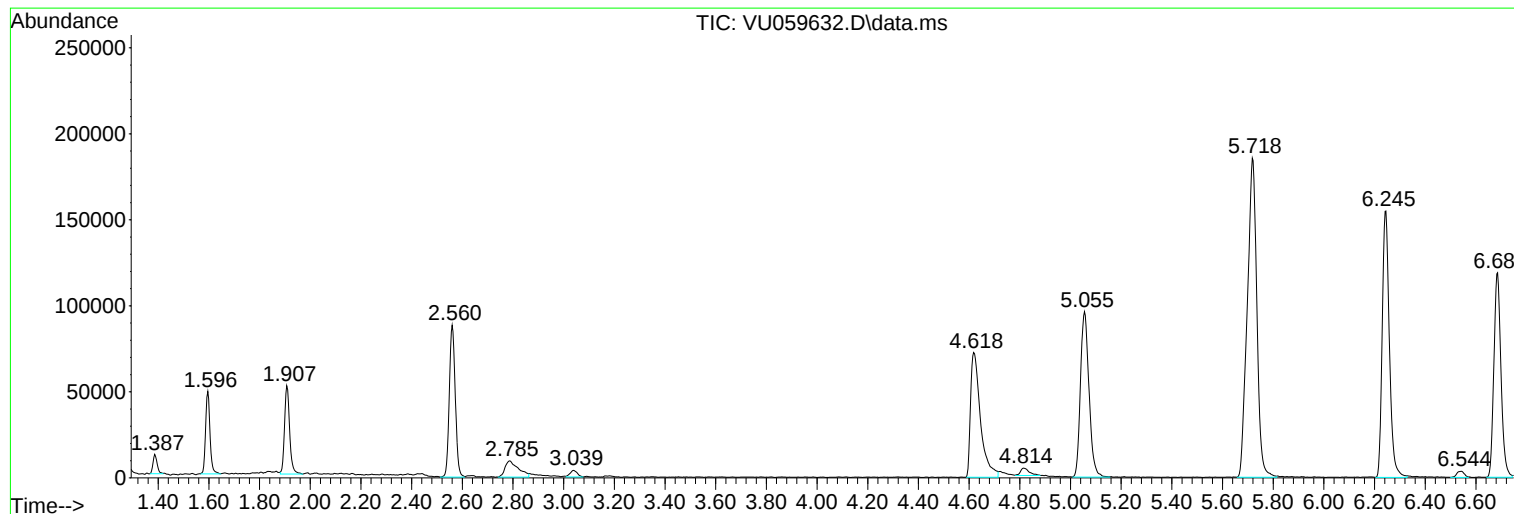

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059632.D
Acq On : 28 Jun 2024 19:53
Operator : MD/SY
Sample : P3068-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCL20










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.785	0.57 ug/L	34720	1,4-Difluorobenzene	6.242

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Propane, 2-ethoxy-	88	C5H12O	000625-54-7	9
2		Ethanol, 2-methoxy-	76	C3H8O2	000109-86-4	5
3		Ethanol, 2-methoxy-	76	C3H8O2	000109-86-4	5
4		2-Hydrazinoethanol	76	C2H8N2O	000109-84-2	5
5		Ethanol, 2-methoxy-	76	C3H8O2	000109-86-4	5

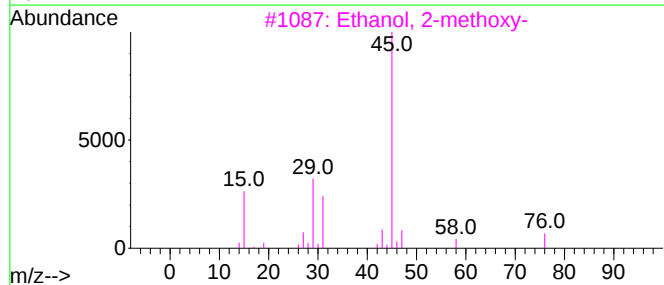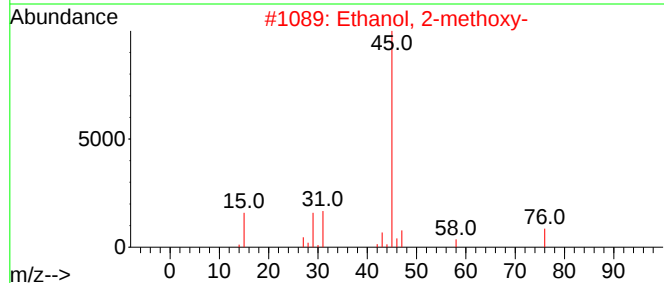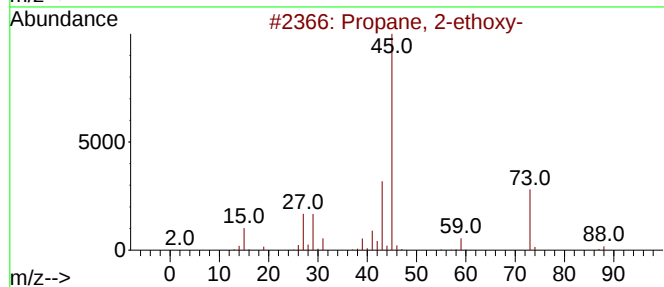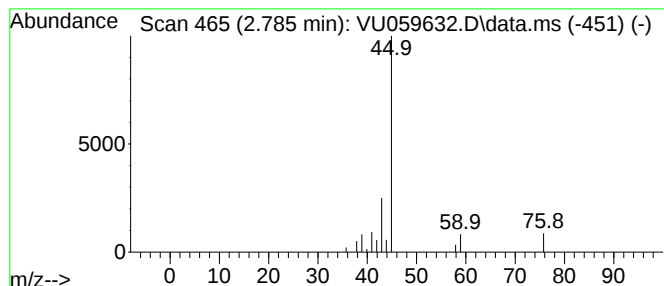

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059632.D
Acq On : 28 Jun 2024 19:53
Operator : MD/SY
Sample : P3068-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCL20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	2.785	0.6	ug/L	34720	1	6.242	304766	5.0