

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059645.D
Acq On : 29 Jun 2024 01:00
Operator : MD/SY
Sample : P3059-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.447	346	360	383	rVB	517048	844212	2.42%	2.198%
2	2.791	443	467	538	rBV	10663848	34956226	100.00%	91.033%
3	4.656	1020	1047	1074	rBV2	150682	548622	1.57%	1.429%
4	5.717	1358	1377	1410	rBV2	180175	471660	1.35%	1.228%
5	7.891	2042	2053	2072	rBV	205076	363399	1.04%	0.946%
6	8.627	2267	2282	2316	rBV	228570	440905	1.26%	1.148%
7	9.412	2512	2526	2550	rBV	245868	415702	1.19%	1.083%
8	11.807	3259	3271	3292	rBV	215295	358961	1.03%	0.935%




Sum of corrected areas: 38399687

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059645.D
Acq On : 29 Jun 2024 01:00
Operator : MD/SY
Sample : P3059-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

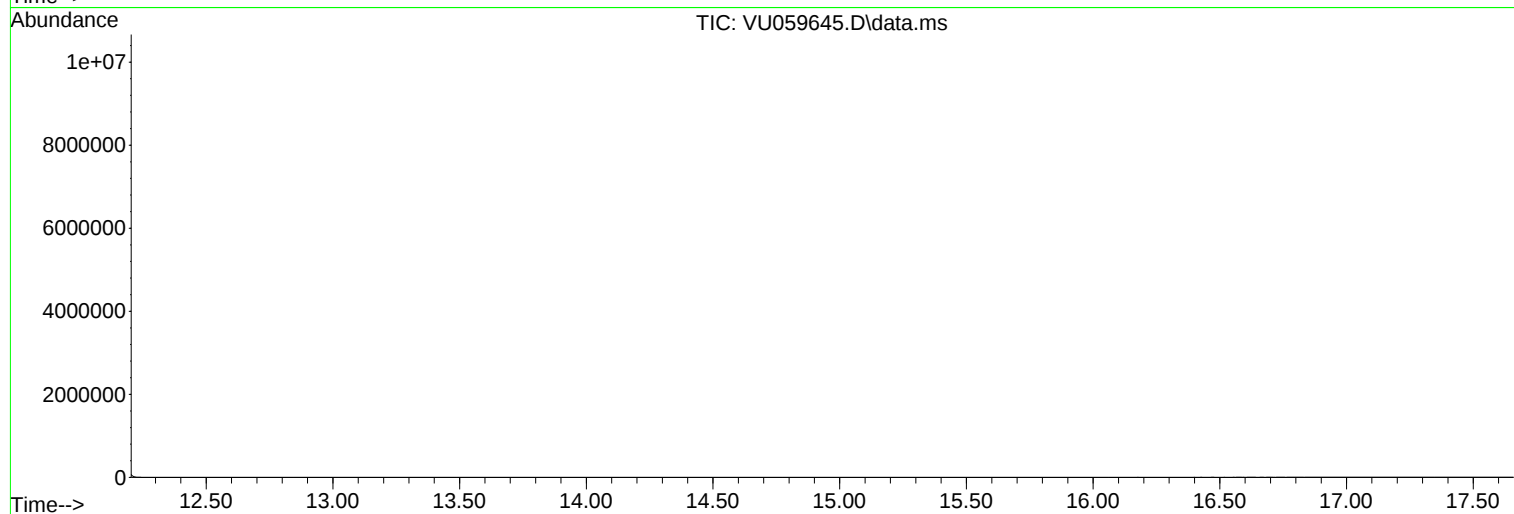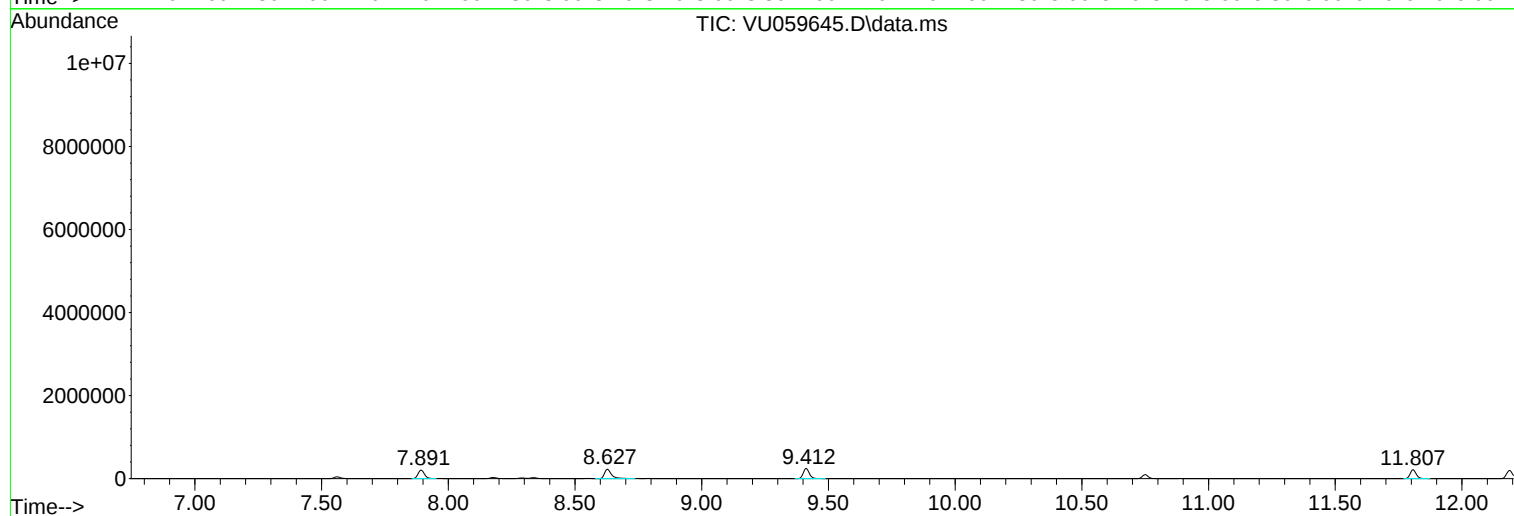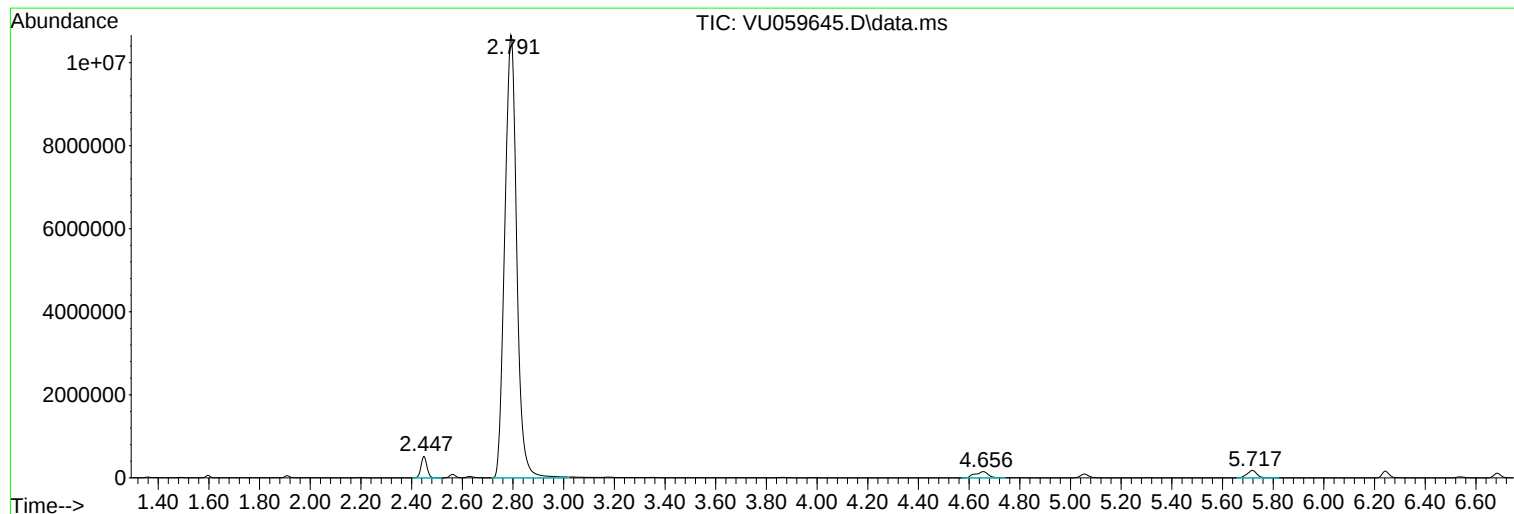

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059645.D
Acq On : 29 Jun 2024 01:00
Operator : MD/SY
Sample : P3059-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN2










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.447	8.95 ug/L	844212	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	64
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	42
4	Propane, 2-nitro-			89	C3H7NO2	000079-46-9	9
5	Acetyl chloride			78	C2H3ClO	000075-36-5	9

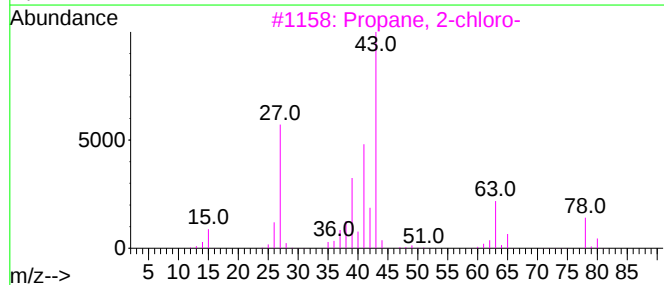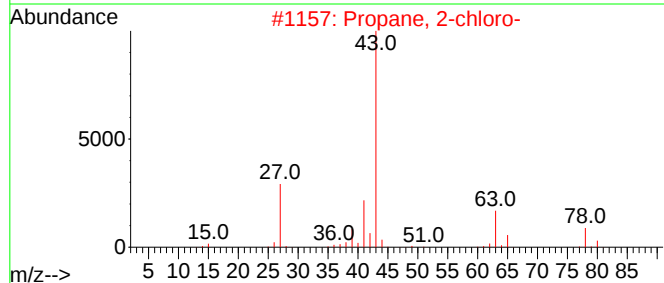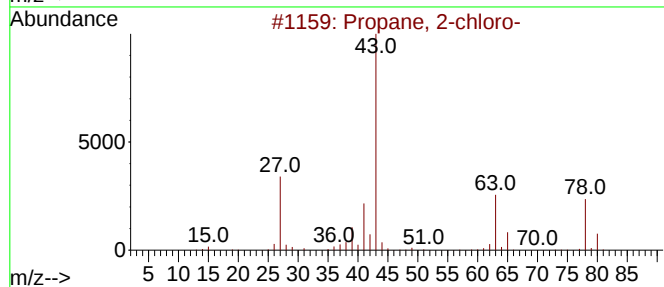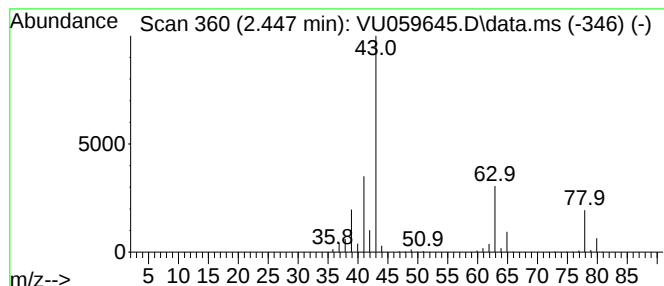

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059645.D
Acq On : 29 Jun 2024 01:00
Operator : MD/SY
Sample : P3059-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN2










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.791	370.57 ug/L	34956200	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

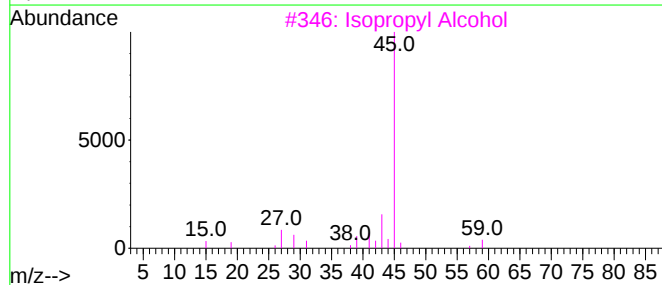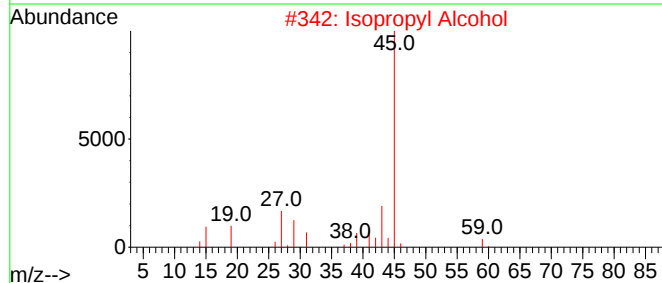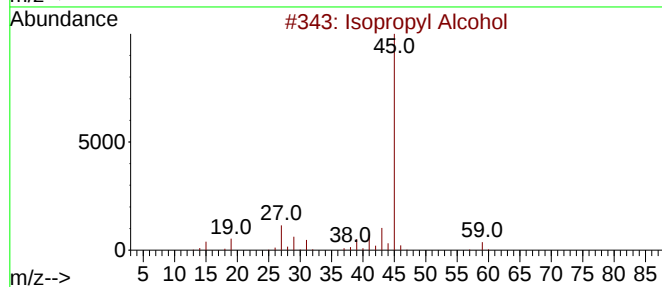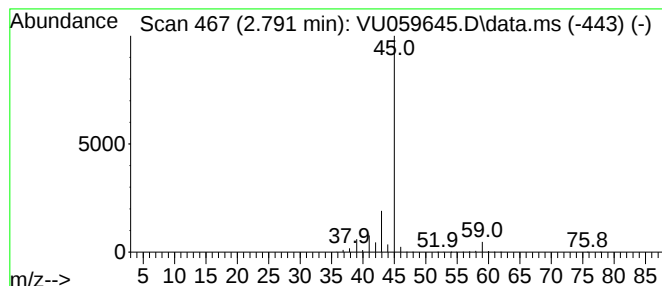

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059645.D
Acq On : 29 Jun 2024 01:00
Operator : MD/SY
Sample : P3059-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.447	8.9	ug/L	844212	1	6.242	471660	5.0
Isopropyl Alcohol	2.791	370.6	ug/L	34956200	1	6.242	471660	5.0