

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059665.D
 Acq On : 29 Jun 2024 08:57
 Operator : MD/SY
 Sample : P3068-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCL26

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU059665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.383	22	29	38	rBV2	14016	16211	3.58%	0.372%
2	1.596	87	95	110	rVB	41350	48201	10.65%	1.107%
3	1.907	184	192	205	rBV	46309	61575	13.61%	1.415%
4	2.075	236	244	253	rBV	27100	37741	8.34%	0.867%
5	2.133	253	262	278	rVB	82213	120747	26.68%	2.774%
6	2.560	383	395	413	rVB	77676	129846	28.69%	2.983%
7	3.036	535	543	556	rVB4	3260	6253	1.38%	0.144%
8	4.621	1025	1036	1068	rBV	61911	176023	38.90%	4.044%
9	4.817	1086	1097	1118	rVB3	5300	13979	3.09%	0.321%
10	5.055	1154	1171	1195	rBV	90543	209493	46.29%	4.813%
11	5.718	1358	1377	1408	rBV2	171839	452519	100.00%	10.397%
12	6.242	1527	1540	1569	rBV	171935	330502	73.04%	7.593%
13	6.538	1616	1632	1651	rBV	177731	337723	74.63%	7.759%
14	6.682	1665	1677	1702	rVB	109308	217903	48.15%	5.006%
15	7.560	1940	1950	1968	rBV	40087	73147	16.16%	1.681%
16	7.891	2041	2053	2079	rBV	198250	347822	76.86%	7.991%
17	8.177	2132	2142	2159	rBV4	23835	42058	9.29%	0.966%
18	8.627	2271	2282	2320	rBV	216216	438057	96.80%	10.065%
19	9.412	2514	2526	2553	rBV	256532	437509	96.68%	10.052%
20	10.750	2931	2942	2956	rBV	93421	153438	33.91%	3.525%
21	10.888	2974	2985	2996	rBV2	4595	6871	1.52%	0.158%
22	11.807	3259	3271	3297	rBV	228252	372677	82.36%	8.562%
23	12.187	3378	3389	3412	rBV	190054	322171	71.20%	7.402%




Sum of corrected areas: 4352466

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059665.D
Acq On : 29 Jun 2024 08:57
Operator : MD/SY
Sample : P3068-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCL26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

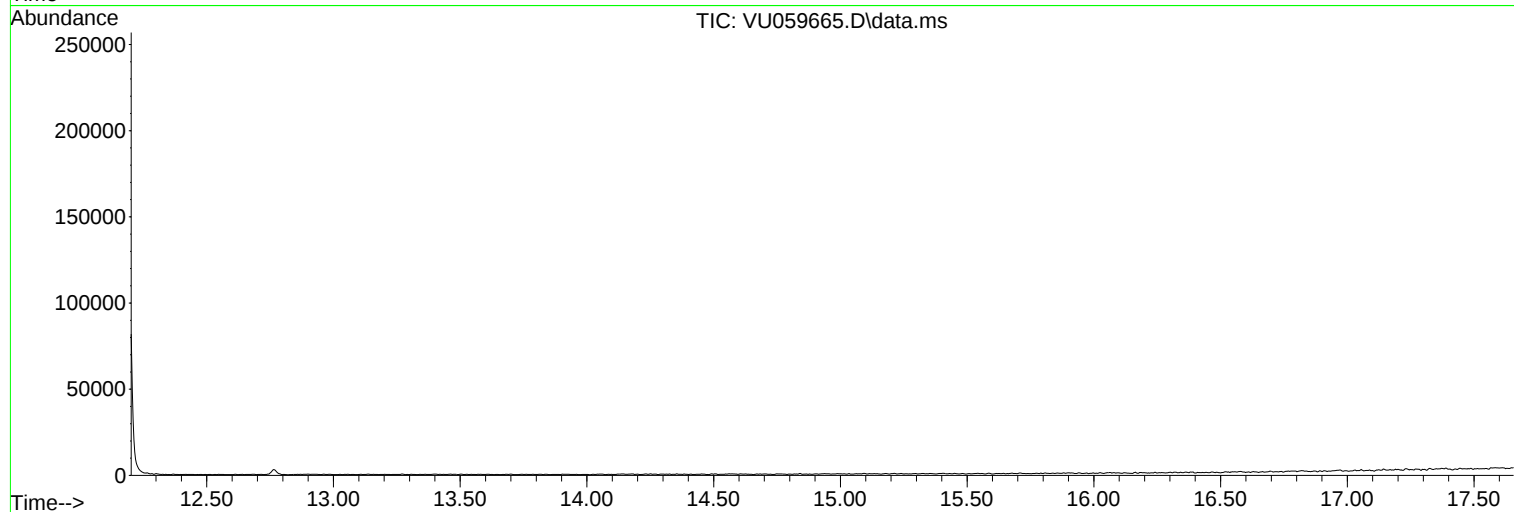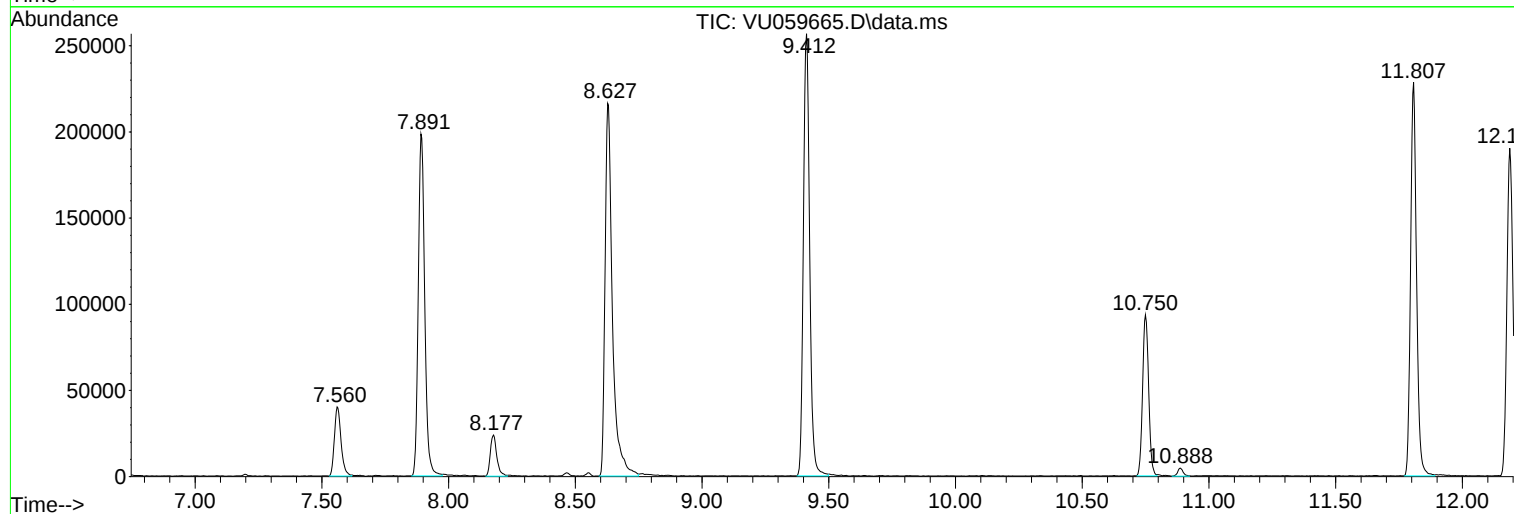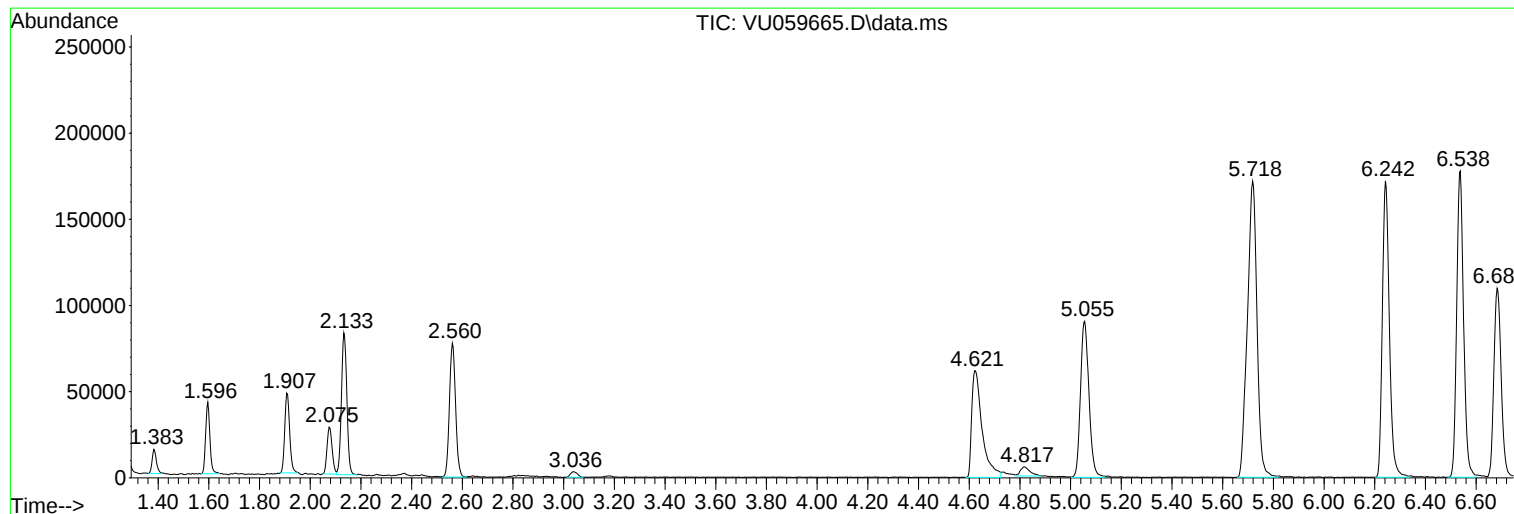

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059665.D
Acq On : 29 Jun 2024 08:57
Operator : MD/SY
Sample : P3068-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCL26










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.075	0.57 ug/L	37741	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	90
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	90
4			1-Hexyne	82	C6H10	000693-02-7	7
5			1-Butyne, 3,3-dimethyl-	82	C6H10	000917-92-0	7

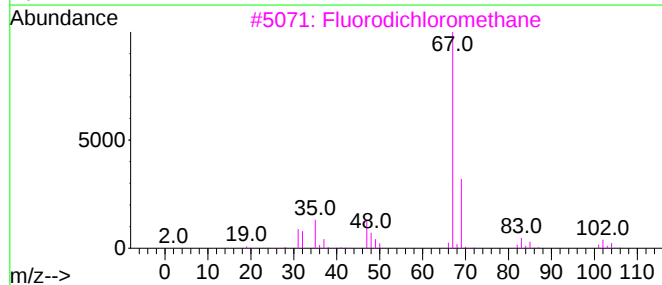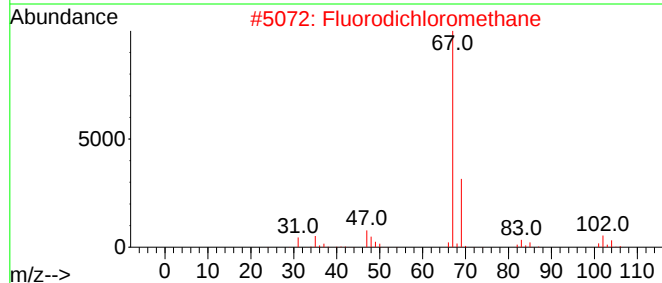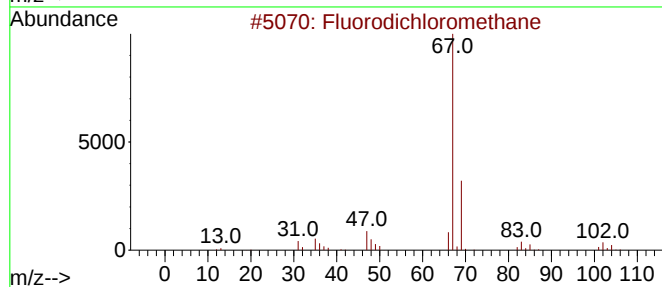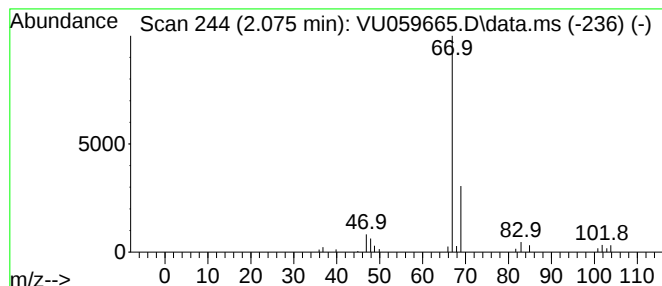

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059665.D
Acq On : 29 Jun 2024 08:57
Operator : MD/SY
Sample : P3068-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCL26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	2.075	0.6	ug/L	37741	1	6.242	330502	5.0