


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059614.D
Acq On : 28 Jun 2024 12:13
Operator : MD/SY
Sample : BFB167
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB167

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jun 29 01:51:23 2024

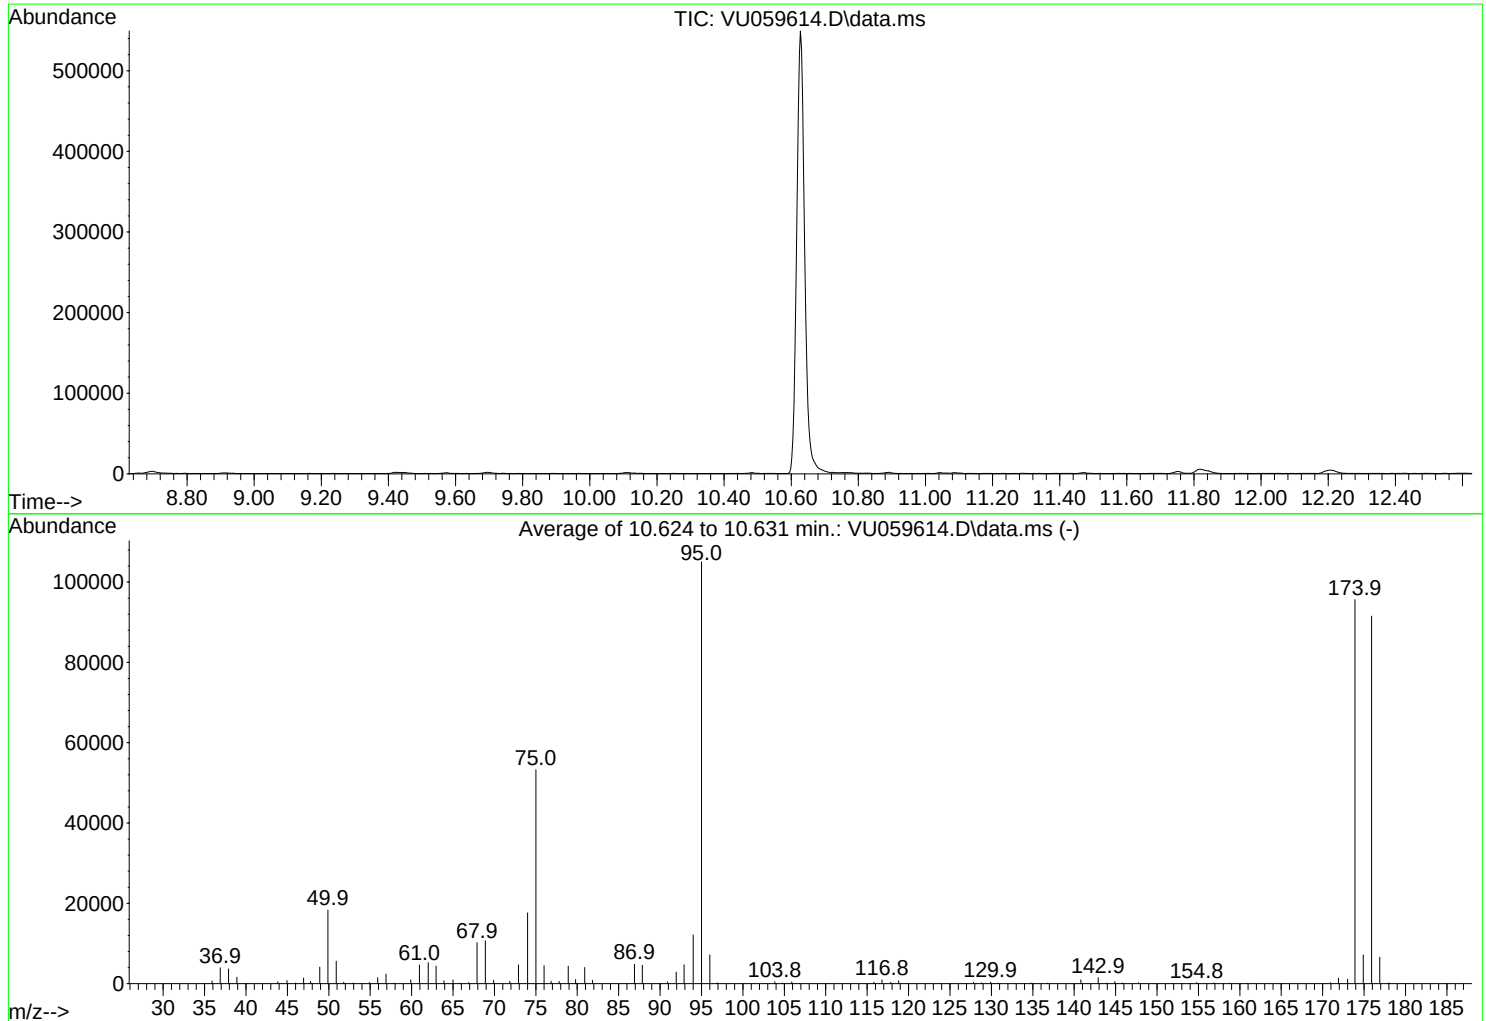

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	18301	PASS
75	95	30	80	50.7	53277	PASS
95	95	100	100	100.0	105040	PASS
96	95	5	9	6.8	7186	PASS
173	174	0.00	2	1.2	1115	PASS
174	95	50	120	91.0	95635	PASS
175	174	5	9	7.5	7171	PASS
176	174	95	101	95.7	91541	PASS
177	176	5	9	7.2	6576	PASS

m/z	Abundance
39.90	243.0
43.80	256.0

Instrument :
MSVOA_U
ClientSampleId :
BFB167

m/z	Abundance
35.90	703.0
36.90	3961.0
37.90	3642.0
38.90	1544.0
39.70	293.0
43.90	771.0
44.90	816.0
46.00	154.0
47.00	1393.0
47.80	582.0
48.90	3852.0
49.90	17928.0
50.90	5574.0
51.80	298.0
53.00	156.0
54.90	324.0
55.90	1463.0
56.90	2421.0
57.90	109.0
59.90	882.0
61.00	4779.0
62.00	5050.0
62.90	4185.0
63.90	724.0
65.00	907.0
65.90	102.0
66.90	308.0
67.90	10296.0
68.90	10535.0
69.90	906.0
71.80	608.0
72.90	4466.0
74.00	17552.0
75.00	52432.0
76.00	4599.0
76.90	572.0
77.80	538.0
78.90	4270.0
79.80	1007.0
80.90	4088.0
81.80	858.0
86.90	4826.0
87.80	4302.0
90.90	413.0
92.00	2861.0
92.90	4677.0
94.00	11667.0
95.00	103672.0
96.00	7174.0
96.90	215.0
103.90	420.0
104.80	191.0
105.90	436.0
106.80	120.0
115.80	408.0
116.80	897.0
117.90	317.0
118.80	735.0
127.80	370.0
128.80	216.0
129.90	448.0
130.80	201.0
134.80	215.0
136.80	109.0
140.80	890.0
142.90	1437.0
143.90	104.0
144.90	503.0
145.80	176.0
147.80	221.0
154.80	271.0
156.80	169.0
158.80	132.0
160.80	151.0
170.90	192.0
171.90	1395.0
173.00	1022.0
173.90	92120.0
174.90	7080.0
175.90	87904.0
176.90	6324.0
178.00	168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB167

m/z	Abundance
35.90	718.0
36.90	4101.0
37.90	3835.0
38.90	1589.0
39.70	278.0
43.90	761.0
44.90	811.0
46.00	167.0
47.00	1483.0
47.80	552.0
48.90	4297.0
49.90	18888.0
50.90	5765.0
51.80	363.0
52.90	140.0
53.90	113.0
54.90	346.0
55.90	1554.0
56.90	2454.0
57.90	104.0
59.90	928.0
60.90	4759.0
62.00	5381.0
63.00	4543.0
63.90	753.0
65.00	923.0
65.80	128.0
66.90	294.0
67.90	10499.0
68.90	11046.0
69.90	860.0
71.80	582.0
72.90	4780.0
74.00	18160.0
75.00	55192.0
76.00	4556.0
76.90	623.0
77.80	589.0
78.90	4556.0
79.80	1040.0
80.90	4181.0
81.80	871.0
86.90	4981.0
87.90	4748.0
90.90	446.0
91.90	2969.0
92.90	4868.0
94.00	12410.0
95.00	108024.0
96.00	7504.0
96.90	208.0
103.90	479.0
104.80	183.0
105.90	433.0
115.80	362.0
116.80	966.0
117.90	302.0
118.80	757.0
127.80	365.0
128.80	226.0
129.90	421.0
130.80	160.0
134.80	158.0
136.80	127.0
140.80	960.0
142.90	1503.0
143.80	125.0
144.90	526.0
145.80	221.0
147.70	252.0
153.00	123.0
154.80	295.0
156.90	219.0
158.70	121.0
160.80	117.0
171.00	233.0
171.90	1433.0
173.00	1134.0
173.90	98568.0
174.90	7291.0
175.90	94456.0
176.90	6802.0
178.00	211.0

Instrument :
MSVOA_U
ClientSampleId :
BFB167

m/z	Abundance
35.90	662.0
36.90	3802.0
37.90	3574.0
38.90	1606.0
39.80	271.0
43.90	688.0
45.00	717.0
46.00	150.0
46.90	1352.0
47.80	513.0
48.90	4125.0
49.90	18088.0
50.90	5411.0
51.80	370.0
52.90	157.0
53.90	103.0
54.90	298.0
55.90	1406.0
56.90	2305.0
57.80	100.0
59.90	983.0
60.90	4511.0
62.00	5197.0
63.00	4414.0
63.90	713.0
65.00	910.0
65.80	139.0
66.90	243.0
67.90	9849.0
68.90	10425.0
69.90	807.0
71.90	581.0
72.90	4730.0
74.00	17096.0
75.00	52208.0
76.00	4215.0
76.80	586.0
77.80	569.0
78.90	4209.0
79.80	1081.0
80.90	3822.0
81.90	780.0
85.90	198.0
86.90	4632.0
87.90	4654.0
90.90	443.0
91.90	2745.0
92.90	4567.0
94.00	12242.0
95.00	103424.0
96.00	6879.0
96.90	167.0
103.80	531.0
104.80	149.0
105.90	433.0
112.00	115.0
115.80	322.0
116.80	883.0
117.80	328.0
118.80	723.0
123.80	104.0
127.90	362.0
128.80	205.0
129.90	389.0
134.90	109.0
136.80	142.0
140.80	988.0
142.90	1434.0
143.80	124.0
144.90	507.0
145.80	237.0
147.70	253.0
152.90	129.0
154.80	279.0
156.90	231.0
158.70	112.0
170.90	284.0
171.90	1298.0
173.00	1190.0
173.90	96216.0
174.90	7141.0
175.90	92264.0
176.90	6602.0
178.00	226.0

Instrument :
MSVOA_U
ClientSampleId :
BFB167