

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU063018\
 Data File : VU025114.D
 Acq On : 01 Jul 2018 02:54
 Operator : MD/SY
 Sample : J3804-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 207TH-STREET-TRIP-BLANK-1-6-28

Manual Integrations
 APPROVED

Quant Time: Jul 02 09:22:02 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 13 13:55:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.99	168	218546	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	323491	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	300458	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.49	152	154872	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	5.31	65	163404	45.80	ug/l	0.00	apatel
Spiked Amount 50.000			Recovery =	91.60%			
35) Dibromofluoromethane	4.89	113	128729	47.95	ug/l	0.00	
Spiked Amount 50.000			Recovery =	95.90%			
50) Toluene-d8	7.57	98	467316	47.72	ug/l	0.00	7/2/2018 4:16:34 PM
Spiked Amount 50.000			Recovery =	95.44%			
62) 4-Bromofluorobenzene	10.31	95	172890	44.47	ug/l	0.00	
Spiked Amount 50.000			Recovery =	88.94%			

Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU063018\
Data File : VU025114.D
Acq On : 01 Jul 2018 02:54
Operator : MD/SY
Sample : J3804-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
207TH-STREET-TRIP-BLANK-1-6-28

Manual Integrations
APPROVED

Quant Time: Jul 02 09:22:02 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 13 13:55:26 2018
Response via : Initial Calibration

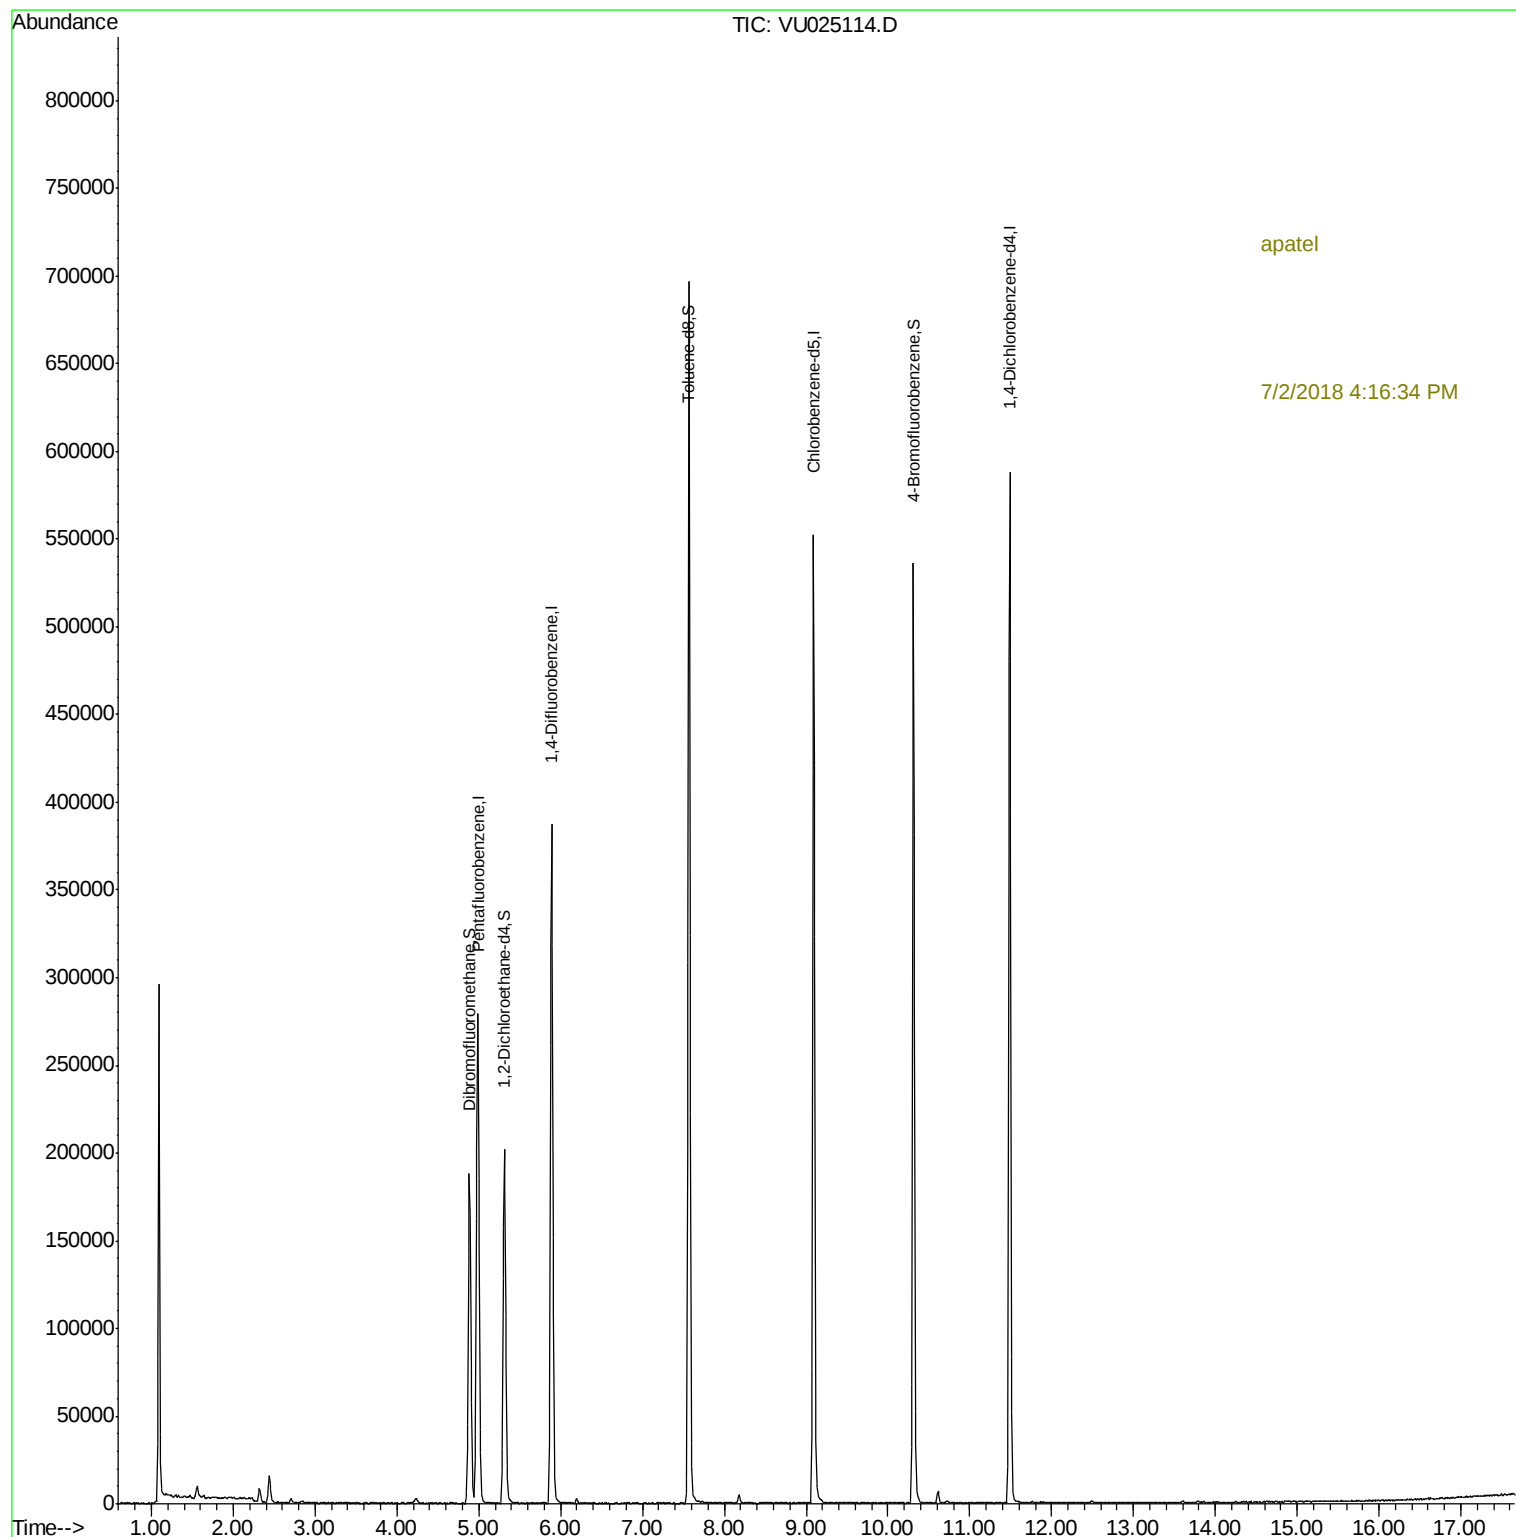

apatel

7/2/2018 4:16:34 PM