

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU063018\
 Data File : VU025130.D
 Acq On : 01 Jul 2018 09:22
 Operator : MD/SY
 Sample : J3789-07DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MW-7DL

Quant Time: Jul 02 08:38:16 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 13 13:55:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.99	168	209308	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	314930	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	289554	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.49	152	148995	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	5.31	65	158994	46.53	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.06%	
35) Dibromofluoromethane	4.89	113	122957	47.04	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.08%	
50) Toluene-d8	7.57	98	447988	46.99	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.98%	
62) 4-Bromofluorobenzene	10.31	95	166121	43.89	ug/l	0.00
Spiked Amount 50.000			Recovery	=	87.78%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	2.82	59	73497	88.44	ug/l	100
16) Acetone	2.33	43	1133	0.62	ug/l	# 88
19) Methyl tert-butyl Ether	3.00	73	298630	33.33	ug/l	96
22) Diisopropyl ether	3.57	45	4650	0.53	ug/l	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU063018\
Data File : VU025130.D
Acq On : 01 Jul 2018 09:22
Operator : MD/SY
Sample : J3789-07DL 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW-7DL

Quant Time: Jul 02 08:38:16 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 13 13:55:26 2018
Response via : Initial Calibration

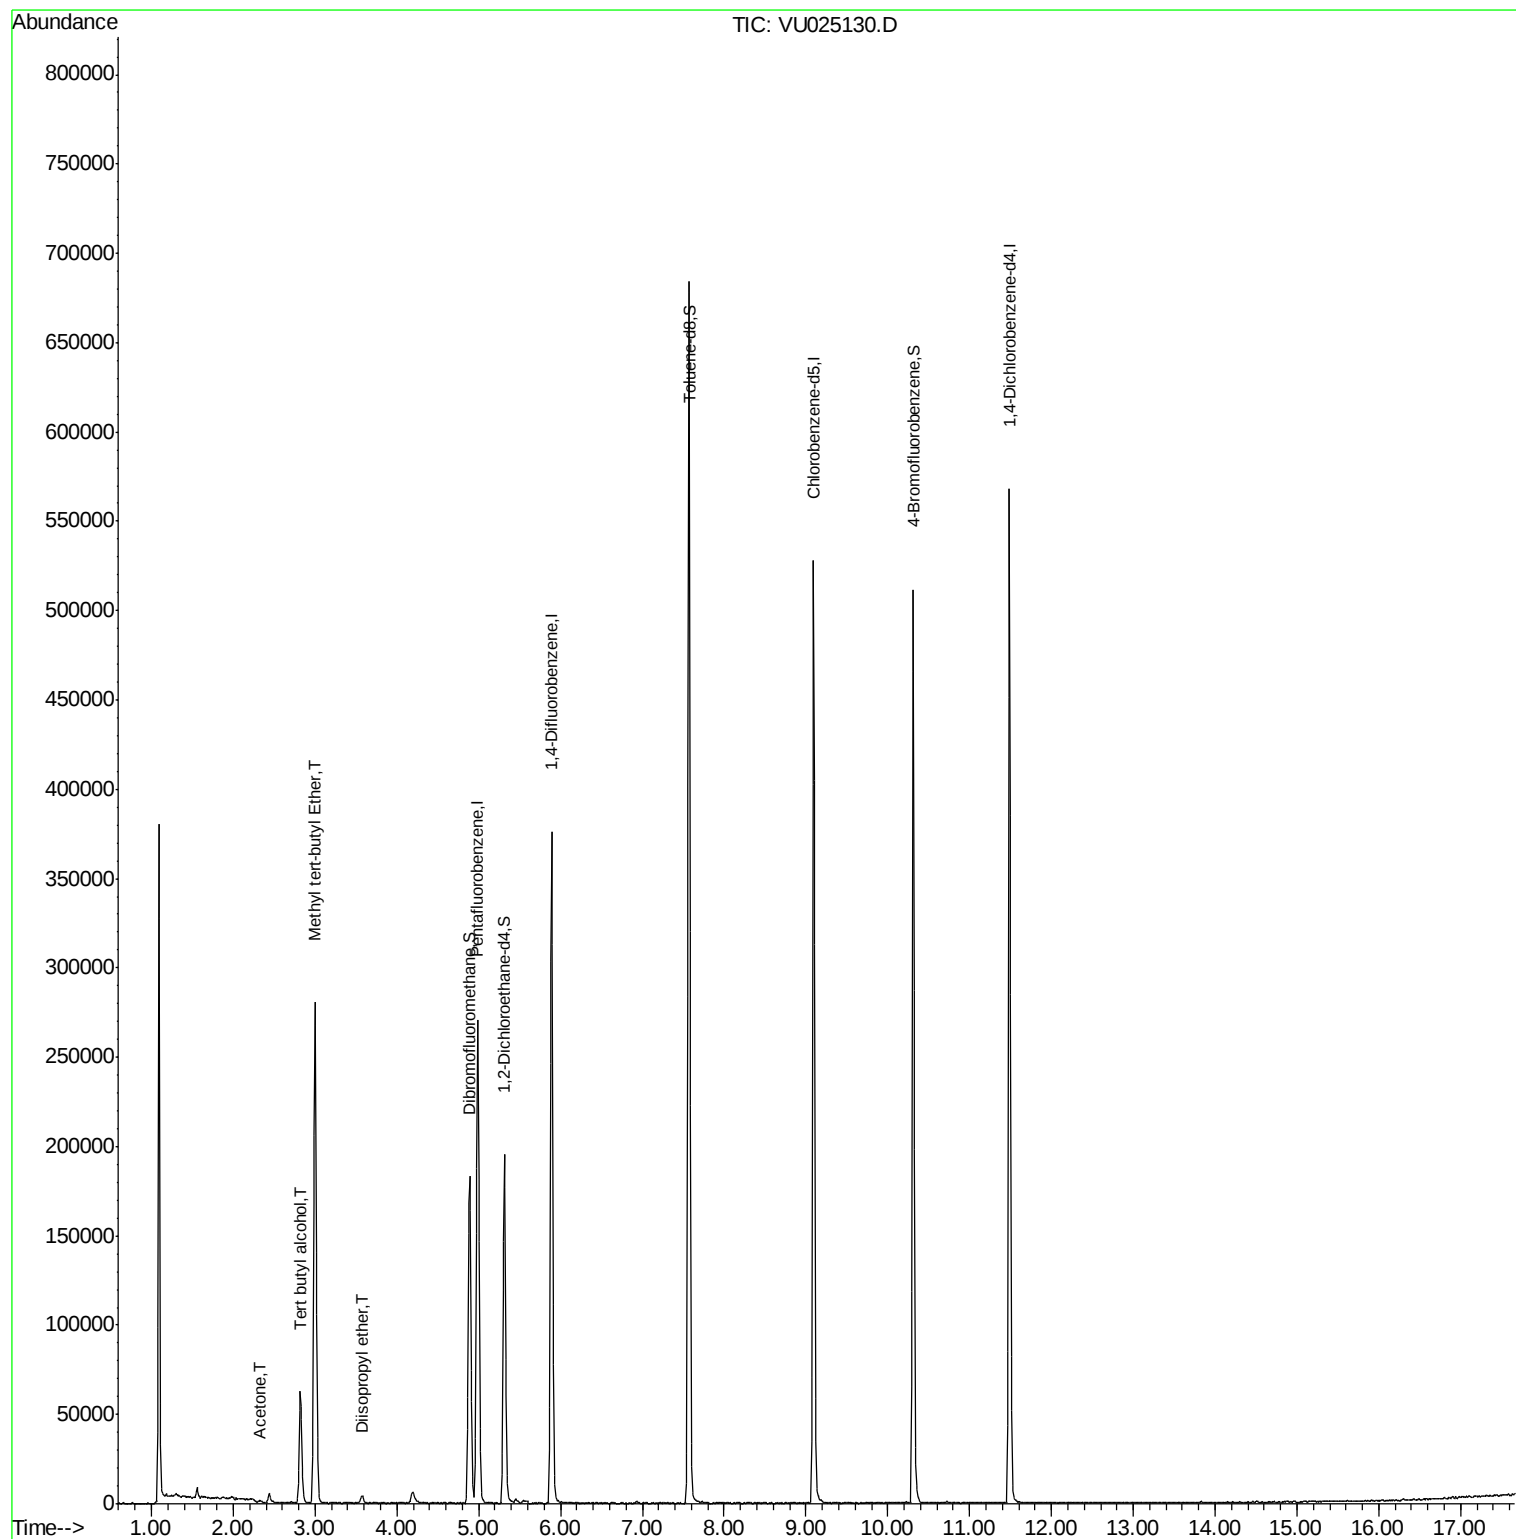



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 4.99 min Scan# 1368

Delta R.T. -0.00 min

Lab File: VU025130.D

Acq: 01 Jul 2018 09:22

Instrument :

MSVOA_U

ClientSampleId :


MW-7DL

Tot Ion:168 Resp: 209308

Ion Ratio Lower Upper




168 100

99 55.5 43.2 64.8

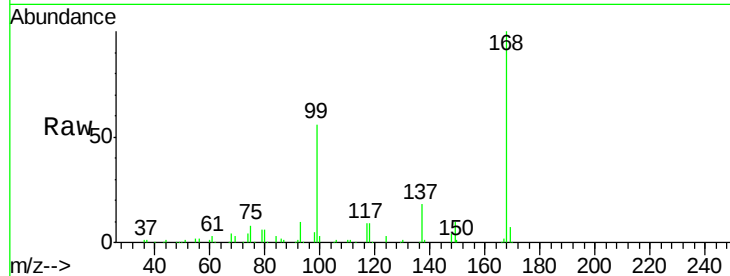

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VU0

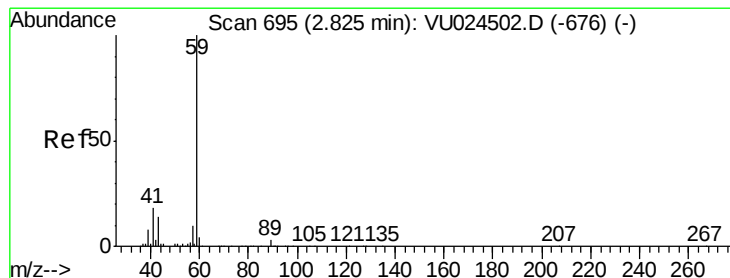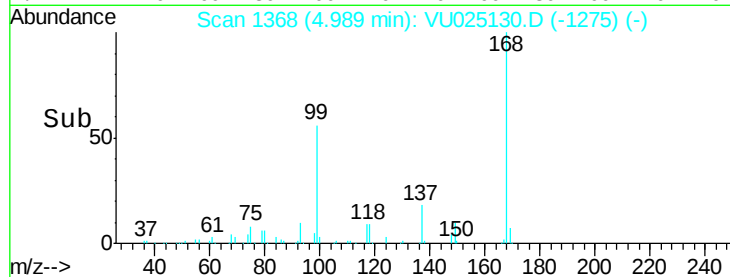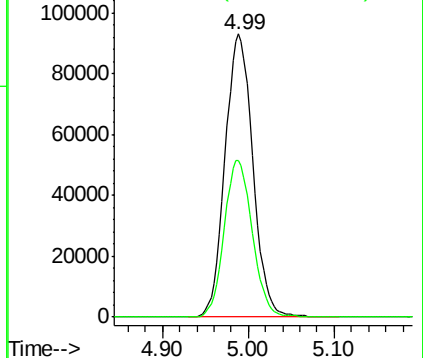

#11

Tert butyl alcohol

Concen: 88.44 ug/l

RT: 2.82 min Scan# 693

Delta R.T. -0.01 min

Lab File: VU025130.D


Acq: 01 Jul 2018 09:22

Tgt Ion: 59 Resp: 73497

Ion Ratio Lower Upper



59 100


57 10.6 8.5 12.7

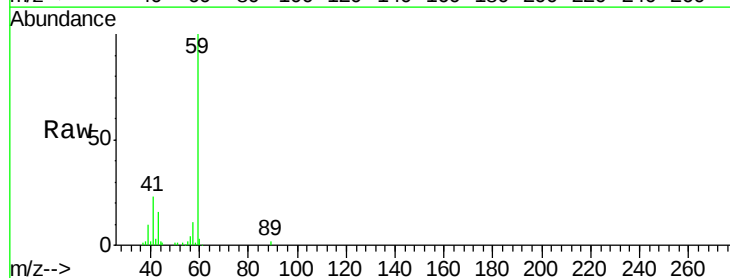

Abundance Ion 59.00 (58.70 to 59.70): VU0

Ion 57.00 (56.70 to 57.70): VU0

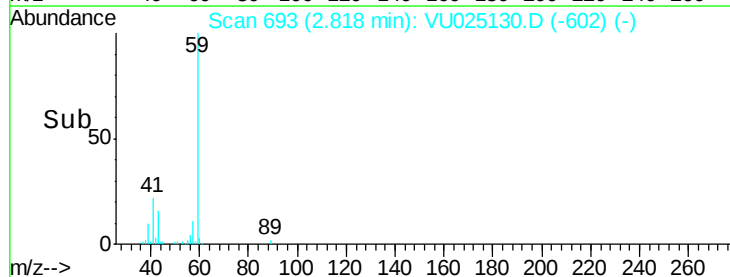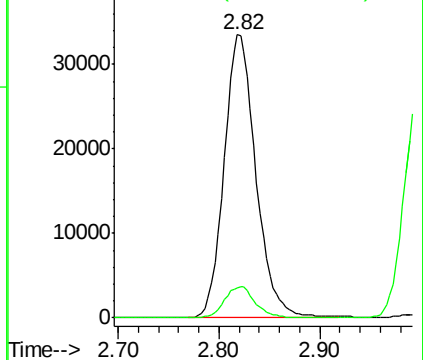

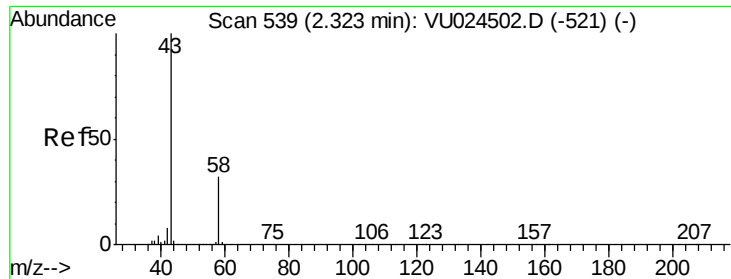

#16

Acetone

Concen: 0.62 ug/l

RT: 2.33 min Scan# 540

Delta R.T. 0.00 min

Lab File: VU025130.D

Acq: 01 Jul 2018 09:22

Instrument :

MSVOA_U

ClientSampleId :


MW-7DL

Tot Ion: 43 Resp: 1133

Ion Ratio Lower Upper




43 100

58 24.2 24.4 36.6#



Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

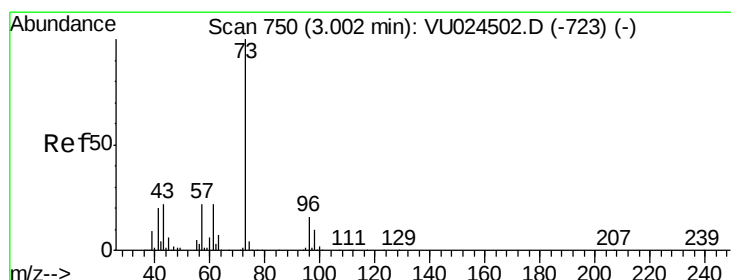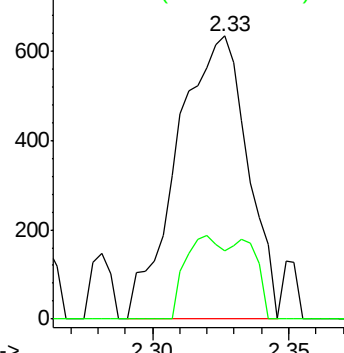

#19

Methyl tert-butyl Ether

Concen: 33.33 ug/l

RT: 3.00 min Scan# 750

Delta R.T. 0.00 min

Lab File: VU025130.D


Acq: 01 Jul 2018 09:22

Tgt Ion: 73 Resp: 298630

Ion Ratio Lower Upper



73 100


57 21.4 18.8 28.2



Abundance Ion 73.00 (72.70 to 73.70): VU0

Ion 57.00 (56.70 to 57.70): VU0

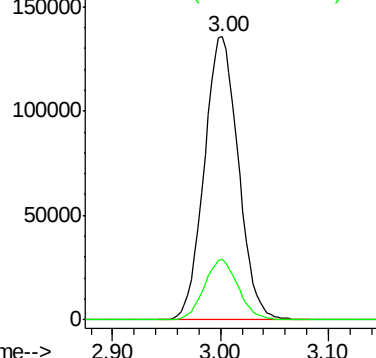



#22

Diisopropyl ether

Concen: 0.53 ug/l

RT: 3.57 min Scan# 928

Delta R.T. -0.00 min

Lab File: VU025130.D

Acq: 01 Jul 2018 09:22

Instrument :

MSVOA_U

ClientSampleId :

MW-7DL

Tot Ion: 45 Resp: 4650


Ion Ratio Lower Upper

45 100

43 53.0 45.8 68.6

87 25.3 20.6 31.0

59 10.7 9.4 14.0



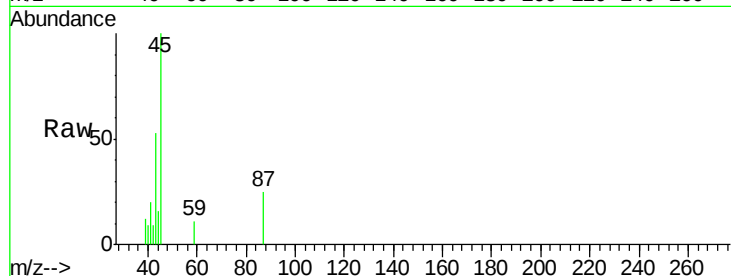


Abundance Ion 45.00 (44.70 to 45.70): VU0

Ion 43.00 (42.70 to 43.70): VU0

Ion 87.00 (86.70 to 87.70): VU0

Ion 59.00 (58.70 to 59.70): VU0

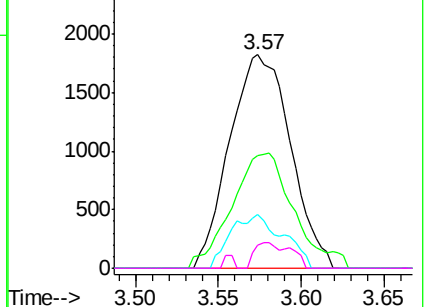

#33

1,2-Dichloroethane-d4

Concen: 46.53 ug/l

RT: 5.31 min Scan# 1469

Delta R.T. 0.00 min

Lab File: VU025130.D


Acq: 01 Jul 2018 09:22

Tgt Ion: 65 Resp: 158994

Ion Ratio Lower Upper



65 100


67 50.4 0.0 107.0



Abundance Ion 64.90 (64.60 to 65.60): VU0

Ion 66.90 (66.60 to 67.60): VU0

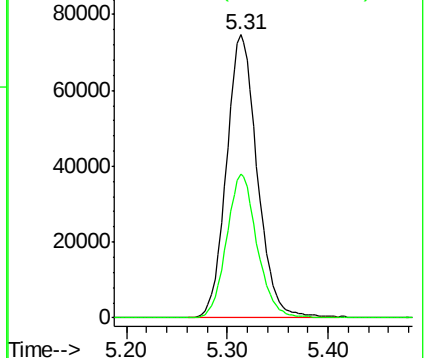

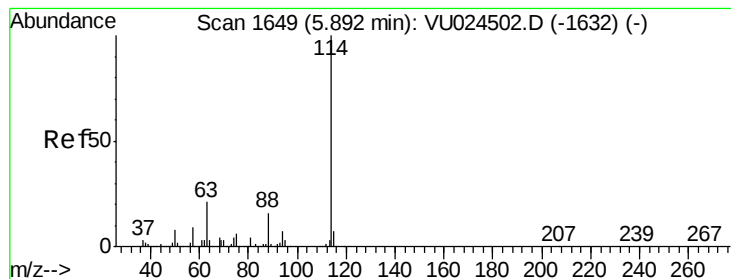

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 5.89 min Scan# 1649

Delta R.T. 0.00 min

Lab File: VU025130.D

Acq: 01 Jul 2018 09:22

Instrument :

MSVOA_U

ClientSampleId :

MW-7DL


Tot Ion:114 Resp: 314930

Ion Ratio Lower Upper

114 100

63 20.2 0.0 45.4




88 15.8 0.0 31.0



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VU0

Ion 87.90 (87.60 to 88.60): VU0

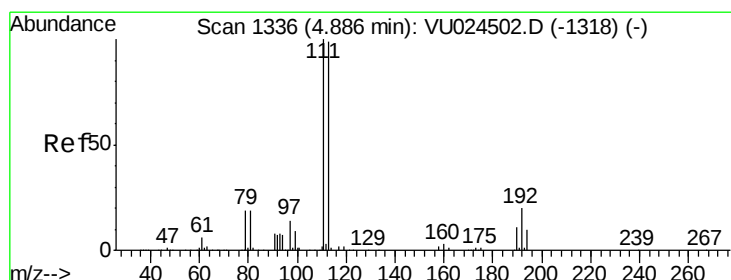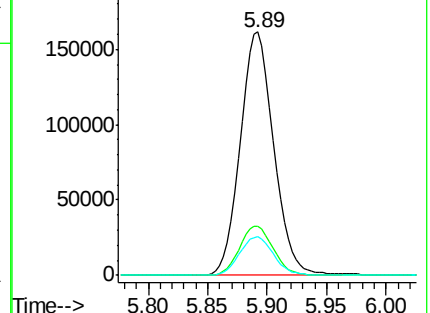

#35

Dibromofluoromethane

Concen: 47.04 ug/l

RT: 4.89 min Scan# 1337

Delta R.T. 0.00 min

Lab File: VU025130.D

Acq: 01 Jul 2018 09:22


Tgt Ion:113 Resp: 122957

Ion Ratio Lower Upper

113 100

111 102.5 82.2 123.4



192 21.1 16.2 24.4



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



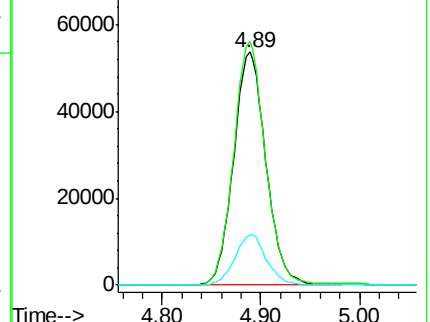





#50
Toluene-d8
Concen: 46.99 ug/l
RT: 7.57 min Scan# 2171
Delta R.T. 0.00 min
Lab File: VU025130.D
Acq: 01 Jul 2018 09:22




Instrument :
MSVOA_U
ClientSampleId :
MW-7DL


Tot Ion: 98 Resp: 447988
Ion Ratio Lower Upper
98 100
100 64.4 51.1 76.7

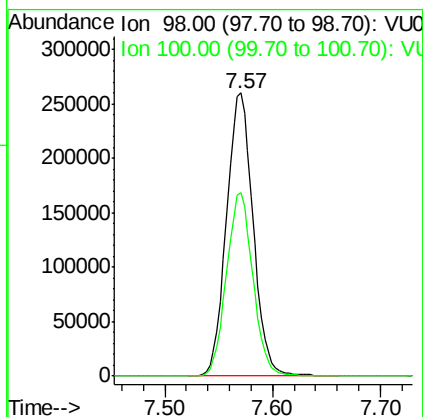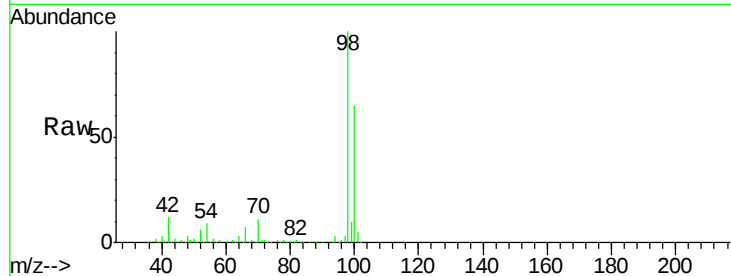

#62
4-Bromofluorobenzene
Concen: 43.89 ug/l
RT: 10.31 min Scan# 3023
Delta R.T. 0.00 min
Lab File: VU025130.D
Acq: 01 Jul 2018 09:22

Tgt Ion: 95 Resp: 166121
Ion Ratio Lower Upper
95 100
174 84.4 0.0 165.8
176 83.2 0.0 159.4

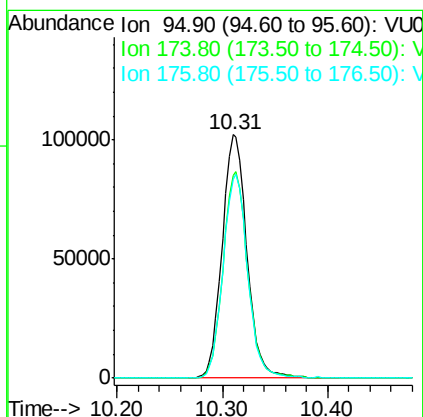


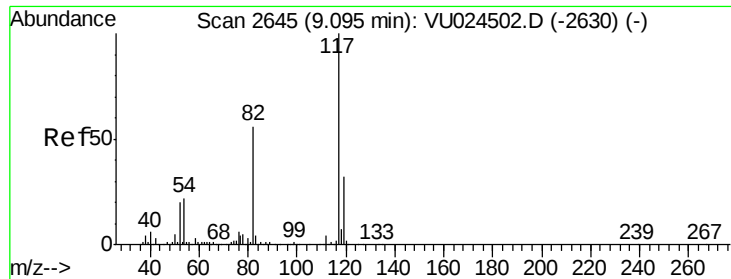




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 9.09 min Scan# 2645
Delta R.T. 0.00 min
Lab File: VU025130.D
Acq: 01 Jul 2018 09:22

Instrument :
MSVOA_U
ClientSampleId :
MW-7DL

Tot Ion	Ratio	Lower	Upper
117	100		
82	56.8	44.3	66.5
119	33.3	25.4	38.2

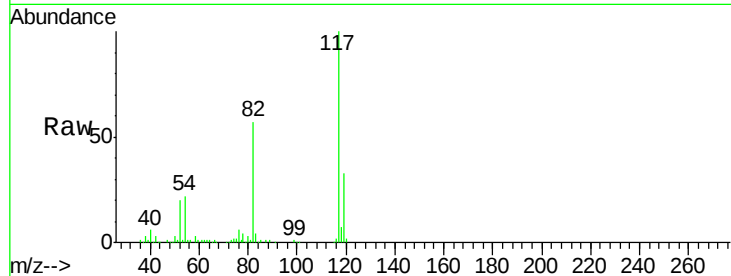


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

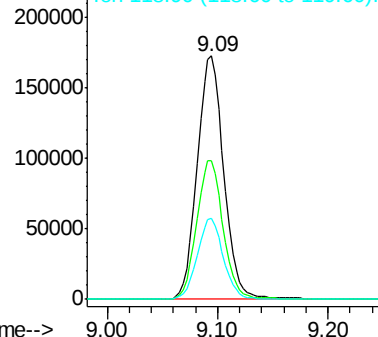

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 11.49 min Scan# 3389
Delta R.T. 0.00 min
Lab File: VU025130.D
Acq: 01 Jul 2018 09:22

Tgt Ion	Ratio	Lower	Upper
152	100		
115	58.4	43.0	129.0
150	155.6	0.0	354.0



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

