


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU063020\
 Data File : VU039233.D
 Acq On : 30 Jun 2020 10:48
 Operator : SY/MD
 Sample : BFB24
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB24

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR063020WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jul 01 21:08:14 2020

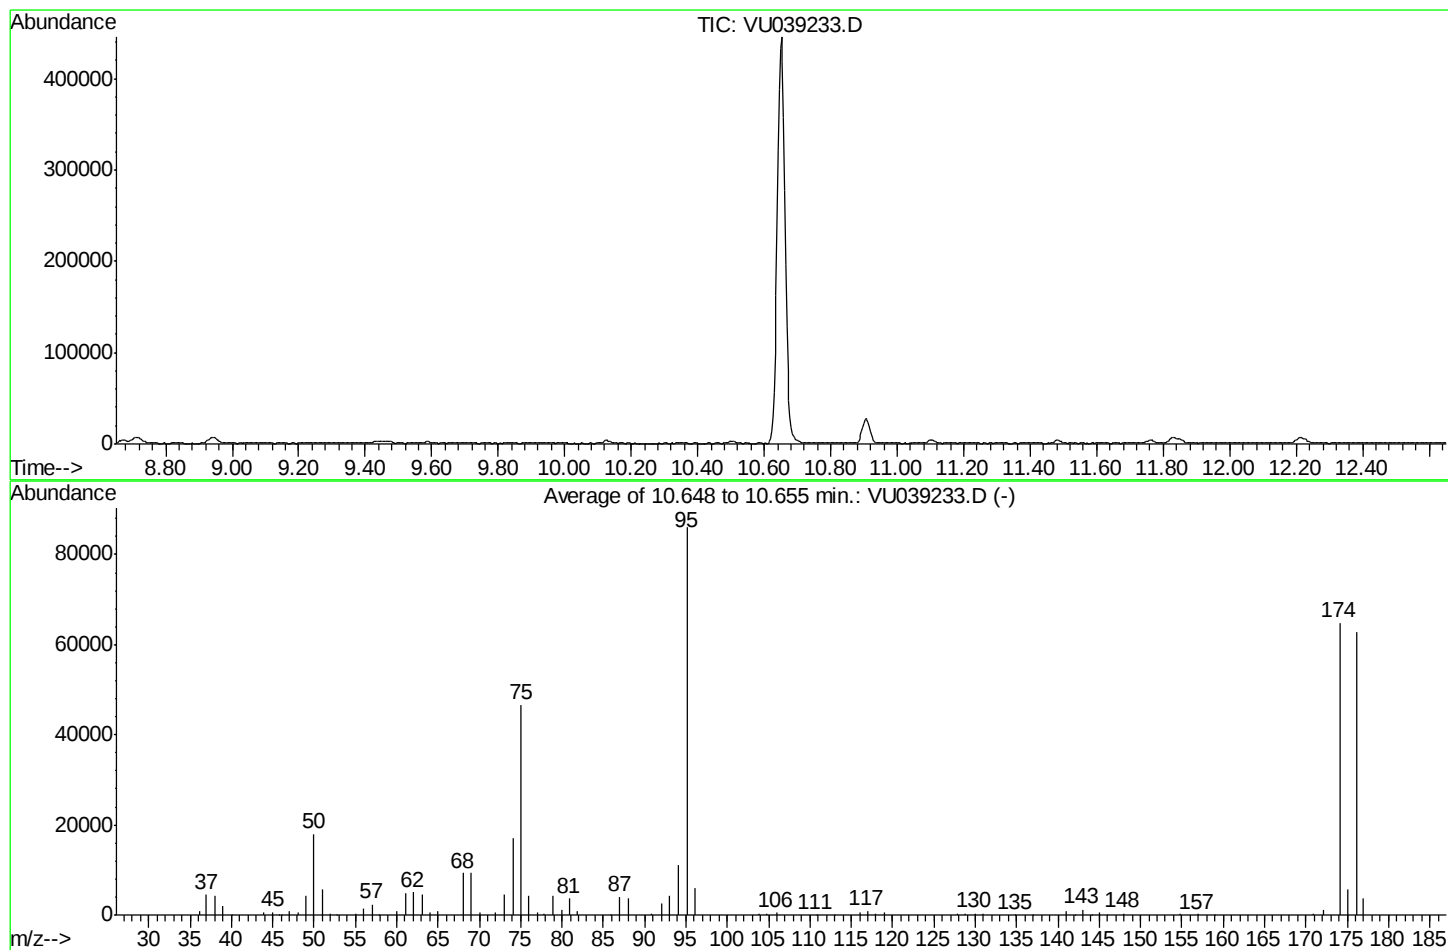

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	18050	PASS
75	95	30	80	54.3	46749	PASS
95	95	100	100	100.0	86058	PASS
96	95	5	9	6.8	5868	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.4	64880	PASS
175	174	5	9	8.6	5585	PASS
176	174	95	101	96.7	62730	PASS
177	176	5	9	5.8	3654	PASS

Scan 2881 (10.603 min): VU039233.D
BFB24

m/z	Abundance
39.40	104.0
40.00	223.0
44.00	490.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.10	818.0
37.00	4396.0
38.00	4418.0
39.00	1977.0
40.00	343.0
43.90	1153.0
45.00	685.0
46.10	225.0
47.00	835.0
48.10	514.0
49.00	4246.0
50.00	18728.0
51.00	5835.0
52.00	275.0
52.80	109.0
55.00	345.0
56.00	1398.0
57.00	2428.0
59.90	992.0
61.00	4998.0
62.00	5066.0
63.10	4738.0
64.10	543.0
65.00	904.0
68.00	9333.0
69.00	9281.0
70.10	484.0
72.00	474.0
73.10	4594.0
74.00	17352.0
75.00	46936.0
76.00	4154.0
77.00	619.0
77.90	459.0
78.90	4286.0
80.00	1225.0
80.90	3649.0
81.90	730.0
85.80	147.0
87.00	3926.0
88.00	3543.0
90.90	535.0
92.00	2683.0
93.00	4351.0
94.10	10864.0
95.10	86832.0
96.10	5795.0
103.90	451.0
104.80	176.0
106.00	523.0
112.80	134.0
116.00	443.0
117.00	967.0
117.90	366.0
119.00	630.0
127.80	256.0
128.80	210.0
130.00	308.0
131.00	133.0
134.80	120.0
137.00	111.0
141.00	885.0
142.10	165.0
143.10	1059.0
145.00	680.0
145.90	105.0
147.90	331.0
154.90	216.0
156.90	216.0
158.90	107.0
170.90	118.0
172.10	1049.0
174.10	64248.0
175.10	5774.0
176.10	61688.0
177.00	3778.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.10	863.0
37.00	4573.0
38.00	4395.0
39.00	2169.0
40.00	332.0
43.90	1048.0
45.00	701.0
46.00	189.0
46.90	915.0
48.10	616.0
49.00	4494.0
50.00	18592.0
51.00	5976.0
52.00	265.0
55.10	382.0
56.00	1522.0
57.00	2409.0
57.90	145.0
60.00	921.0
61.00	4923.0
62.00	5232.0
63.00	4551.0
64.00	500.0
65.00	945.0
68.00	9634.0
69.00	9658.0
70.00	602.0
72.00	487.0
73.00	4757.0
74.10	17632.0
75.10	48280.0
76.00	4373.0
77.00	701.0
77.80	477.0
78.90	4285.0
80.00	1267.0
80.90	3765.0
81.90	749.0
85.80	136.0
87.00	4116.0
88.00	3878.0
90.90	444.0
92.00	2750.0
93.00	4420.0
94.10	11455.0
95.10	88032.0
96.10	6137.0
103.90	427.0
104.70	171.0
106.00	570.0
112.90	130.0
116.00	449.0
117.00	895.0
117.80	356.0
119.00	673.0
127.90	316.0
128.80	201.0
130.00	338.0
131.00	198.0
134.90	150.0
137.00	140.0
141.00	904.0
143.00	1160.0
144.10	101.0
145.00	600.0
145.90	111.0
147.90	330.0
154.90	200.0
156.90	242.0
158.90	101.0
171.00	143.0
172.10	1211.0
174.10	66632.0
175.10	5749.0
176.10	64776.0
177.00	3645.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.10	755.0
37.00	4463.0
38.00	4091.0
39.00	1994.0
40.00	291.0
43.90	966.0
45.00	623.0
45.80	165.0
46.90	952.0
48.20	611.0
49.00	4070.0
50.00	16832.0
51.00	5559.0
52.00	205.0
55.10	322.0
56.00	1511.0
57.00	2307.0
57.90	138.0
60.10	744.0
61.10	4440.0
62.00	4921.0
63.00	4126.0
64.00	498.0
65.00	926.0
68.00	9117.0
69.10	9026.0
70.00	719.0
72.00	485.0
73.00	4295.0
74.10	15936.0
75.10	45032.0
76.00	4050.0
77.00	643.0
78.90	3858.0
79.90	1221.0
80.90	3568.0
81.90	776.0
85.80	105.0
87.00	3949.0
88.00	3793.0
90.90	319.0
92.10	2650.0
93.00	3998.0
94.10	10729.0
95.10	83312.0
96.10	5673.0
103.90	390.0
104.60	137.0
106.00	530.0
110.80	103.0
113.00	106.0
116.00	416.0
117.00	758.0
117.80	343.0
118.90	670.0
127.90	358.0
128.80	127.0
130.00	311.0
131.00	196.0
134.90	157.0
136.90	142.0
141.00	849.0
142.90	1222.0
144.10	104.0
145.00	485.0
145.90	124.0
147.90	301.0
154.80	186.0
156.90	224.0
171.00	221.0
172.10	1210.0
174.10	63760.0
175.10	5232.0
176.10	61728.0
177.00	3540.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24