

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU063021\  
 Data File : VU044267.D  
 Acq On : 30 Jun 2021 18:03  
 Operator : SY/MD  
 Sample : M2905-11  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :

Quant Time: Jul 01 02:39:55 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR062121WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Jul 01 02:36:13 2021  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|
| -----                         |        |       |          |          |        |          |
| Internal Standards            |        |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 6.256  | 114   | 149232   | 5.000    | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 9.423  | 117   | 141505   | 5.000    | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.819 | 152   | 78390    | 5.000    | ug/L   | 0.00     |
| System Monitoring Compounds   |        |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.600  | 65    | 34900    | 4.319    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 86.400%  |
| 7) Chloroethane-d5            | 1.919  | 69    | 34586    | 4.347    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 87.000%  |
| 11) 1,1-Dichloroethene-d2     | 2.571  | 65    | 18688    | 4.506    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 90.200%  |
| 20) 2-Butanone-d5             | 4.649  | 46    | 107127   | 36.005   | ug/L   | 0.02     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 72.000%  |
| 24) Chloroform-d              | 5.070  | 84    | 86551    | 4.758    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 95.200%  |
| 26) 1,2-Dichloroethane-d4     | 5.710  | 65    | 48956    | 4.503    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 90.000%  |
| 32) Benzene-d6                | 5.735  | 84    | 169562   | 4.825    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 96.400%  |
| 36) 1,2-Dichloropropane-d6    | 6.697  | 67    | 54530    | 4.788    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 95.800%  |
| 41) Toluene-d8                | 7.902  | 98    | 158461   | 4.859    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 97.200%  |
| 43) trans-1,3-Dichloroprop... | 8.185  | 79    | 23299    | 4.410    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 88.200%  |
| 46) 2-Hexanone-d5             | 8.639  | 63    | 110173   | 43.785   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 87.560%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.764 | 84    | 47927    | 4.733    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 94.600%  |
| 66) 1,2-Dichlorobenzene-d4    | 12.198 | 152   | 69152    | 5.354    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 107.000% |
| Target Compounds              |        |       |          |          |        |          |
|                               |        |       |          |          | Qvalue |          |
| 5) Vinyl chloride             | 1.607  | 62    | 28189    | 2.673    | ug/L   | 99       |
| 8) Chloroethane               | 1.938  | 64    | 3528     | 0.492    | ug/L # | 69       |
| 13) Acetone                   | 2.671  | 43    | 10277    | 7.725    | ug/L # | 48       |
| 14) Carbon disulfide          | 2.803  | 76    | 1840     | 0.069    | ug/L # | 74       |
| 17) Methyl tert-butyl Ether   | 3.378  | 73    | 2028     | 0.079    | ug/L # | 63       |
| 18) trans-1,2-Dichloroethene  | 3.359  | 96    | 16210    | 1.767    | ug/L   | 98       |
| 19) 1,1-Dichloroethane        | 3.880  | 63    | 21675    | 1.239    | ug/L   | 97       |
| 21) 2-Butanone                | 4.459  | 43    | 456664   | 151.098  | ug/L # | 5        |
| 22) cis-1,2-Dichloroethene    | 4.671  | 96    | 2242     | 0.223    | ug/L   | 87       |
| 27) 1,2-Dichloroethane        | 5.793  | 62    | 3826     | 0.307    | ug/L   | 97       |
| 30) Cyclohexane               | 5.398  | 56    | 3133     | 0.191    | ug/L # | 92       |
| 33) Benzene                   | 5.780  | 78    | 186065   | 5.012    | ug/L   | 100      |
| 35) Methylcyclohexane         | 6.774  | 83    | 1772     | 0.107    | ug/L # | 33       |
| 37) 1,2-Dichloropropane       | 6.800  | 63    | 5741     | 0.586    | ug/L # | 92       |
| 39) cis-1,3-Dichloropropene   | 7.574  | 75    | 1686     | 0.105    | ug/L # | 64       |
| 40) 4-Methyl-2-pentanone      | 7.800  | 43    | 7748     | 0.983    | ug/L # | 89       |
| 42) Toluene                   | 7.976  | 91    | 7804     | 0.191    | ug/L   | 96       |
| 48) 2-Hexanone                | 8.639  | 43    | 291082   | 52.429   | ug/L # | 39       |
| 51) Chlorobenzene             | 9.452  | 112   | 114831   | 4.386    | ug/L   | 98       |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU063021\  
 Data File : VU044267.D  
 Acq On : 30 Jun 2021 18:03  
 Operator : SY/MD  
 Sample : M2905-11  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :

Quant Time: Jul 01 02:39:55 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR062121WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Jul 01 02:36:13 2021  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |  |
|-------------------------------|--------|------|----------|--------|--------|----------|--|
| -----                         |        |      |          |        |        |          |  |
| 57) 1,1,2,2-Tetrachloroethane | 10.709 | 83   | 822032   | 83.963 | ug/L # | 31       |  |
| 60) Isopropylbenzene          | 10.491 | 105  | 39297    | 0.824  | ug/L   | 98       |  |
| 62) 1,3,5-Trimethylbenzene    | 11.298 | 105  | 6172     | 0.149  | ug/L # | 76       |  |
| 63) 1,2,4-Trimethylbenzene    | 11.298 | 105  | 6172     | 0.145  | ug/L # | 80       |  |
| 64) 1,3-Dichlorobenzene       | 11.751 | 146  | 3330     | 0.155  | ug/L # | 73       |  |
| 65) 1,4-Dichlorobenzene       | 11.841 | 146  | 17223    | 0.794  | ug/L # | 83       |  |
| 67) 1,2-Dichlorobenzene       | 12.221 | 146  | 10638    | 0.526  | ug/L   | 95       |  |
| 68) 1,2-Dibromo-3-chloropr... | 13.028 | 75   | 15235    | 8.242  | ug/L # | 1        |  |
| 71) Naphthalene               | 14.092 | 128  | 46302    | 1.842  | ug/L # | 81       |  |
| 72) 1,2,3-Trichlorobenzene    | 14.336 | 180  | 3321     | 0.277  | ug/L # | 34       |  |
| -----                         |        |      |          |        |        |          |  |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU063021\  
Data File : VU044267.D  
Acq On : 30 Jun 2021 18:03  
Operator : SY/MD  
Sample : M2905-11  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :

Quant Time: Jul 01 02:39:55 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR062121WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Jul 01 02:36:13 2021  
Response via : Initial Calibration

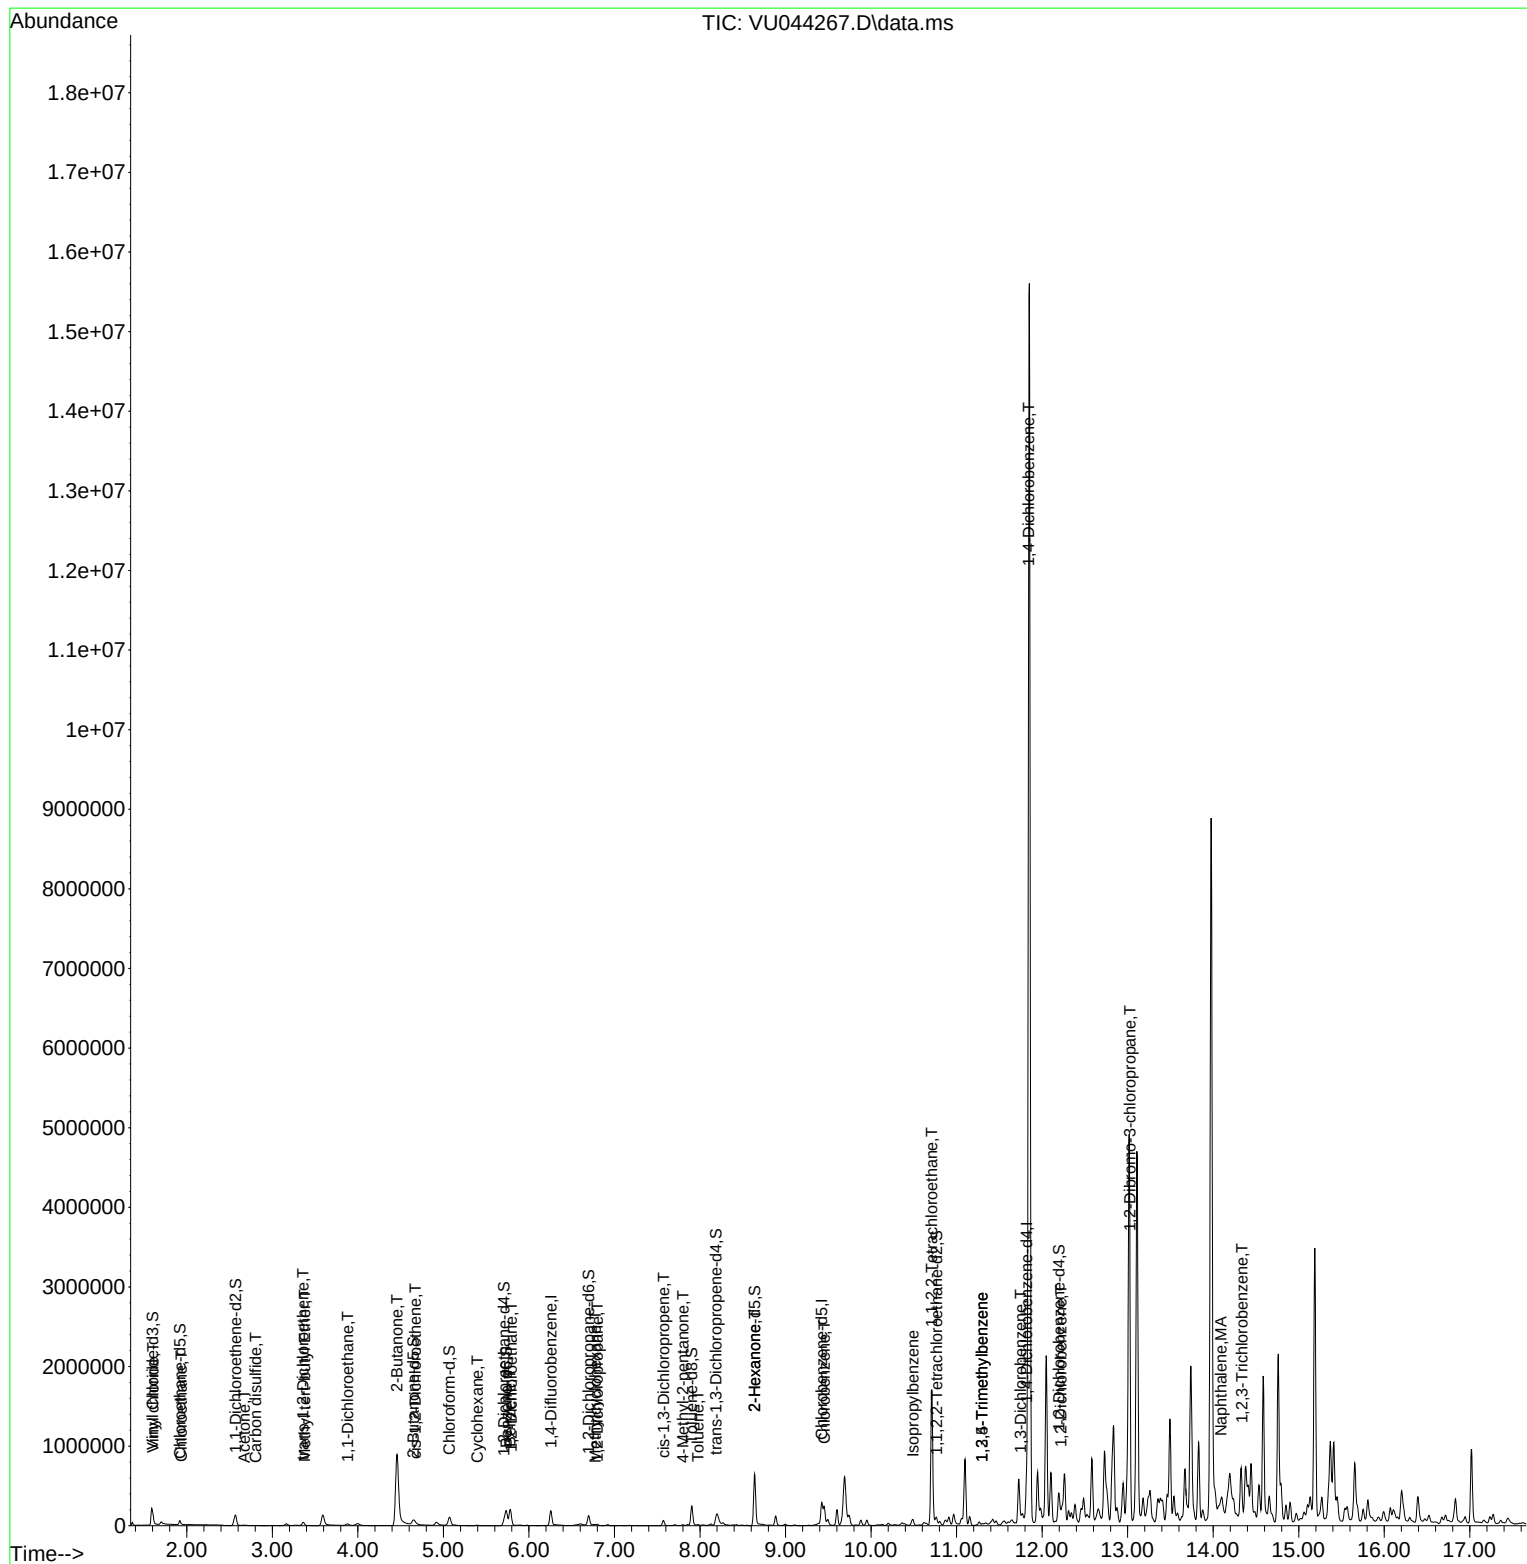



#5

Vinyl chloride

Concen: 2.673 ug/L

RT: 1.607 min Scan# 83

Delta R.T. -0.000 min

Lab File: VU044267.D





Acq: 30 Jun 2021 18:03

Tgt Ion: 62 Resp: 28189

Ion Ratio Lower Upper

62 100

64 33.5 23.7 44.1

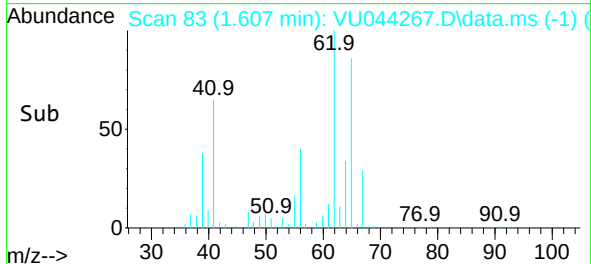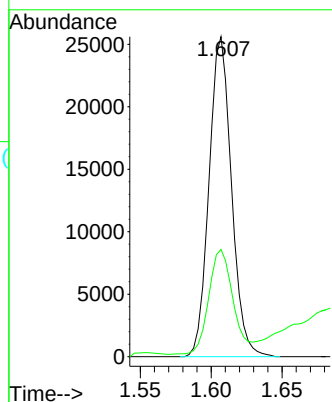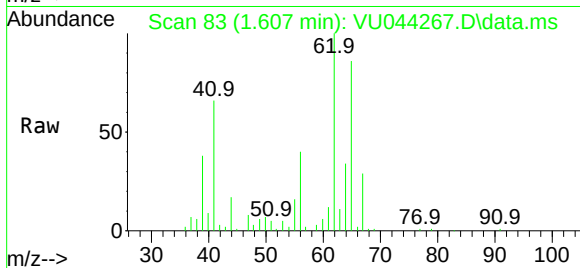

#8

Chloroethane

Concen: 0.492 ug/L

RT: 1.938 min Scan# 186

Delta R.T. -0.000 min

Lab File: VU044267.D




Acq: 30 Jun 2021 18:03


Tgt Ion: 64 Resp: 3528

Ion Ratio Lower Upper

64 100

66 15.0 22.7 42.3#


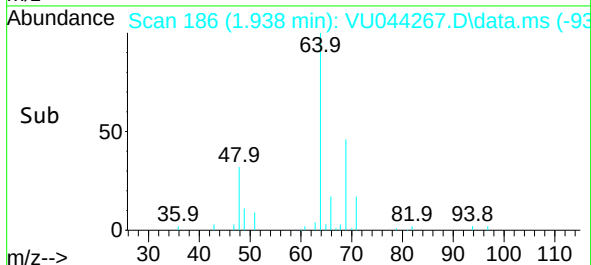

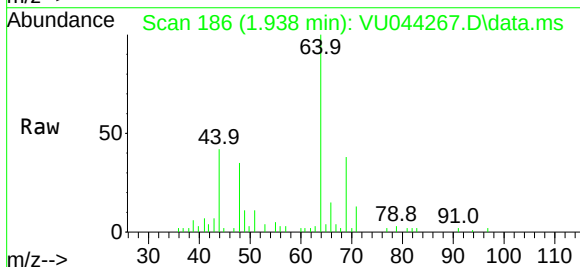




#13  
Acetone  
Concen: 7.725 ug/L  
RT: 2.671 min Scan# 414  
Delta R.T. 0.039 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03




Instrument :  
MSVOA\_U  
ClientSampled :


Tgt Ion: 43 Resp: 10277  
Ion Ratio Lower Upper  
43 100  
58 0.0 0.0 53.8

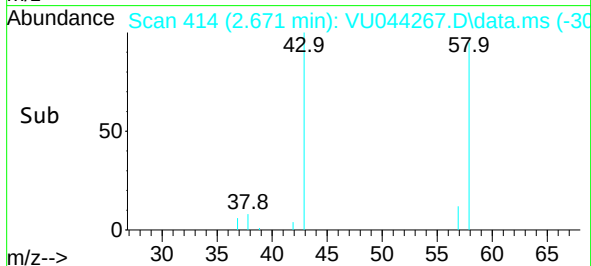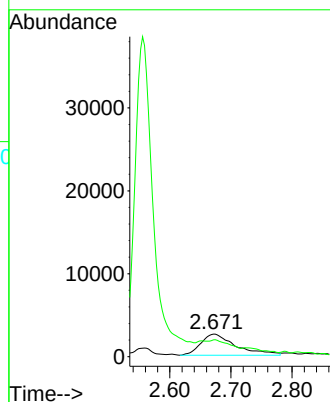

#14  
Carbon disulfide  
Concen: 0.069 ug/L  
RT: 2.803 min Scan# 455  
Delta R.T. 0.003 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03

Tgt Ion: 76 Resp: 1840  
Ion Ratio Lower Upper  
76 100  
78 0.0 7.4 11.2#


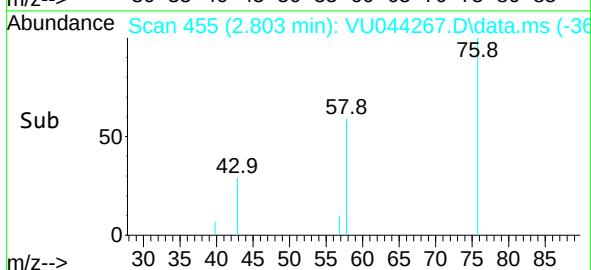
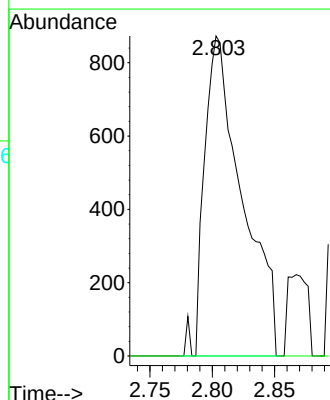
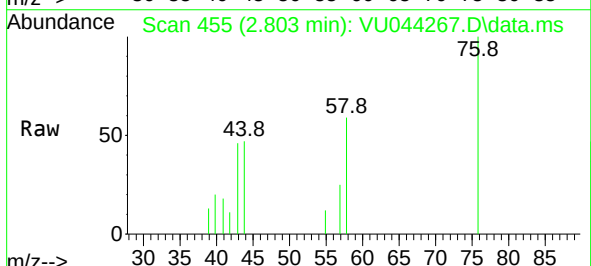




#17  
Methyl tert-butyl Ether  
Concen: 0.079 ug/L  
RT: 3.378 min Scan# 634  
Delta R.T. 0.003 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03




Instrument :  
MSVOA\_U  
ClientSampled :


Tgt Ion: 73 Resp: 2028  
Ion Ratio Lower Upper  
73 100  
43 0.0 17.6 26.4#  
57 8.7 17.8 26.8#

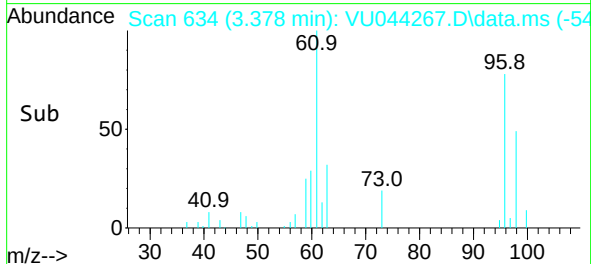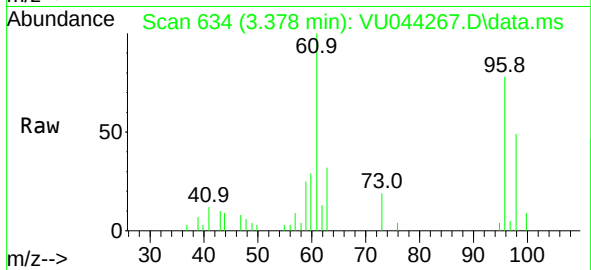

#18  
trans-1,2-Dichloroethene  
Concen: 1.767 ug/L  
RT: 3.359 min Scan# 628  
Delta R.T. -0.003 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03

Tgt Ion: 96 Resp: 16210  
Ion Ratio Lower Upper  
96 100  
61 146.6 100.2 186.2  
98 65.1 44.9 83.5

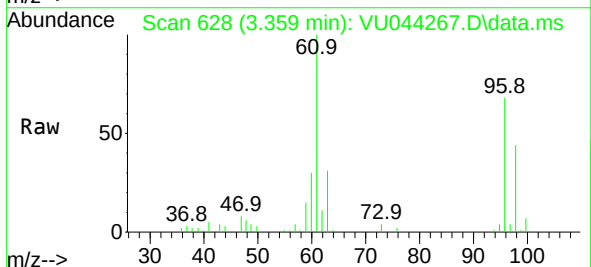

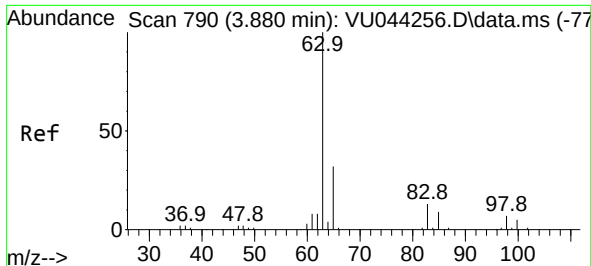

#19

1,1-Dichloroethane

Concen: 1.239 ug/L

RT: 3.880 min Scan# 790





Delta R.T. -0.000 min

Lab File: VU044267.D

Acq: 30 Jun 2021 18:03

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 63    | Resp: | 21675 |
| Ion      | Ratio | Lower | Upper |
| 63       | 100   |       |       |
| 65       | 34.2  | 22.3  | 41.3  |
| 83       | 14.6  | 9.9   | 18.5  |

Instrument :  
MSVOA\_U  
ClientSampleId :

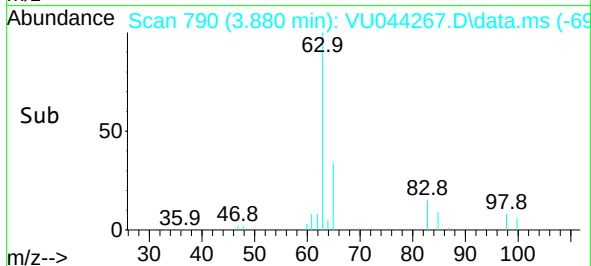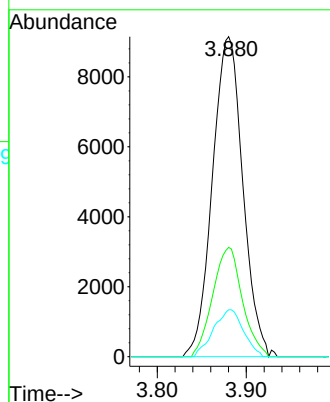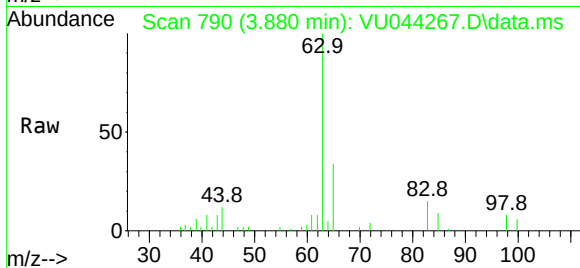

#21

2-Butanone

Concen: 151.098 ug/L




RT: 4.459 min Scan# 970


Delta R.T. -0.251 min

Lab File: VU044267.D

Acq: 30 Jun 2021 18:03

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 43    | Resp: | 456664 |
| Ion      | Ratio | Lower | Upper  |
| 43       | 100   |       |        |
| 72       | 75.9  | 13.4  | 40.1#  |


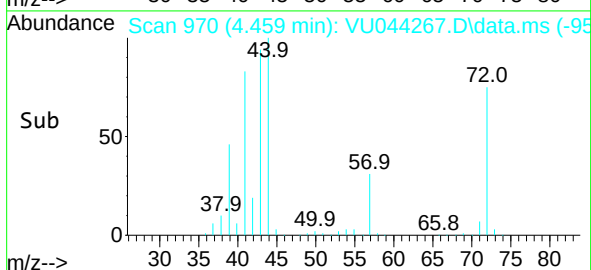
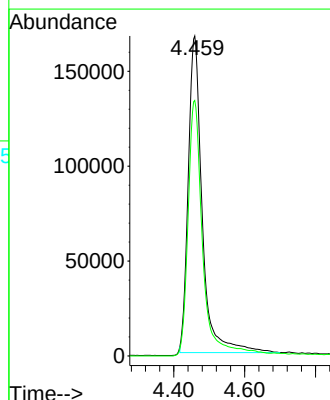
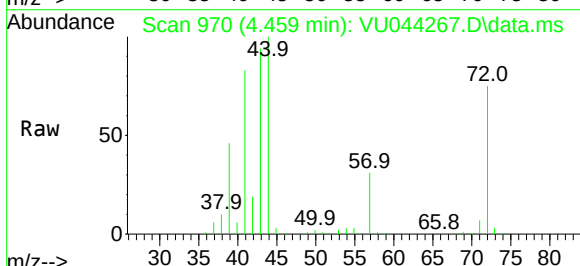


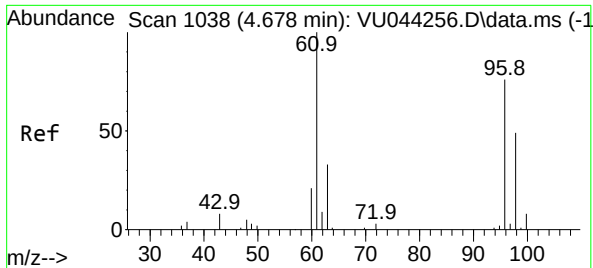

#22  
 cis-1,2-Dichloroethene  
 Concen: 0.223 ug/L  
 RT: 4.671 min Scan# 1036  
 Delta R.T. -0.006 min  
 Lab File: VU044267.D  
 Acq: 30 Jun 2021 18:03




Instrument :  
 MSVOA\_U  
 ClientSampled :

Tgt Ion: 96 Resp: 2242  
 Ion Ratio Lower Upper  
 96 100  
 61 122.8 98.8 183.6  
 98 56.3 44.8 83.2

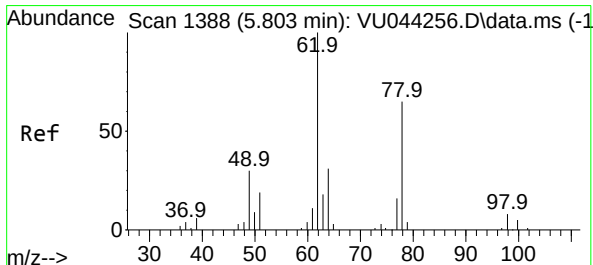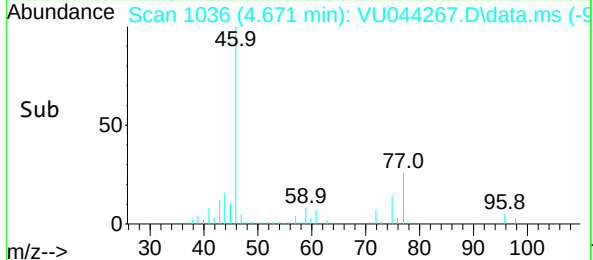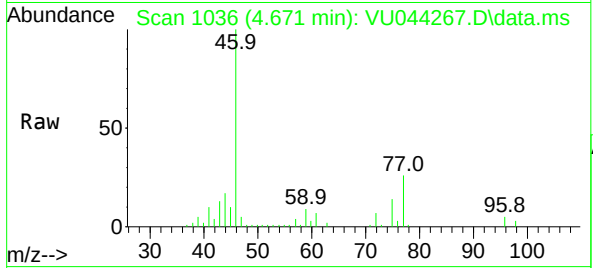


#27  
 1,2-Dichloroethane  
 Concen: 0.307 ug/L  
 RT: 5.793 min Scan# 1385  
 Delta R.T. -0.010 min  
 Lab File: VU044267.D  
 Acq: 30 Jun 2021 18:03

Tgt Ion: 62 Resp: 3826  
 Ion Ratio Lower Upper  
 62 100  
 98 7.4 6.8 10.2

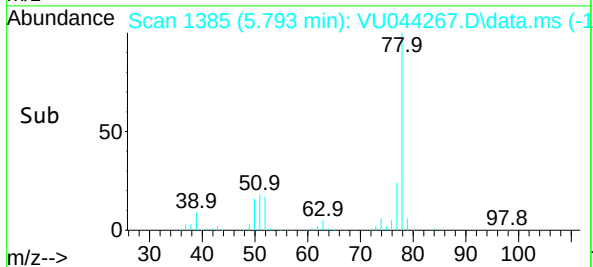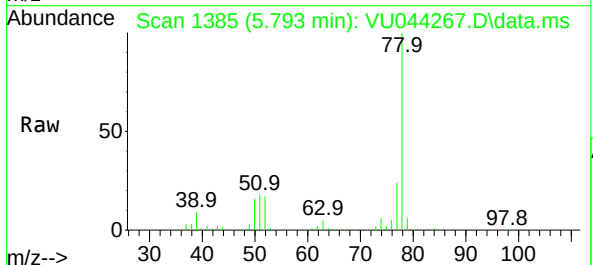



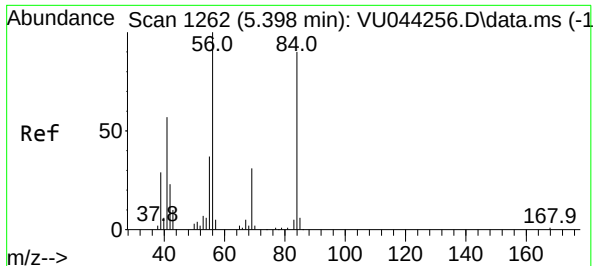

#30

Cyclohexane

Concen: 0.191 ug/L

RT: 5.398 min Scan# 1262

Delta R.T. -0.000 min

Lab File: VU044267.D

Acq: 30 Jun 2021 18:03





Tgt Ion: 56 Resp: 3133

Ion Ratio Lower Upper

56 100

69 23.8 24.8 37.2#

84 90.9 67.8 101.8

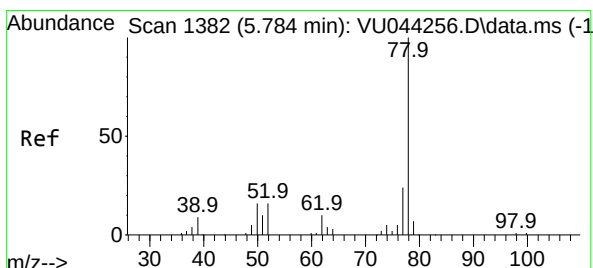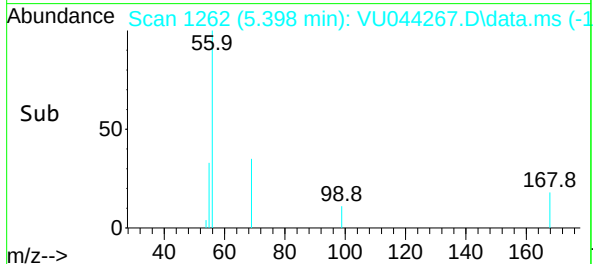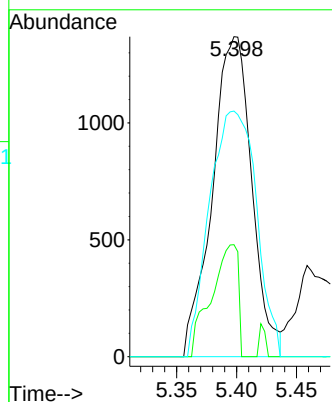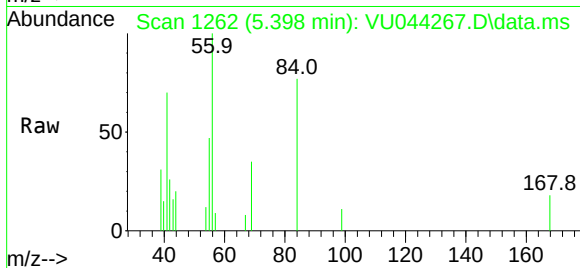

#33

Benzene

Concen: 5.012 ug/L




RT: 5.780 min Scan# 1381


Delta R.T. -0.003 min

Lab File: VU044267.D

Acq: 30 Jun 2021 18:03

Tgt Ion: 78 Resp: 186065


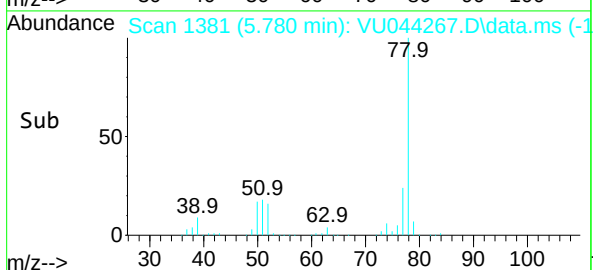

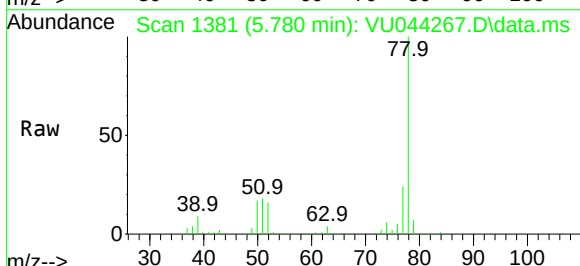


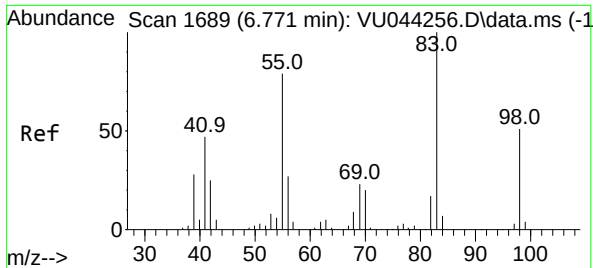

#35  
Methylcyclohexane  
Concen: 0.107 ug/L  
RT: 6.774 min Scan# 1690  
Delta R.T. 0.003 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion: 83 Resp: 1772  
Ion Ratio Lower Upper  
83 100  
55 167.9 63.4 95.0#  
98 41.1 39.4 59.0

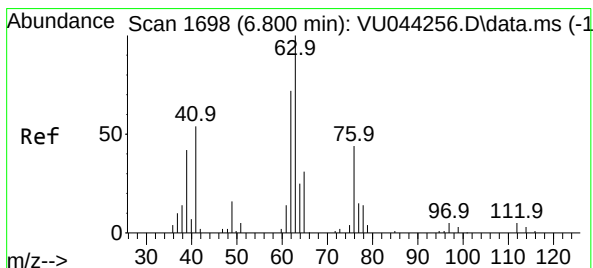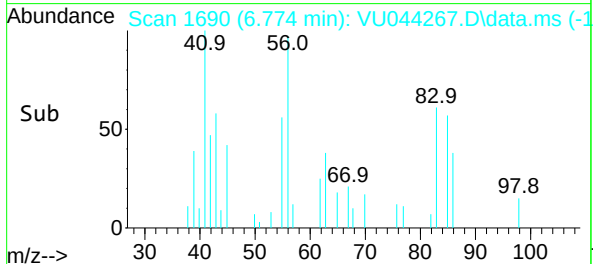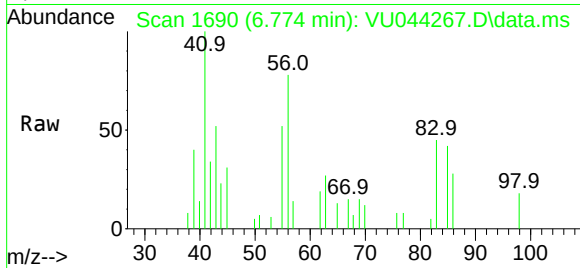

#37  
1,2-Dichloropropane  
Concen: 0.586 ug/L  
RT: 6.800 min Scan# 1698  
Delta R.T. -0.000 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03

Tgt Ion: 63 Resp: 5741  
Ion Ratio Lower Upper  
63 100  
112 1.8 3.5 5.3#

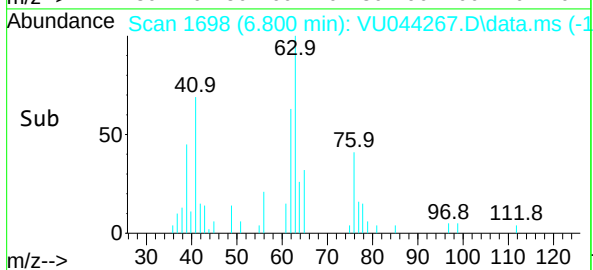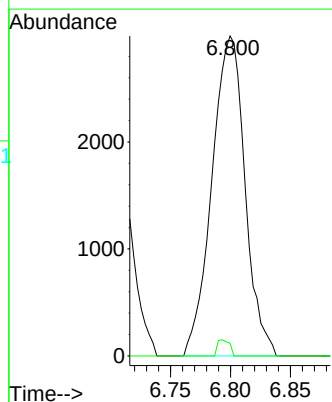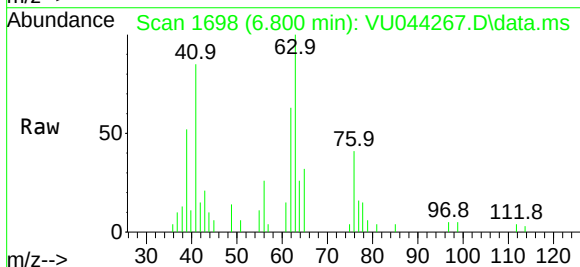




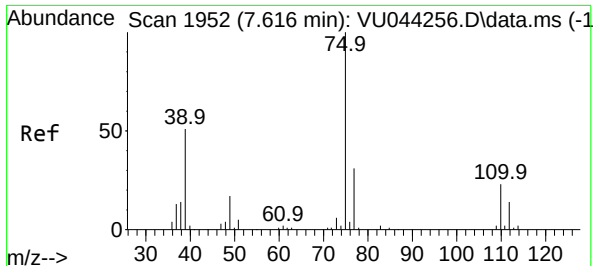


#39

cis-1,3-Dichloropropene  
Concen: 0.105 ug/L  
RT: 7.574 min Scan# 1939  
Delta R.T. -0.042 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03

Instrument :  
MSVOA\_U  
ClientSampled :




Tgt Ion: 75 Resp: 1686  
Ion Ratio Lower Upper  
75 100  
77 52.0 22.5 41.7#

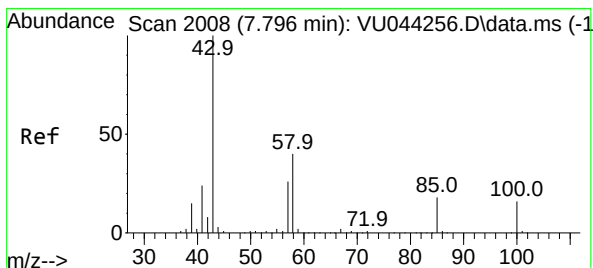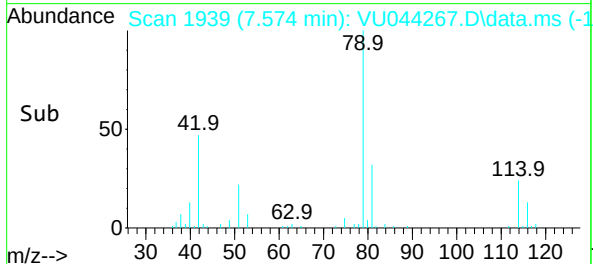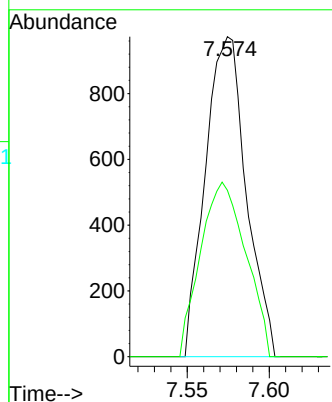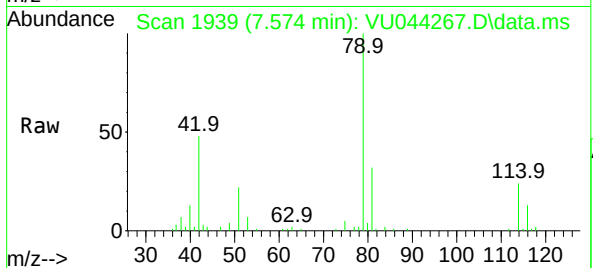


#40

4-Methyl-2-pentanone  
Concen: 0.983 ug/L  
RT: 7.800 min Scan# 2009  
Delta R.T. 0.003 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03

Tgt Ion: 43 Resp: 7748  
Ion Ratio Lower Upper  
43 100  
58 39.4 31.2 46.8  
100 0.0 12.3 18.5#

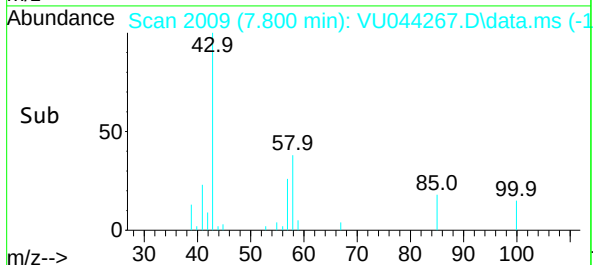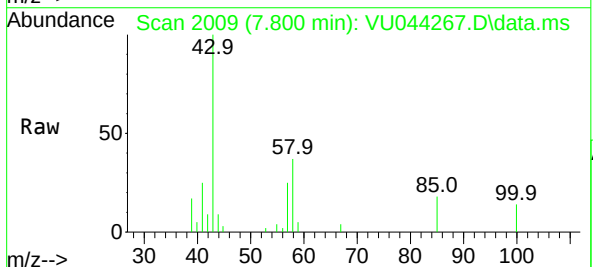

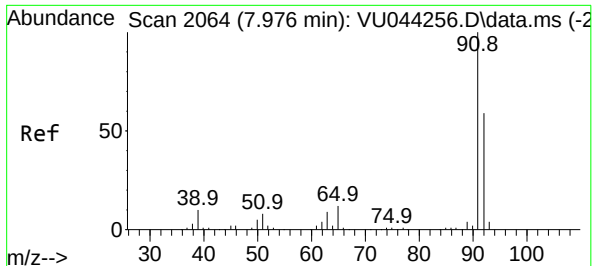

#42

Toluene

Concen: 0.191 ug/L

RT: 7.976 min Scan# 2064





Delta R.T. -0.000 min

Lab File: VU044267.D

Acq: 30 Jun 2021 18:03

Tgt Ion: 91 Resp: 7804

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 91  | 100   |       |       |
| 92  | 61.9  | 41.2  | 76.6  |

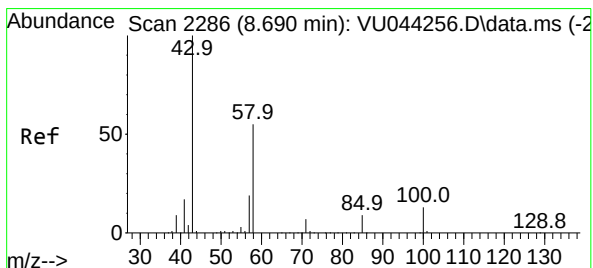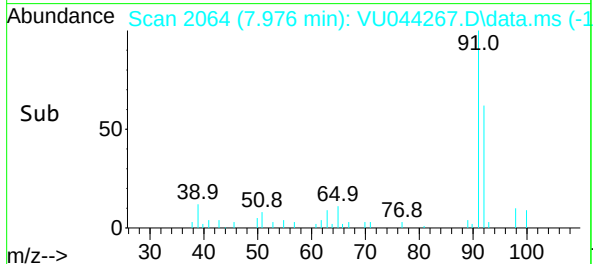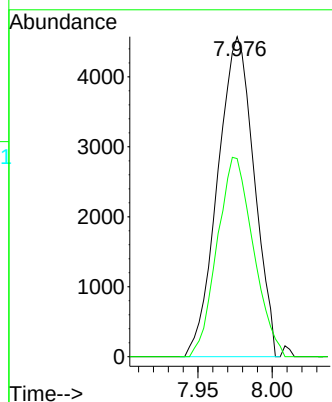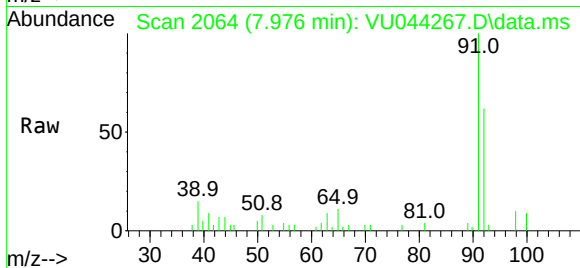

#48

2-Hexanone

Concen: 52.429 ug/L

RT: 8.639 min Scan# 2270




Delta R.T. -0.051 min


Lab File: VU044267.D

Acq: 30 Jun 2021 18:03

Tgt Ion: 43 Resp: 291082

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 43  | 100   |       |       |
| 58  | 0.9   | 44.7  | 67.1# |
| 57  | 1.5   | 15.7  | 23.5# |
| 100 | 0.0   | 9.8   | 14.8# |


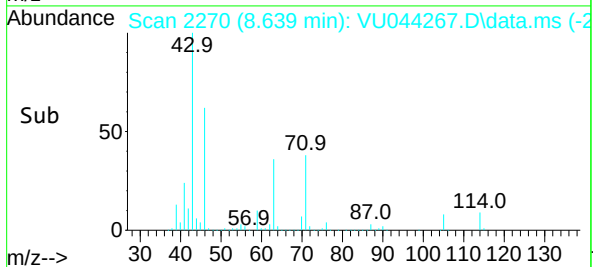

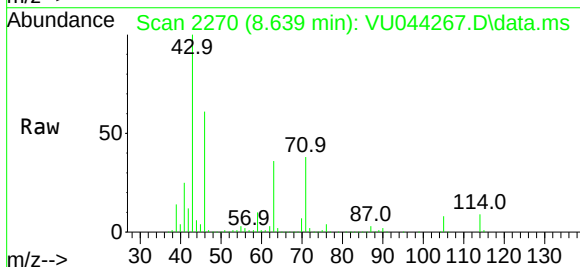


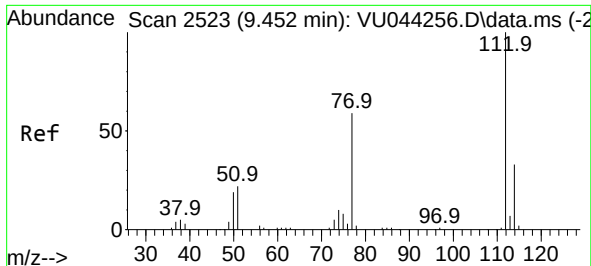

#51  
Chlorobenzene  
Concen: 4.386 ug/L  
RT: 9.452 min Scan# 2523  
Delta R.T. -0.000 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03




Instrument :  
MSVOA\_U  
ClientSampled :


Tgt Ion:112 Resp: 114831  
Ion Ratio Lower Upper  
112 100  
114 33.6 22.0 41.0  
77 61.7 48.9 73.3

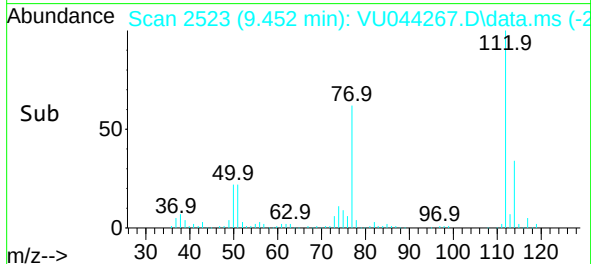

#57  
1,1,2,2-Tetrachloroethane  
Concen: 83.963 ug/L  
RT: 10.709 min Scan# 2914  
Delta R.T. -0.080 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03

Tgt Ion: 83 Resp: 822032  
Ion Ratio Lower Upper  
83 100  
85 5.8 45.5 84.5#  
131 0.2 7.9 11.9#


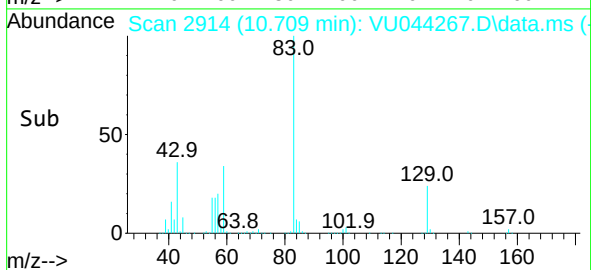

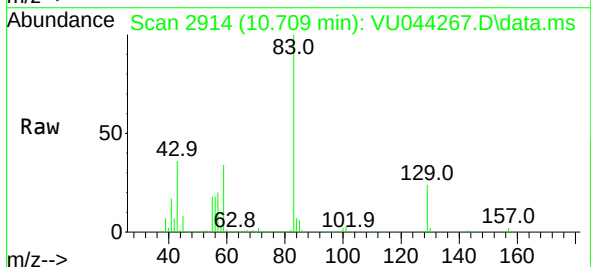




#60  
Isopropylbenzene  
Concen: 0.824 ug/L  
RT: 10.491 min Scan# 2846  
Delta R.T. -0.000 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03




Instrument :  
MSVOA\_U  
ClientSampled :


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 105   | Resp: | 39297 |
| Ion      | Ratio | Lower | Upper |
| 105      | 100   |       |       |
| 120      | 25.6  | 20.7  | 31.1  |
| 77       | 17.4  | 12.9  | 19.3  |

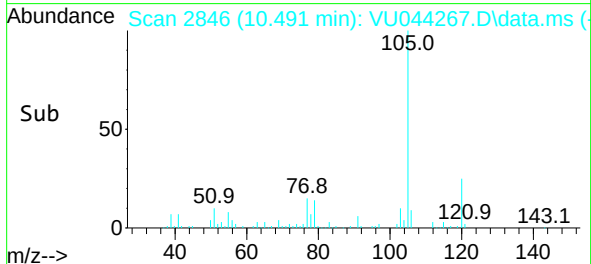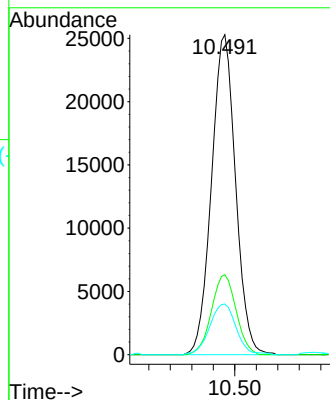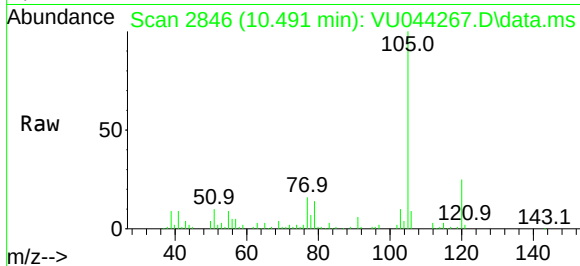

#62  
1,3,5-Trimethylbenzene  
Concen: 0.149 ug/L  
RT: 11.298 min Scan# 3097  
Delta R.T. 0.203 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 105   | Resp: | 6172  |
| Ion      | Ratio | Lower | Upper |
| 105      | 100   |       |       |
| 120      | 31.4  | 38.0  | 57.0# |


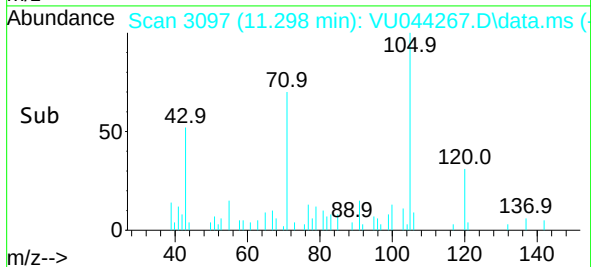
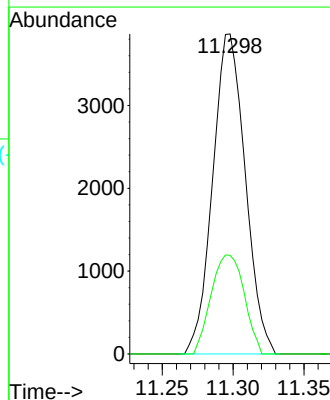
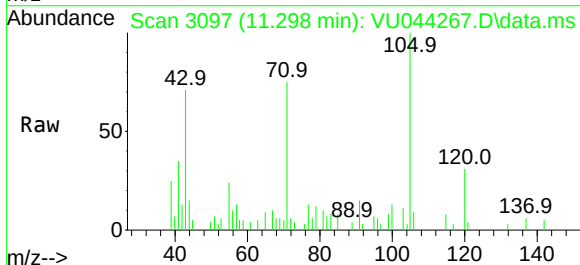




#63  
1,2,4-Trimethylbenzene  
Concen: 0.145 ug/L  
RT: 11.298 min Scan# 3097  
Delta R.T. -0.177 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03




Instrument :  
MSVOA\_U  
ClientSampled :


Tgt Ion:105 Resp: 6172  
Ion Ratio Lower Upper  
105 100  
120 31.4 35.6 53.4#

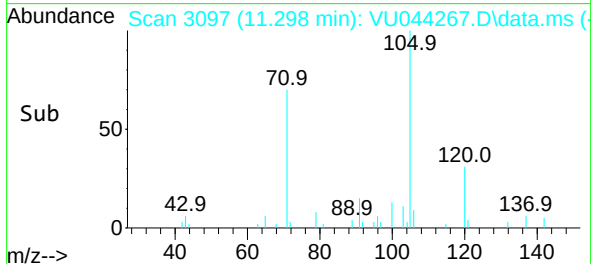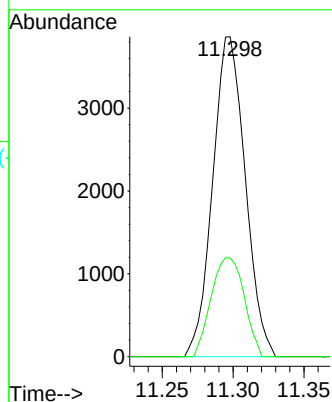

#64  
1,3-Dichlorobenzene  
Concen: 0.155 ug/L  
RT: 11.751 min Scan# 3238  
Delta R.T. -0.000 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03

Tgt Ion:146 Resp: 3330  
Ion Ratio Lower Upper  
146 100  
111 85.1 29.8 55.3#  
148 66.8 45.8 85.2


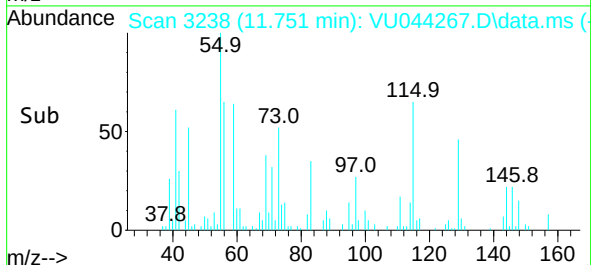

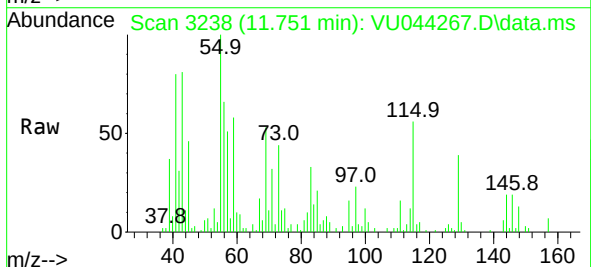


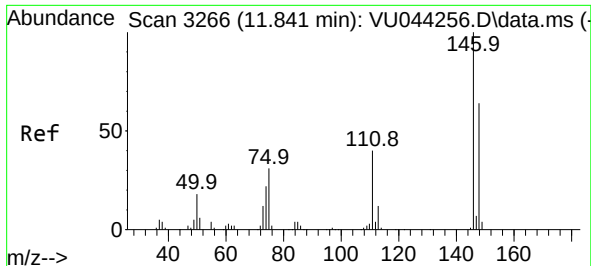

#65  
1,4-Dichlorobenzene  
Concen: 0.794 ug/L  
RT: 11.841 min Scan# 3266  
Delta R.T. -0.000 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03




Instrument :  
MSVOA\_U  
ClientSampleId :

Tgt Ion:146 Resp: 17223  
Ion Ratio Lower Upper  
146 100  
111 67.0 28.2 52.4#  
148 64.5 45.1 83.9

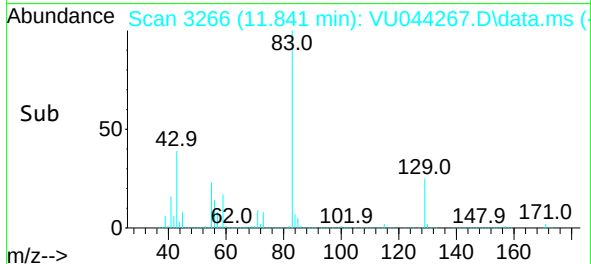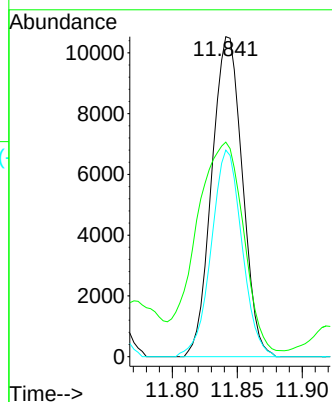


#67  
1,2-Dichlorobenzene  
Concen: 0.526 ug/L  
RT: 12.221 min Scan# 3384  
Delta R.T. 0.003 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03

Tgt Ion:146 Resp: 10638  
Ion Ratio Lower Upper  
146 100  
111 51.6 35.0 52.6  
148 63.5 51.2 76.8

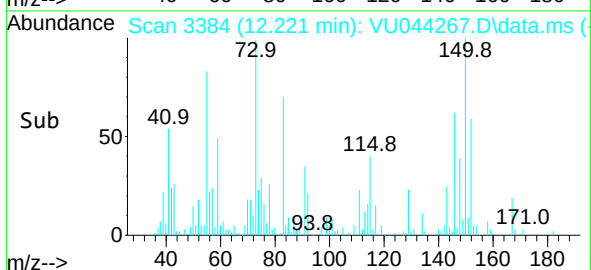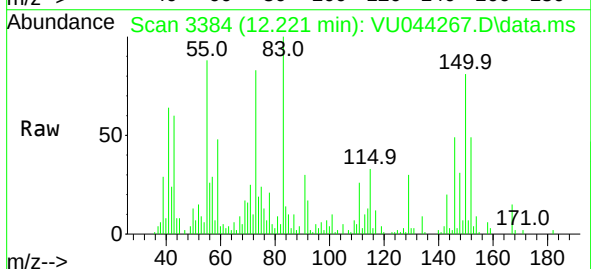







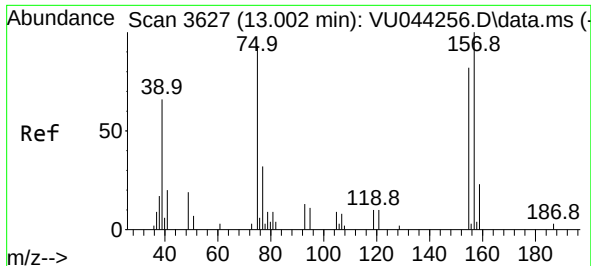

#68  
1,2-Dibromo-3-chloropropane  
Concen: 8.242 ug/L  
RT: 13.028 min Scan# 3635  
Delta R.T. 0.026 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion: 75 Resp: 15235  
Ion Ratio Lower Upper  
75 100  
155 3.3 59.9 89.9#  
157 426.6 79.3 118.9#

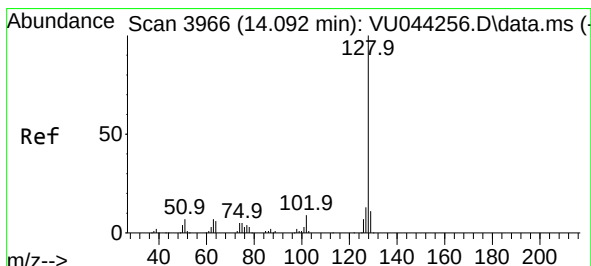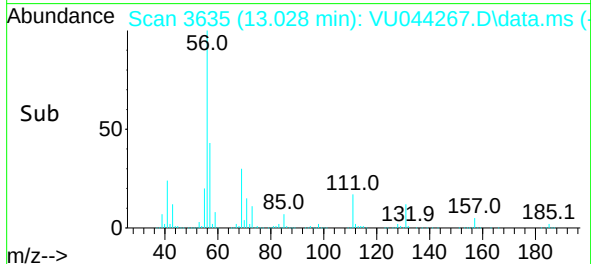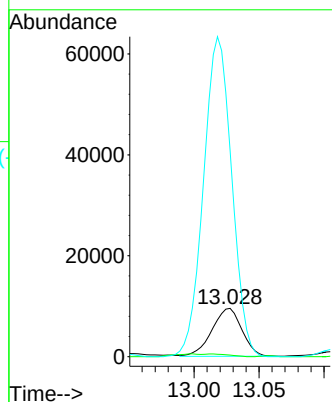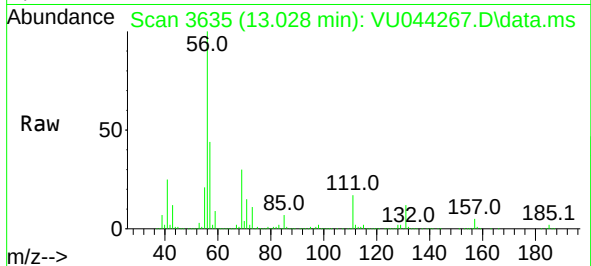

#71  
Naphthalene  
Concen: 1.842 ug/L  
RT: 14.092 min Scan# 3966  
Delta R.T. -0.000 min  
Lab File: VU044267.D  
Acq: 30 Jun 2021 18:03

Tgt Ion:128 Resp: 46302  
Ion Ratio Lower Upper  
128 100  
129 0.0 8.9 13.3#  
127 17.3 10.3 15.5#

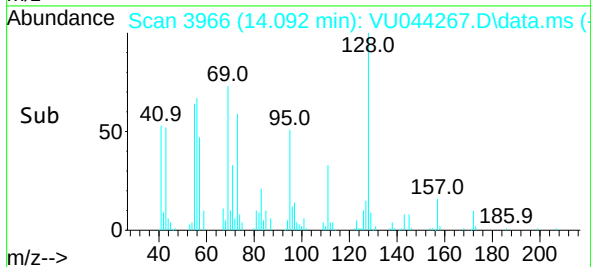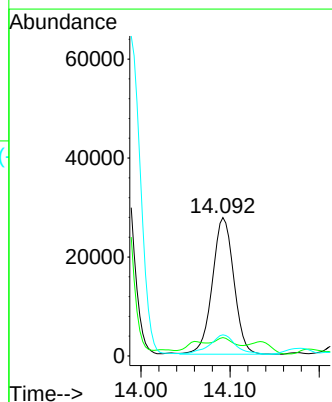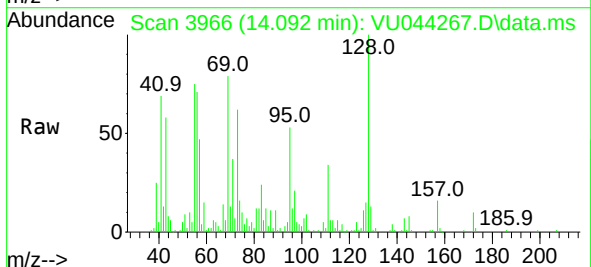

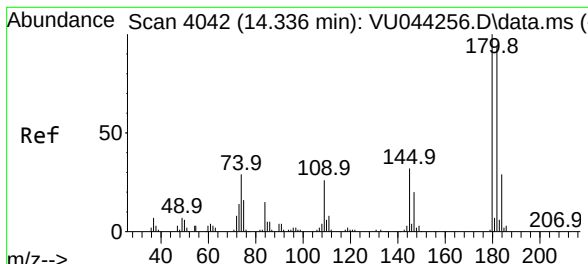

#72  
 1,2,3-Trichlorobenzene  
 Concen: 0.277 ug/L  
 RT: 14.336 min Scan# 4042  
 Delta R.T. -0.000 min  
 Lab File: VU044267.D  
 Acq: 30 Jun 2021 18:03

Instrument :  
 MSVOA\_U  
 ClientSampleId :

|           |       |       |        |
|-----------|-------|-------|--------|
| Tgt Ion:  | 180   | Resp: | 3321   |
| Ion Ratio | Lower | Upper |        |
| 180       | 100   |       |        |
| 182       | 28.6  | 76.4  | 114.6# |
| 145       | 0.0   | 26.5  | 39.7#  |

