




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063021\
Data File : VU044269.D
Acq On : 30 Jun 2021 18:51
Operator : SY/MD
Sample : M2905-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBK36

Manual Integrations
APPROVED

MMDadoda
7/1/2021 1:30:11 PM

Quant Time: Jul 01 02:40:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR062121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 01 02:36:13 2021
Response via : Initial Calibration

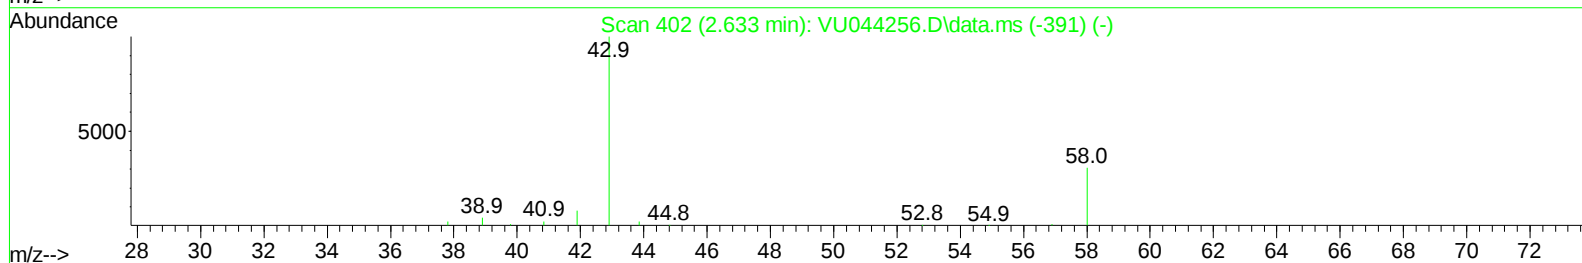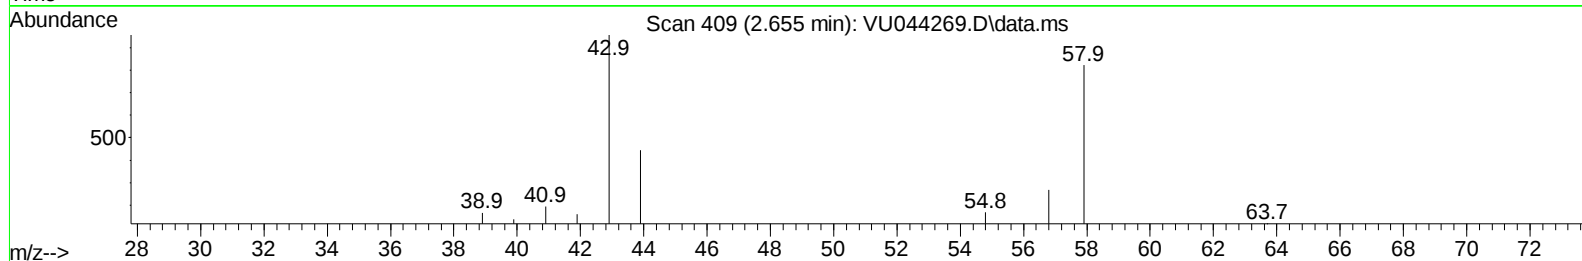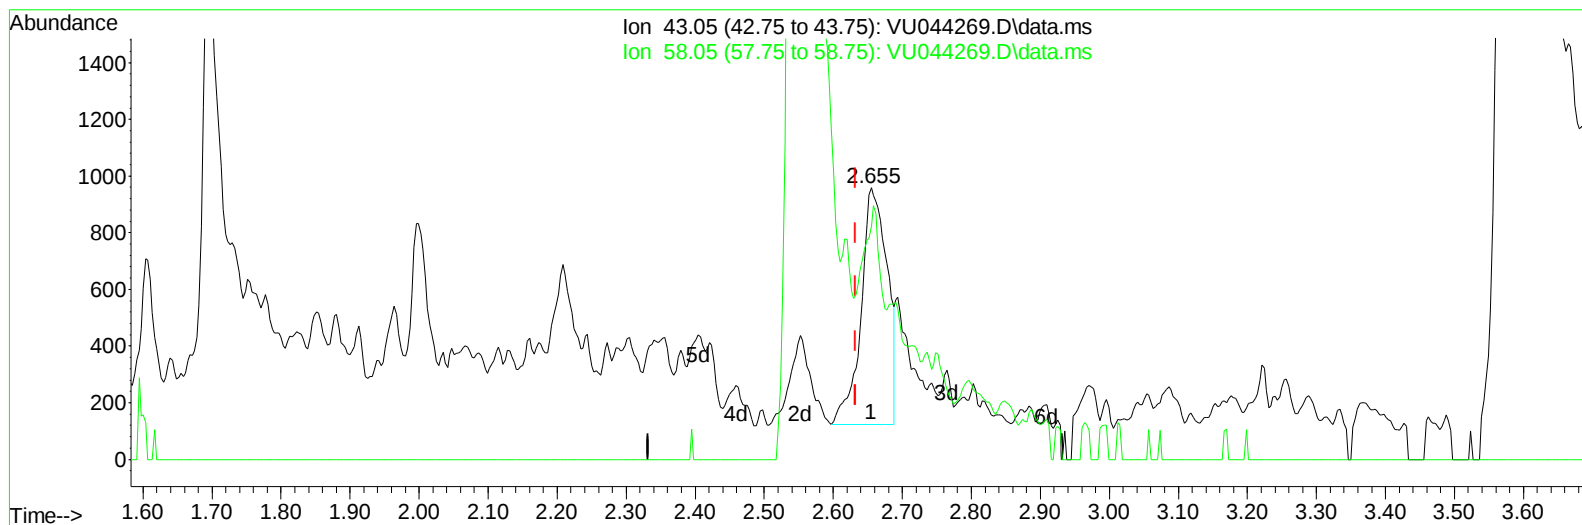

TIC: VU044269.D\data.ms

(13) Acetone (T)

2.655min (+ 0.023) 1.63 ug/L

response 2174

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	26.90	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063021\
Data File : VU044269.D
Acq On : 30 Jun 2021 18:51
Operator : SY/MD
Sample : M2905-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
DBK36

Manual Integrations
APPROVED

MMDadoda
7/1/2021 1:30:11 PM

Quant Time: Jul 01 02:40:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR062121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 01 02:36:13 2021
Response via : Initial Calibration

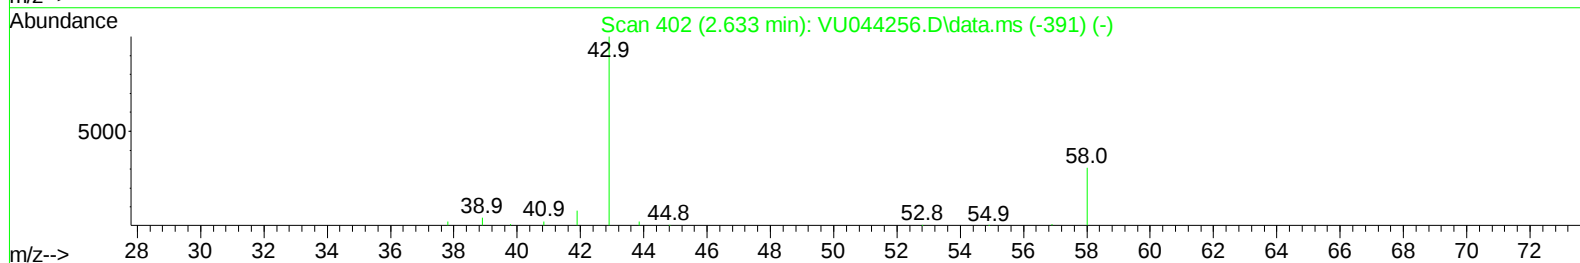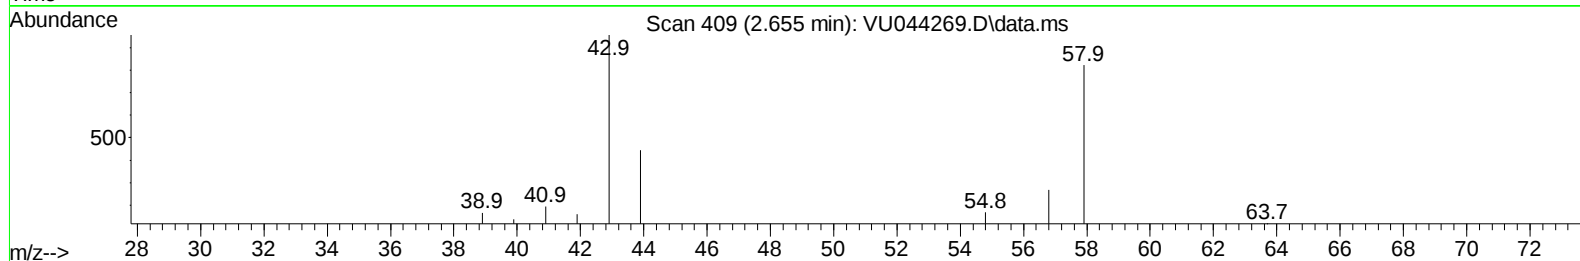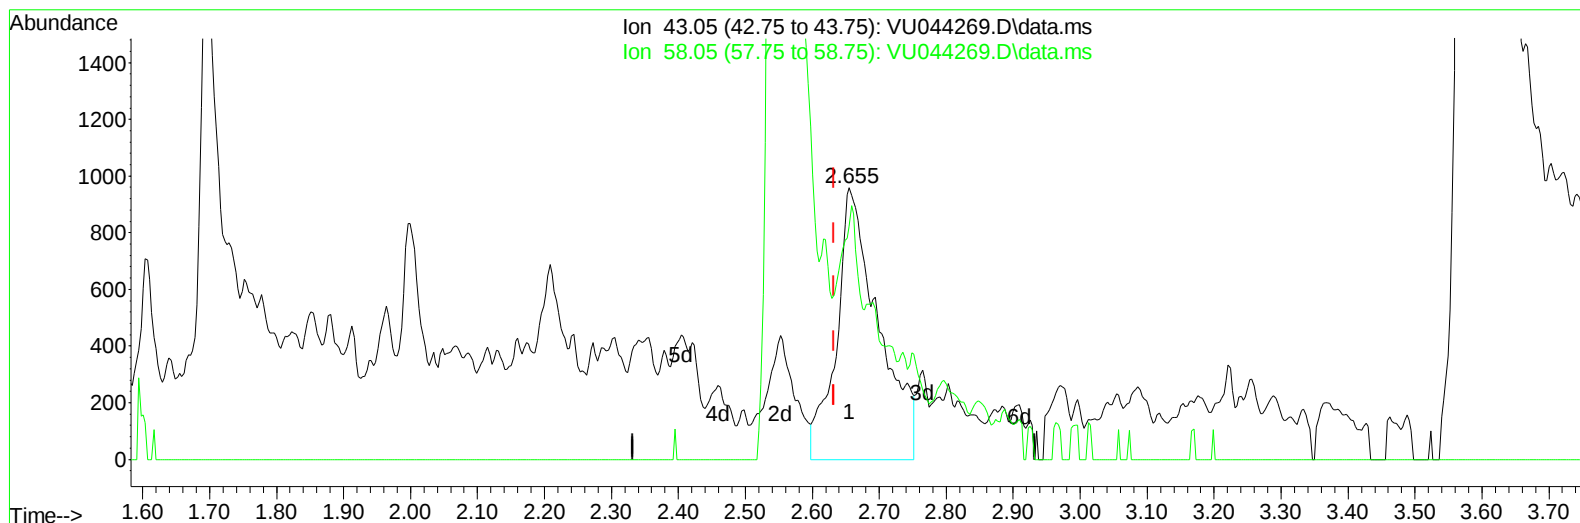

TIC: VU044269.D\data.ms

(13) Acetone (T)

2.655min (+ 0.023) 3.13 ug/L m

response 4171

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	26.90	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063021\
 Data File : VU044269.D
 Acq On : 30 Jun 2021 18:51
 Operator : SY/MD
 Sample : M2905-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBK36

Manual Integrations
 APPROVED

MMDadoda
 7/1/2021 1:30:11 PM

Quant Time: Jul 01 02:40:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR062121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jul 01 02:36:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	149520	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	141487	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	75833	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	37560	4.640	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.800%
7) Chloroethane-d5	1.919	69	38024	4.770	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.400%
11) 1,1-Dichloroethene-d2	2.572	65	19602	4.718	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	94.400%
20) 2-Butanone-d5	4.642	46	131235	44.023	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.040%
24) Chloroform-d	5.073	84	91209	5.005	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.000%
26) 1,2-Dichloroethane-d4	5.713	65	52607	4.829	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.600%
32) Benzene-d6	5.736	84	182180	5.184	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.600%
36) 1,2-Dichloropropane-d6	6.700	67	59329	5.210	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.200%
41) Toluene-d8	7.903	98	167435	5.135	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.600%
43) trans-1,3-Dichloroprop...	8.186	79	24503	4.639	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.800%
46) 2-Hexanone-d5	8.639	63	127445	50.655	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.320%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	50063	4.945	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.800%
66) 1,2-Dichlorobenzene-d4	12.198	152	70886	5.673	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.400%
Target Compounds						Qvalue
13) Acetone	2.655	43	4171m	3.129	ug/L	
14) Carbon disulfide	2.810	76	2128	0.080	ug/L	96
18) trans-1,2-Dichloroethene	3.363	96	3392	0.369	ug/L	95
19) 1,1-Dichloroethane	3.880	63	16122	0.920	ug/L #	87
22) cis-1,2-Dichloroethene	4.674	96	4420	0.440	ug/L	96
30) Cyclohexane	5.401	56	1856	0.113	ug/L	93
42) Toluene	7.977	91	5278	0.129	ug/L	96
51) Chlorobenzene	9.452	112	21900	0.836	ug/L	99
60) Isopropylbenzene	10.488	105	16389	0.355	ug/L	98
64) 1,3-Dichlorobenzene	11.751	146	2828	0.136	ug/L	94
65) 1,4-Dichlorobenzene	11.841	146	3533	0.168	ug/L #	87
67) 1,2-Dichlorobenzene	12.218	146	1955	0.100	ug/L #	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063021\
Data File : VU044269.D
Acq On : 30 Jun 2021 18:51
Operator : SY/MD
Sample : M2905-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBK36

Manual Integrations
APPROVED

MMDadoda
7/1/2021 1:30:11 PM

Quant Time: Jul 01 02:40:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR062121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 01 02:36:13 2021
Response via : Initial Calibration

