

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063021\
 Data File : VU044271.D
 Acq On : 30 Jun 2021 19:40
 Operator : SY/MD
 Sample : M2905-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBK38

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR062121WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU044271.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.571	372	383	400	rBV	95398	159264	2.24%	1.146%
2	4.674	1013	1037	1065	rBV2	159616	529835	7.45%	3.812%
3	5.073	1144	1161	1182	rBV	97646	217702	3.06%	1.566%
4	5.732	1345	1366	1378	rBV2	194613	517245	7.27%	3.721%
5	6.256	1515	1529	1545	rBV	196978	369459	5.19%	2.658%
6	6.549	1606	1620	1650	rBV	395050	744328	10.46%	5.355%
7	6.700	1653	1667	1687	rVB	126786	248192	3.49%	1.786%
8	7.571	1925	1938	1955	rBV	67553	119429	1.68%	0.859%
9	7.906	2023	2042	2056	rBV	258992	445985	6.27%	3.209%
10	8.185	2118	2129	2145	rBV3	43684	77524	1.09%	0.558%
11	8.558	2231	2245	2260	rBV	4274054	7113919	100.00%	51.183%
12	8.642	2261	2271	2303	rVB	348681	718061	10.09%	5.166%
13	9.423	2501	2514	2518	rBV	287291	449886	6.32%	3.237%
14	9.452	2519	2523	2552	rVB	309910	457621	6.43%	3.293%
15	10.764	2917	2931	2942	rBV	102168	164967	2.32%	1.187%
16	11.819	3246	3259	3278	rBV2	318013	605299	8.51%	4.355%
17	12.102	3336	3347	3360	rVB	46143	72363	1.02%	0.521%
18	12.208	3364	3380	3403	rVV2	363057	887802	12.48%	6.388%




Sum of corrected areas: 13898881

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063021\
Data File : VU044271.D
Acq On : 30 Jun 2021 19:40
Operator : SY/MD
Sample : M2905-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBK38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR062121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

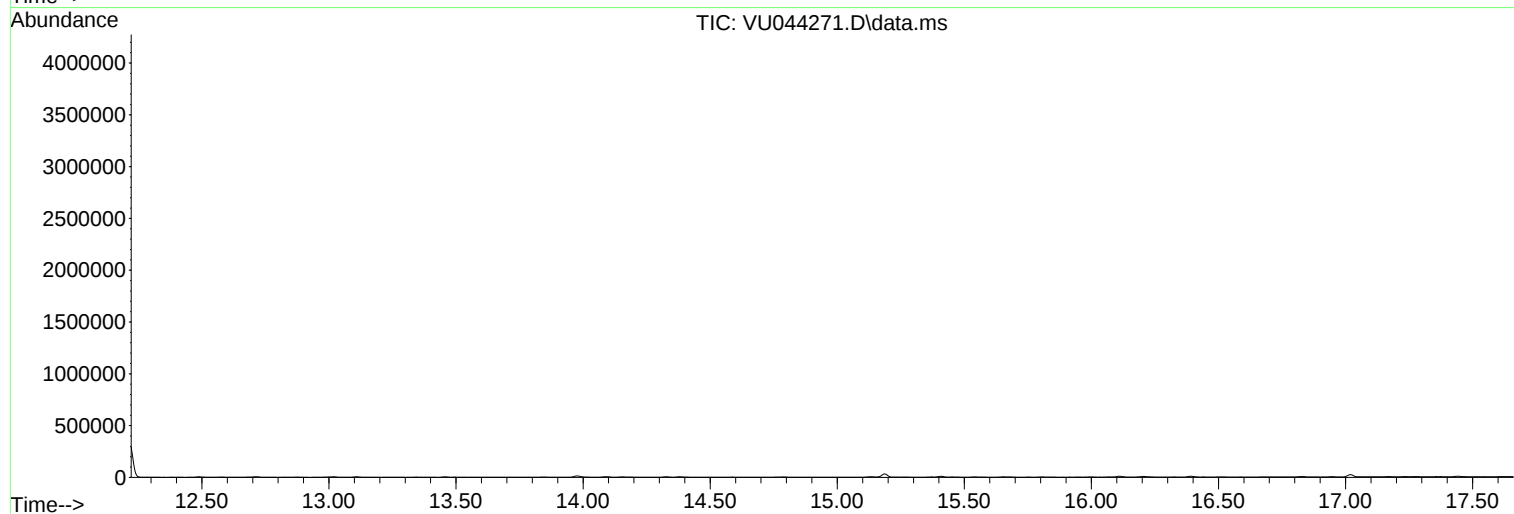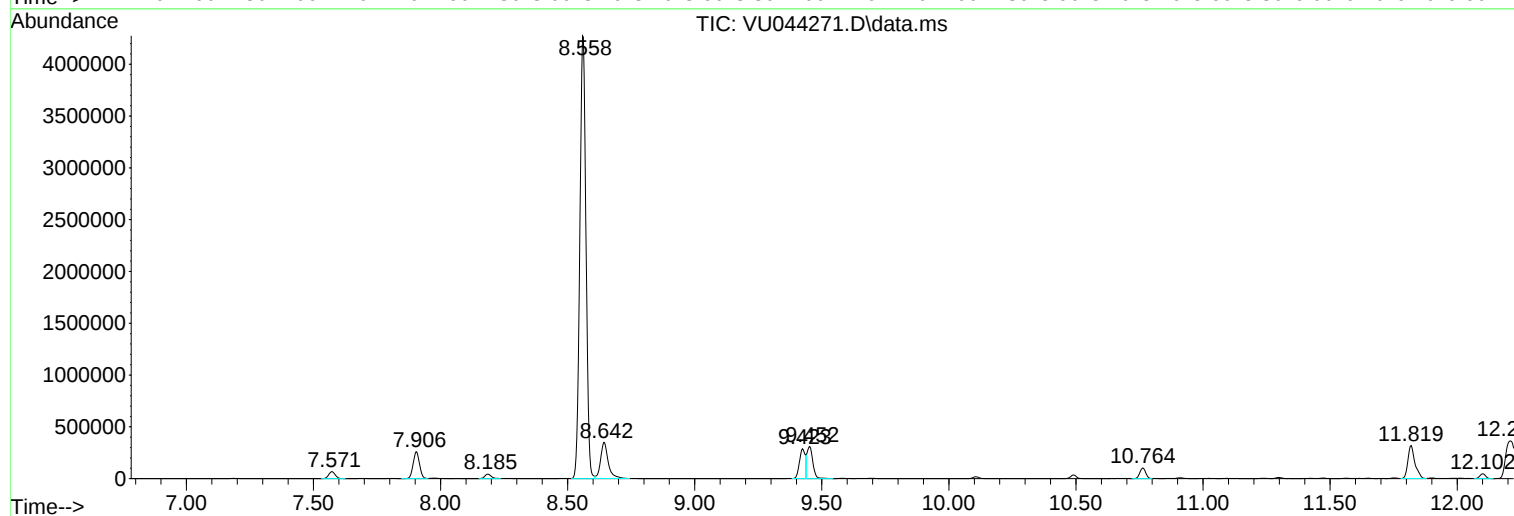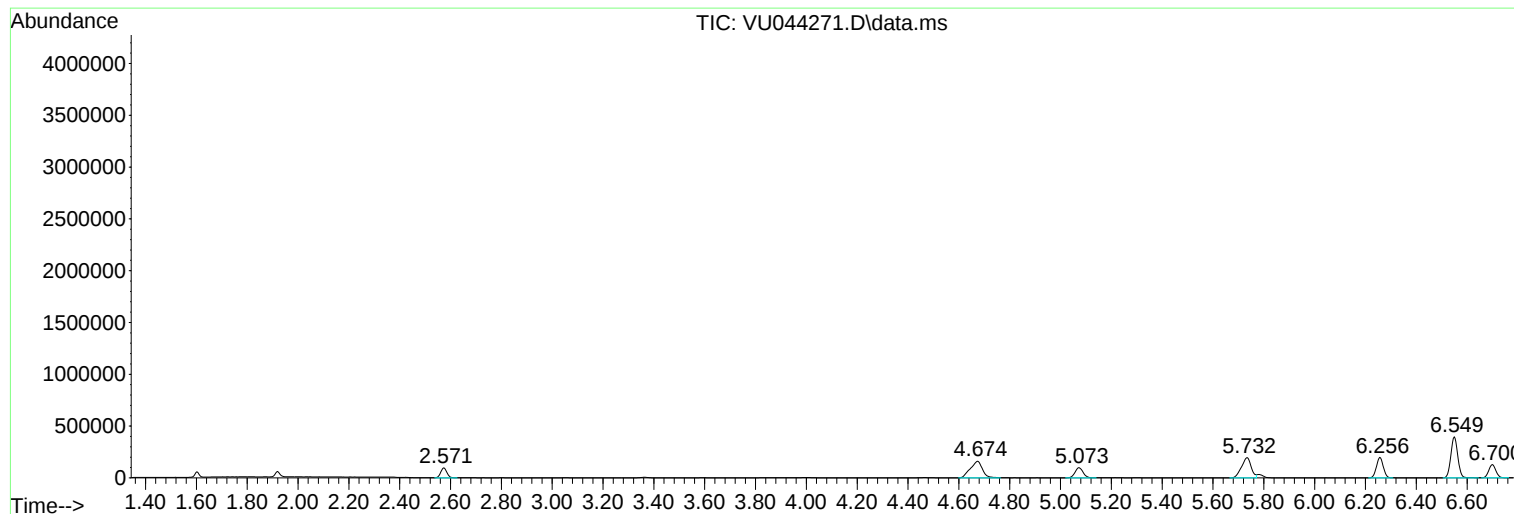

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063021\
Data File : VU044271.D
Acq On : 30 Jun 2021 19:40
Operator : SY/MD
Sample : M2905-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBK38










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR062121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Indane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.102	0.60 ug/L	72363	1,4-Dichlorobenzene-d4	11.819

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Indane			118	C9H10	000496-11-7	91
2	Indane			118	C9H10	000496-11-7	91
3	Benzene, cyclopropyl-			118	C9H10	000873-49-4	81
4	Benzene, cyclopropyl-			118	C9H10	000873-49-4	81
5	Indane			118	C9H10	000496-11-7	81

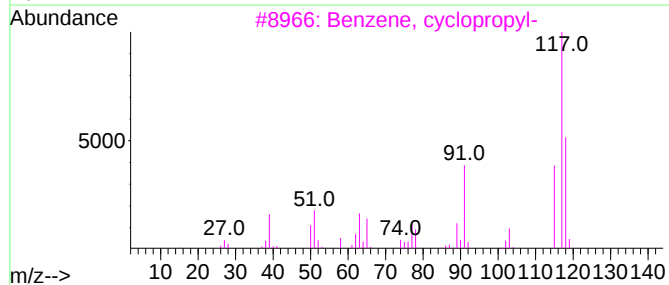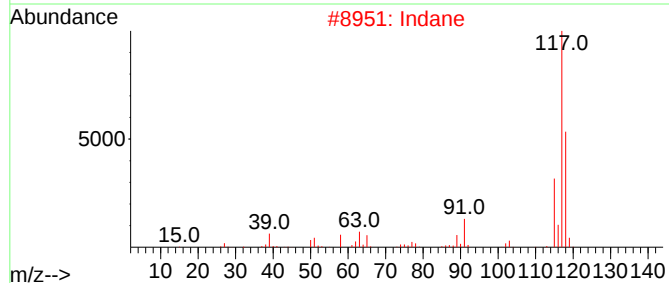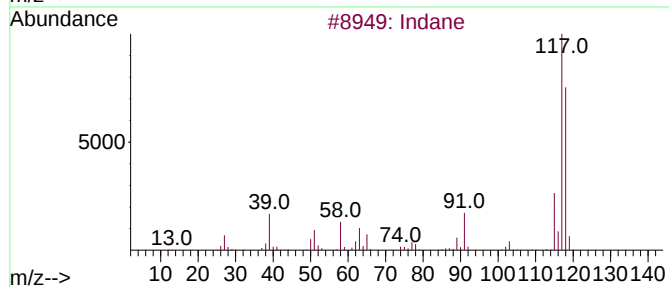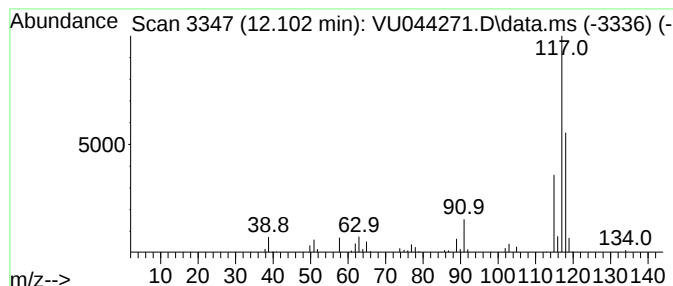

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063021\
Data File : VU044271.D
Acq On : 30 Jun 2021 19:40
Operator : SY/MD
Sample : M2905-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBK38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR062121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	12.102	0.6	ug/L	72363	3	11.819	605299	5.0