
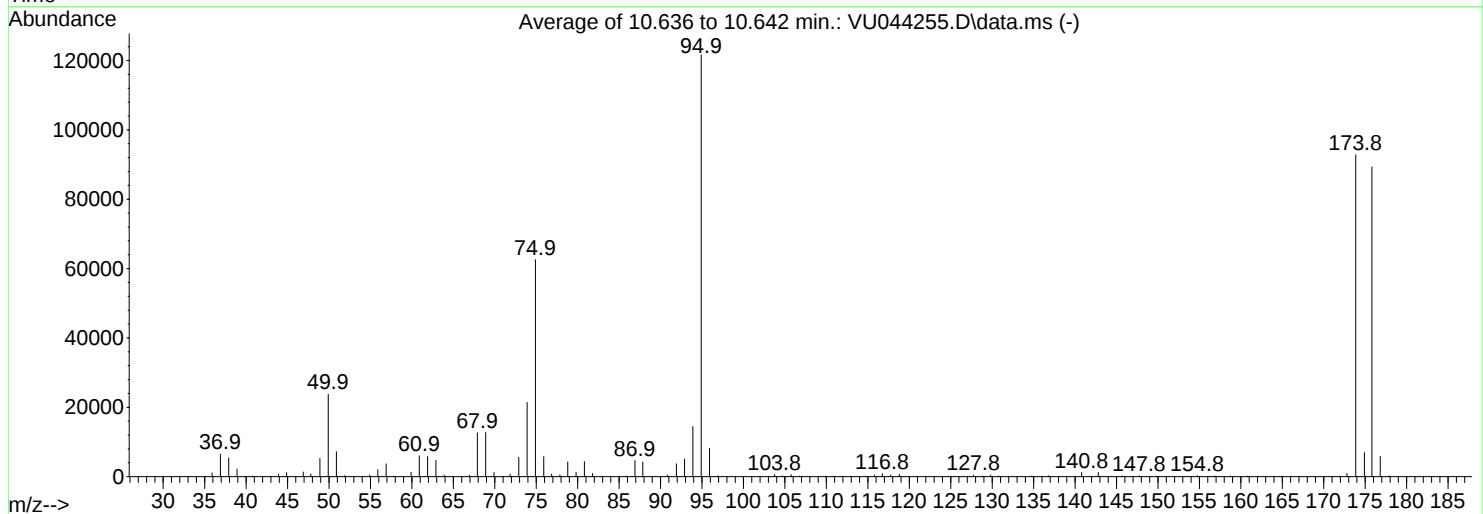


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063021\
 Data File : VU044255.D
 Acq On : 30 Jun 2021 09:19
 Operator : SY/MD
 Sample : BFB47
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB147

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR062121WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Jul 03 04:56:00 2021

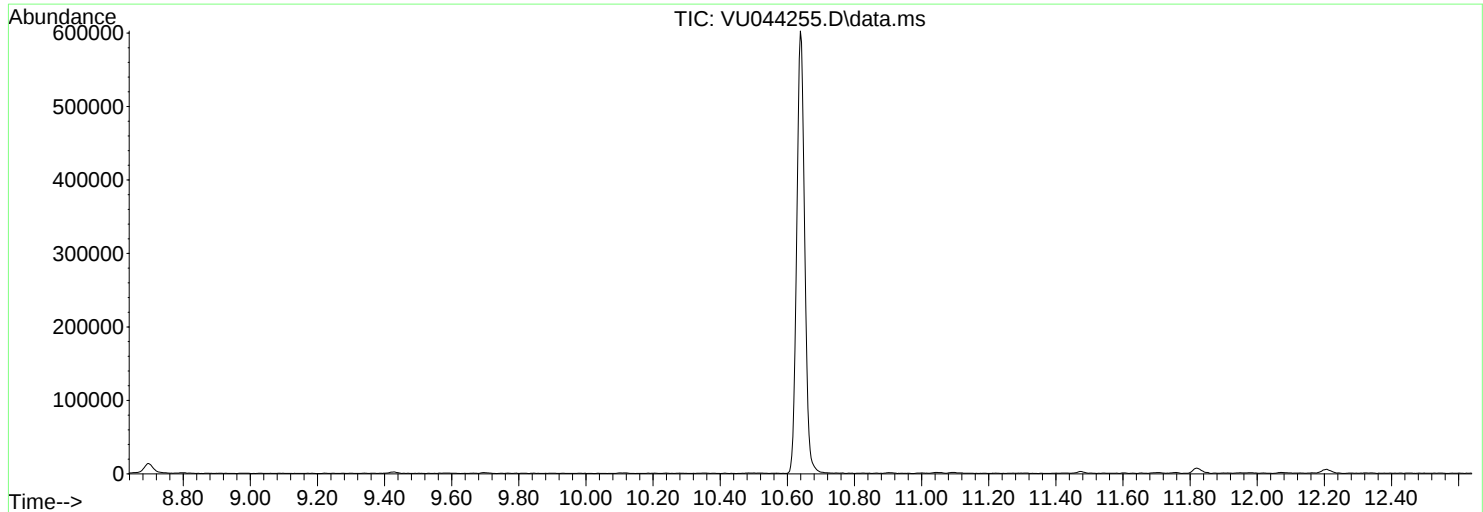

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	23763	PASS
75	95	30	80	51.4	62557	PASS
95	95	100	100	100.0	121635	PASS
96	95	5	9	6.7	8148	PASS
173	174	0.00	2	1.0	925	PASS
174	95	50	120	76.3	92853	PASS
175	174	5	9	7.5	6942	PASS
176	174	95	101	96.2	89323	PASS
177	176	5	9	6.5	5809	PASS

m/z	Abundance
35.90	1033.0
36.90	6420.0
37.90	5500.0
38.90	2183.0
39.80	169.0
40.80	155.0
42.90	196.0
43.90	1176.0
44.90	1148.0
46.90	1347.0
47.80	778.0
48.90	5138.0
49.90	23368.0
50.90	7181.0
51.90	347.0
54.90	447.0
55.90	1969.0
56.90	3732.0
57.80	103.0
59.90	1259.0
60.90	5781.0
61.90	5588.0
62.90	4596.0
63.90	483.0
67.00	327.0
67.90	12481.0
68.90	12446.0
69.90	1202.0
70.90	119.0
71.80	675.0
72.90	5579.0
73.90	21336.0
74.90	60680.0
75.90	5505.0
76.90	599.0
77.90	517.0
78.80	4064.0
79.80	1225.0
80.80	4199.0
81.80	901.0
85.90	182.0
86.90	4285.0
87.90	4169.0
90.90	445.0
91.90	3551.0
92.90	4894.0
93.90	14129.0
94.90	118208.0
95.90	7970.0
96.90	235.0
103.70	612.0
104.70	196.0
105.80	579.0
106.70	130.0
110.70	123.0
111.80	100.0
112.90	153.0
114.80	139.0
115.80	448.0
116.80	815.0
117.70	389.0
118.80	699.0
127.70	469.0
128.80	206.0
129.80	381.0
130.80	155.0
134.80	234.0
136.80	258.0
140.80	1133.0
142.80	1141.0
145.70	185.0
147.80	209.0
149.80	124.0
154.70	291.0
156.80	174.0
158.80	128.0
160.80	148.0
172.00	144.0
172.80	881.0
173.90	87824.0
174.90	6698.0
175.80	84200.0
176.80	5531.0
177.90	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
39.80	154.0
42.80	128.0
43.90	490.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
35.90	1010.0
36.90	6245.0
37.90	5143.0
38.90	2134.0
39.80	187.0
40.80	167.0
42.80	232.0
43.90	1103.0
44.90	1130.0
46.90	1329.0
47.80	742.0
48.90	5247.0
49.90	23464.0
50.90	6995.0
51.90	318.0
54.90	454.0
55.90	1926.0
56.90	3526.0
57.80	141.0
59.90	1199.0
60.90	6011.0
61.90	5823.0
62.90	4546.0
63.90	410.0
66.90	357.0
67.90	12393.0
68.90	12724.0
69.90	1146.0
71.90	709.0
72.90	5475.0
73.90	20816.0
74.90	62544.0
75.90	5740.0
76.80	725.0
77.80	520.0
78.80	4292.0
79.80	1280.0
80.80	4392.0
81.80	930.0
82.80	136.0
86.00	179.0
86.90	4913.0
87.80	4145.0
90.80	502.0
91.90	3713.0
92.90	5111.0
93.90	14229.0
94.90	121208.0
95.90	8062.0
96.90	229.0
103.80	572.0
104.80	227.0
105.70	592.0
106.80	147.0
110.70	160.0
114.80	159.0
115.80	430.0
116.70	857.0
117.80	507.0
118.80	690.0
127.80	393.0
128.80	209.0
129.80	408.0
130.70	142.0
134.80	212.0
136.80	232.0
140.80	1288.0
141.90	170.0
142.80	1255.0
145.70	196.0
147.70	228.0
148.60	100.0
149.80	118.0
154.80	274.0
156.80	232.0
158.70	131.0
160.80	167.0
171.90	156.0
172.80	936.0
173.80	95144.0
174.90	6998.0
175.80	91872.0
176.80	5921.0
177.80	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
35.90	1079.0
36.90	6737.0
37.90	5553.0
38.90	2206.0
39.80	184.0
40.80	173.0
42.90	212.0
43.90	1157.0
44.90	1173.0
46.90	1405.0
47.80	813.0
48.90	5402.0
49.90	24456.0
50.90	7438.0
51.90	357.0
54.90	479.0
55.90	2024.0
56.90	3819.0
57.80	106.0
59.90	1264.0
60.90	6218.0
61.90	5918.0
62.90	4831.0
63.90	456.0
67.00	365.0
67.90	13043.0
68.90	13064.0
69.90	1228.0
70.80	107.0
71.90	717.0
72.90	5756.0
73.90	22016.0
74.90	64448.0
75.90	6030.0
76.90	735.0
77.80	531.0
78.80	4330.0
79.80	1346.0
80.80	4435.0
81.80	968.0
82.80	119.0
85.90	210.0
86.90	4727.0
87.80	4281.0
90.90	486.0
91.90	3759.0
92.90	5194.0
93.90	14957.0
94.90	125488.0
95.90	8413.0
96.90	240.0
103.80	606.0
104.70	233.0
105.80	605.0
106.80	153.0
110.70	158.0
111.80	104.0
112.90	126.0
114.70	144.0
115.80	442.0
116.70	911.0
117.80	464.0
118.80	717.0
127.70	447.0
128.80	216.0
129.80	409.0
130.70	154.0
134.80	229.0
136.80	276.0
140.80	1241.0
141.90	143.0
142.80	1251.0
145.70	208.0
147.70	225.0
149.80	129.0
154.80	298.0
156.80	192.0
158.70	137.0
160.80	175.0
172.00	154.0
172.80	958.0
173.80	95592.0
174.90	7130.0
175.80	91896.0
176.80	5976.0
177.80	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147