


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063022\
Data File : VU049552.D
Acq On : 30 Jun 2022 09:23
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Title : SW846 8260
Last Update : Tue Jun 28 10:35:43 2022

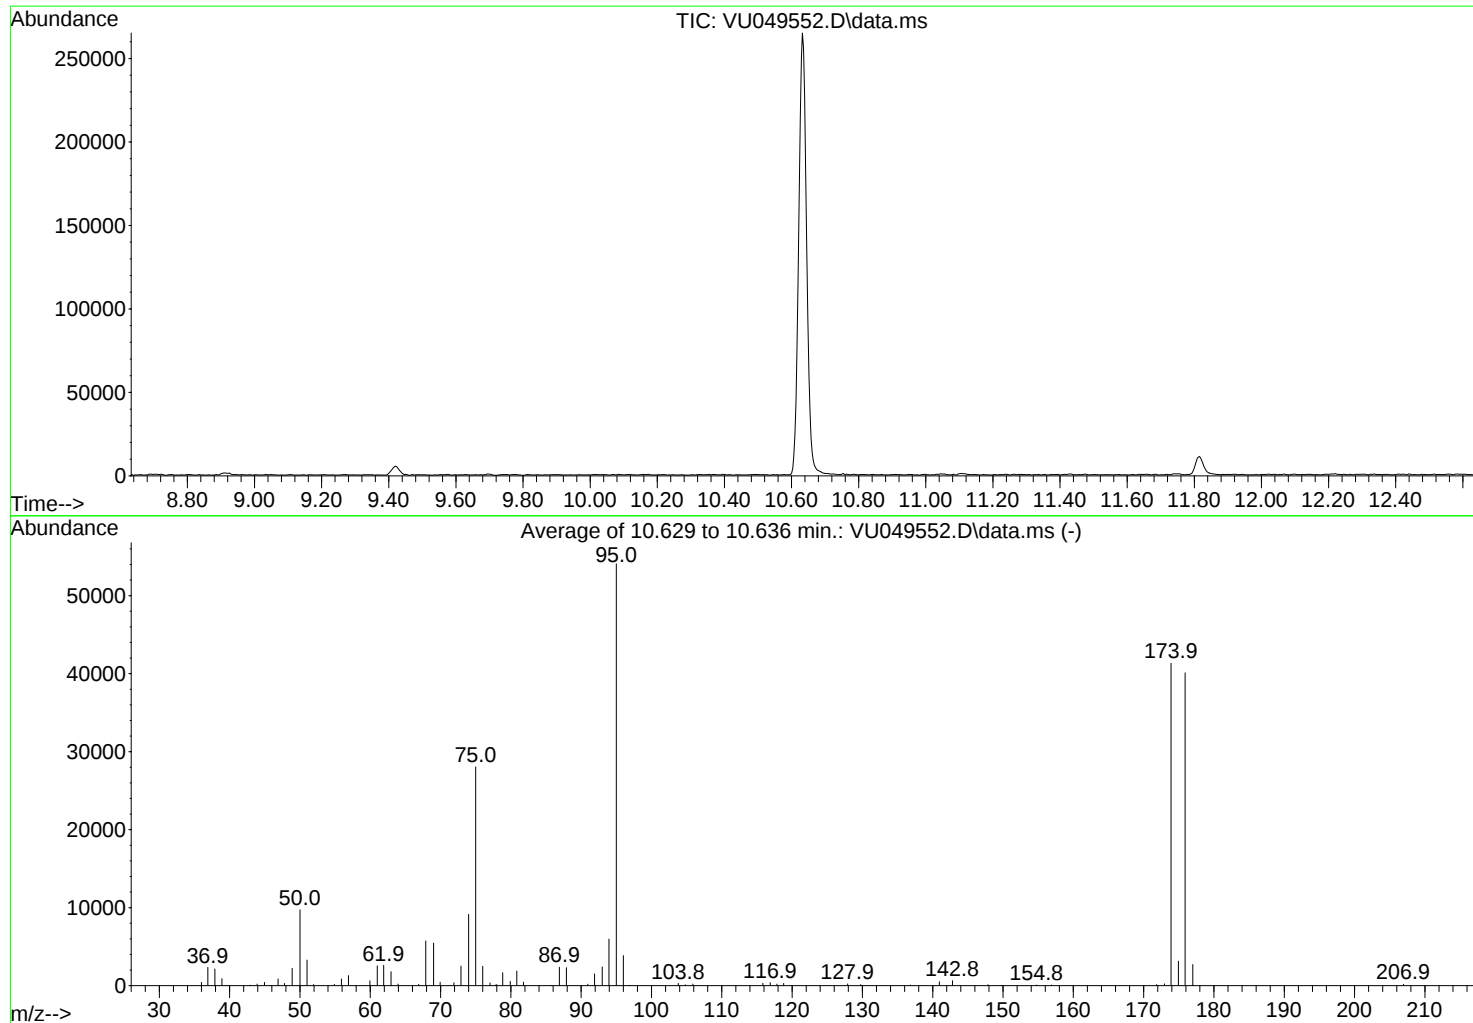

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	9723	PASS
75	95	30	60	51.9	28053	PASS
95	95	100	100	100.0	54077	PASS
96	95	5	9	7.1	3855	PASS
173	174	0.00	2	0.5	221	PASS
174	95	50	100	76.4	41331	PASS
175	174	5	9	7.6	3137	PASS
176	174	95	101	97.0	40096	PASS
177	176	5	9	6.8	2711	PASS