

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054711.D
 Acq On : 30 Jun 2023 10:36
 Operator : MD/SY
 Sample : VU0630WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK013

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054711.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	111	rVB	111071	137449	12.60%	1.679%
2	1.910	185	193	209	rBV	95438	135574	12.43%	1.656%
3	2.560	384	395	414	rVB	182727	300236	27.53%	3.667%
4	3.042	534	545	559	rBV2	13400	26601	2.44%	0.325%
5	3.181	572	588	606	rBV	38212	87858	8.06%	1.073%
6	4.627	1023	1038	1073	rBV	169373	500347	45.88%	6.110%
7	5.058	1157	1172	1196	rVB	178314	402073	36.87%	4.910%
8	5.721	1357	1378	1398	rBV3	347415	906068	83.08%	11.065%
9	6.245	1524	1541	1559	rBV	342358	663019	60.80%	8.097%
10	6.534	1620	1631	1643	rBV7	5463	11923	1.09%	0.146%
11	6.685	1664	1678	1696	rBV	225615	449226	41.19%	5.486%
12	7.563	1939	1951	1970	rBV	109909	201726	18.50%	2.464%
13	7.894	2041	2054	2077	rBV	394260	694704	63.70%	8.484%
14	8.177	2132	2142	2162	rBV	70205	123582	11.33%	1.509%
15	8.550	2246	2258	2271	rBV3	32910	60868	5.58%	0.743%
16	8.630	2271	2283	2313	rBV2	565269	1090572	100.00%	13.318%
17	9.415	2512	2527	2550	rBV	474170	807444	74.04%	9.861%
18	10.753	2931	2943	2960	rBV	176045	287757	26.39%	3.514%
19	11.807	3259	3271	3286	rBV	430538	698474	64.05%	8.530%
20	12.190	3377	3390	3410	rBV	366511	602990	55.29%	7.364%




Sum of corrected areas: 8188491

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054711.D
Acq On : 30 Jun 2023 10:36
Operator : MD/SY
Sample : VU0630WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

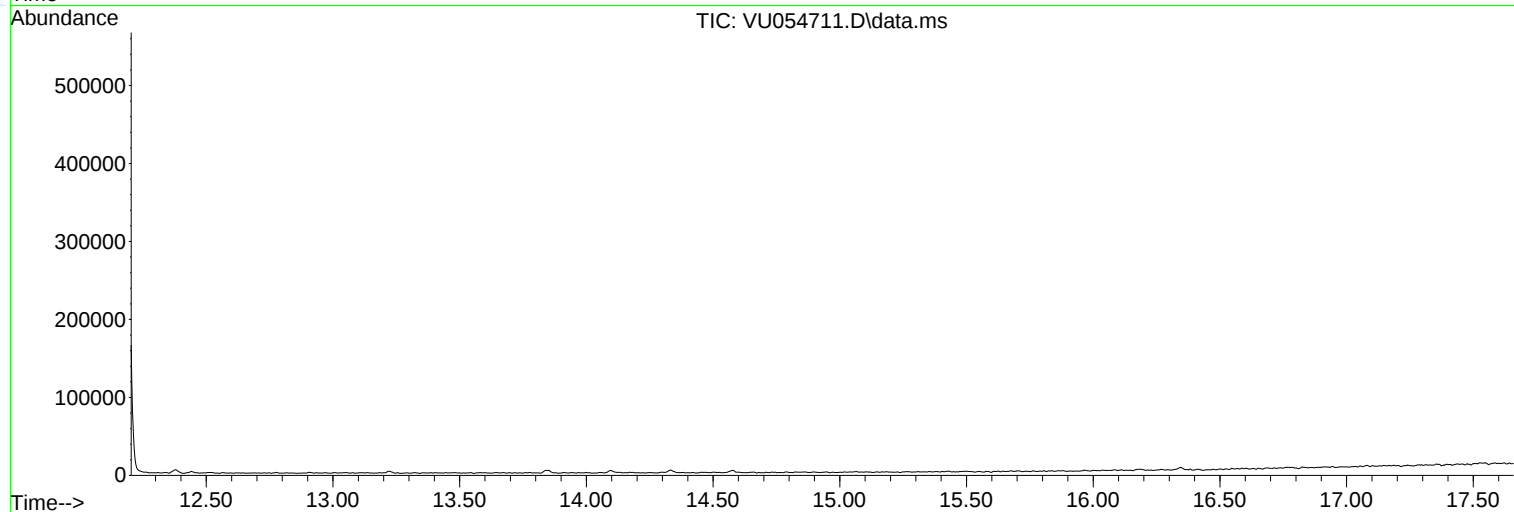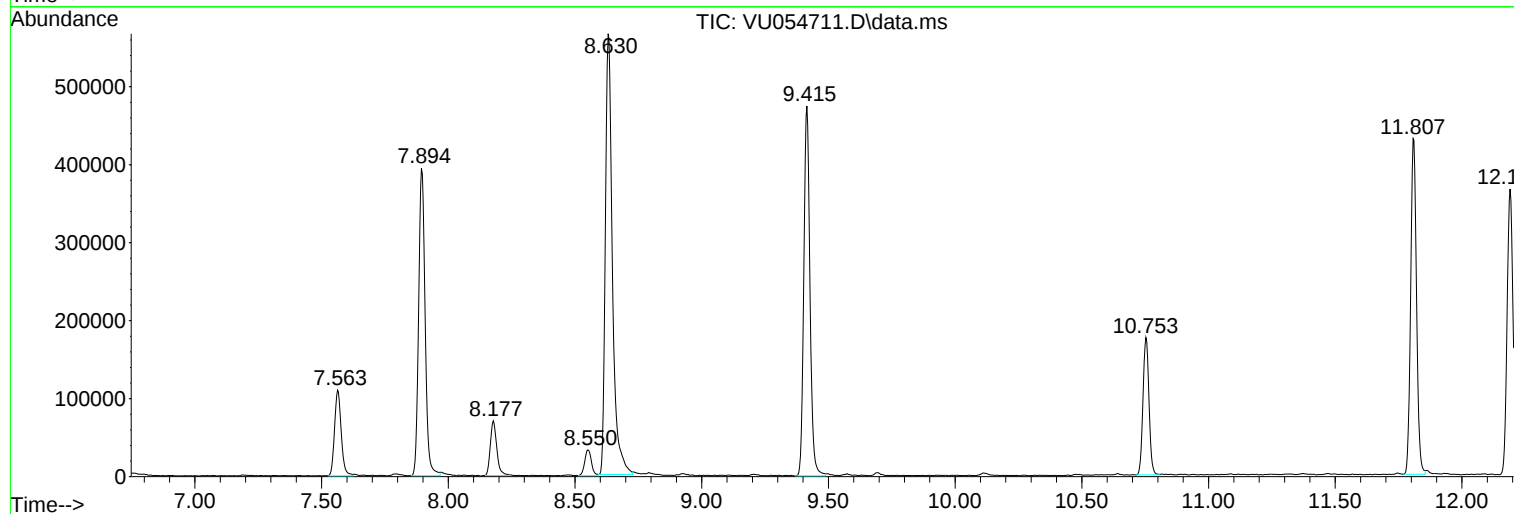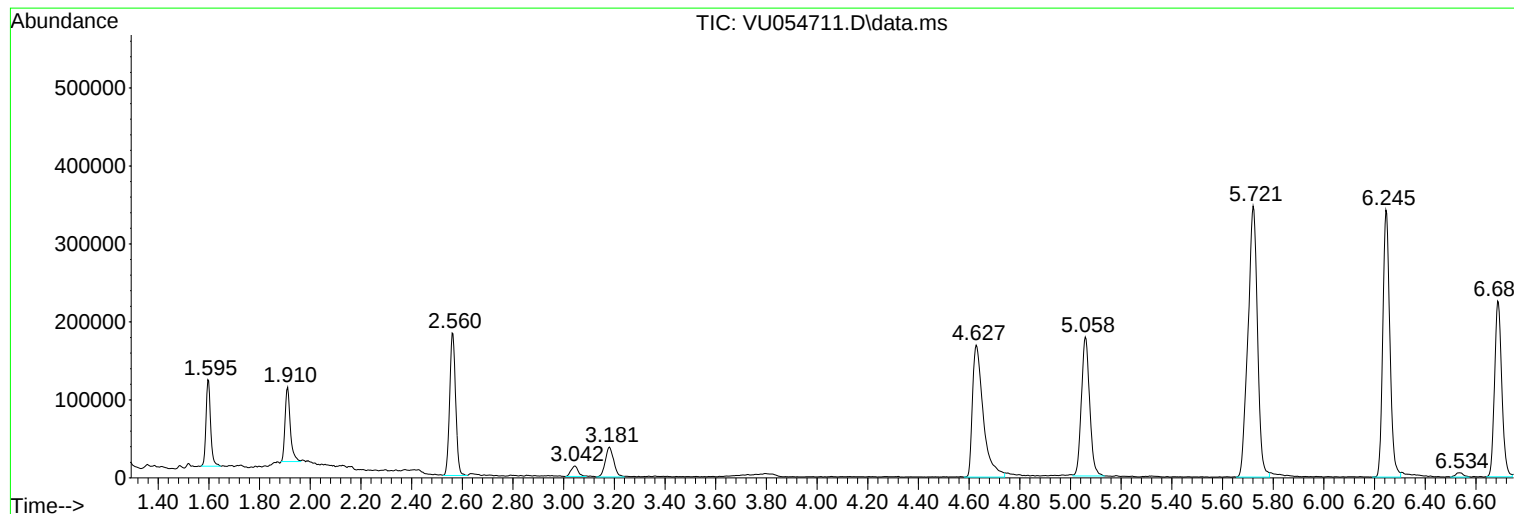

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054711.D
Acq On : 30 Jun 2023 10:36
Operator : MD/SY
Sample : VU0630WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054711.D
Acq On : 30 Jun 2023 10:36
Operator : MD/SY
Sample : VU0630WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc