

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054712.D
 Acq On : 30 Jun 2023 11:03
 Operator : MD/SY
 Sample : 03477-07DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HOA45DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	109	rBV	108808	133210	8.62%	1.341%
2	1.907	185	192	210	rBV	91754	128324	8.31%	1.292%
3	2.563	384	396	413	rVB2	180512	304125	19.68%	3.062%
4	3.039	532	544	562	rVB2	10784	23067	1.49%	0.232%
5	3.181	573	588	608	rVB2	43454	100253	6.49%	1.009%
6	4.627	1021	1038	1085	rBV	165481	514017	33.27%	5.175%
7	5.058	1156	1172	1191	rVB2	162557	365283	23.64%	3.678%
8	5.312	1238	1251	1267	rVB3	24930	56938	3.69%	0.573%
9	5.721	1358	1378	1412	rBV2	323832	867554	56.15%	8.734%
10	6.245	1524	1541	1564	rBV	402678	793182	51.34%	7.986%
11	6.537	1616	1632	1648	rBV3	43969	86569	5.60%	0.872%
12	6.685	1662	1678	1696	rBV	214376	426154	27.58%	4.290%
13	7.563	1938	1951	1969	rBV	102227	186762	12.09%	1.880%
14	7.894	2041	2054	2074	rBV	372438	648064	41.94%	6.525%
15	8.177	2130	2142	2158	rBV	63589	112578	7.29%	1.133%
16	8.550	2245	2258	2273	rBV	898596	1545098	100.00%	15.556%
17	8.630	2273	2283	2313	rVB2	528327	1021121	66.09%	10.281%
18	9.415	2514	2527	2553	rBV	567277	956538	61.91%	9.630%
19	10.753	2931	2943	2964	rBV2	161602	265543	17.19%	2.673%
20	11.807	3259	3271	3294	rBV	516867	840809	54.42%	8.465%
21	12.190	3377	3390	3405	rBV	336325	557328	36.07%	5.611%




Sum of corrected areas: 9932517

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054712.D
Acq On : 30 Jun 2023 11:03
Operator : MD/SY
Sample : 03477-07DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

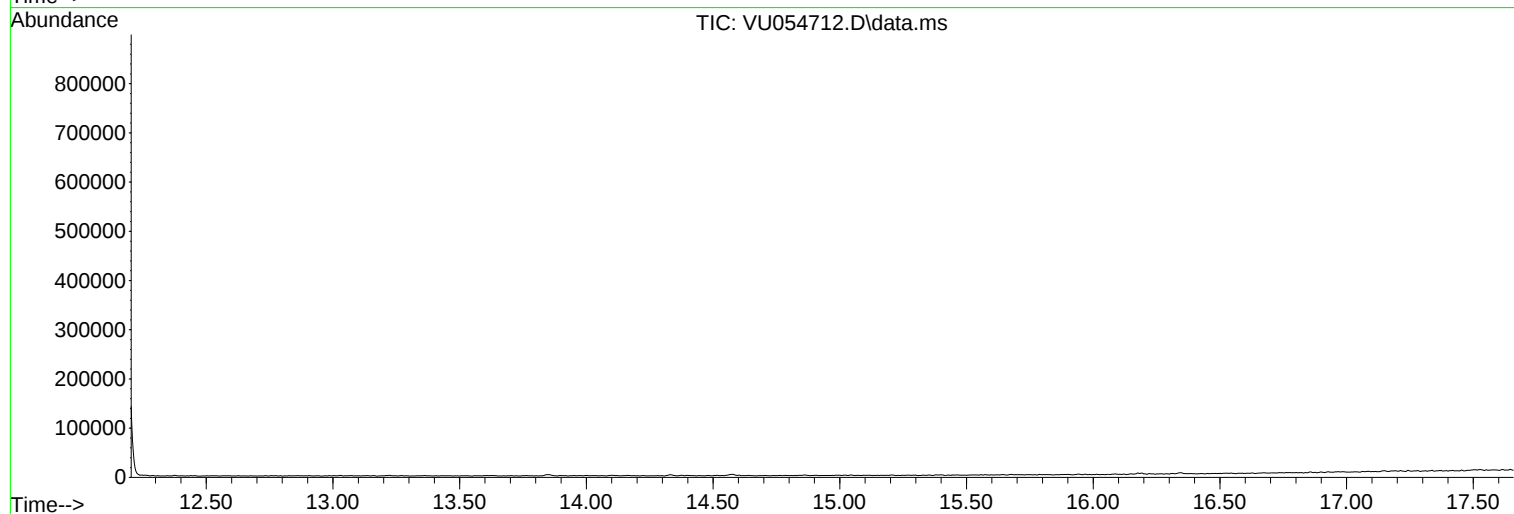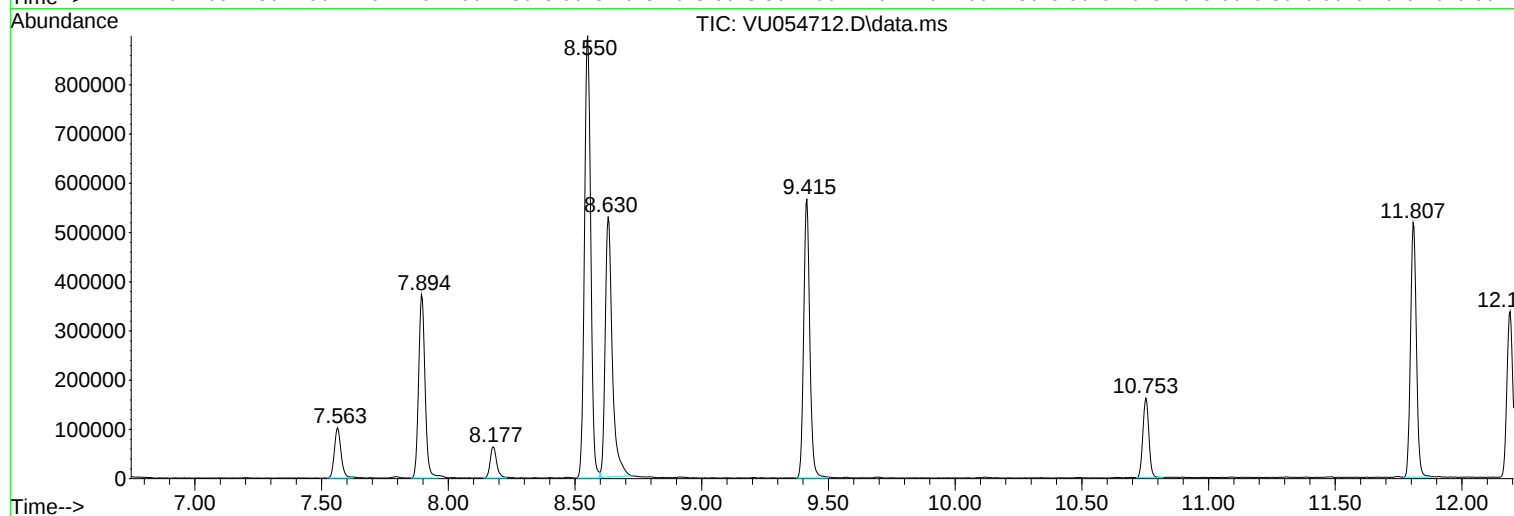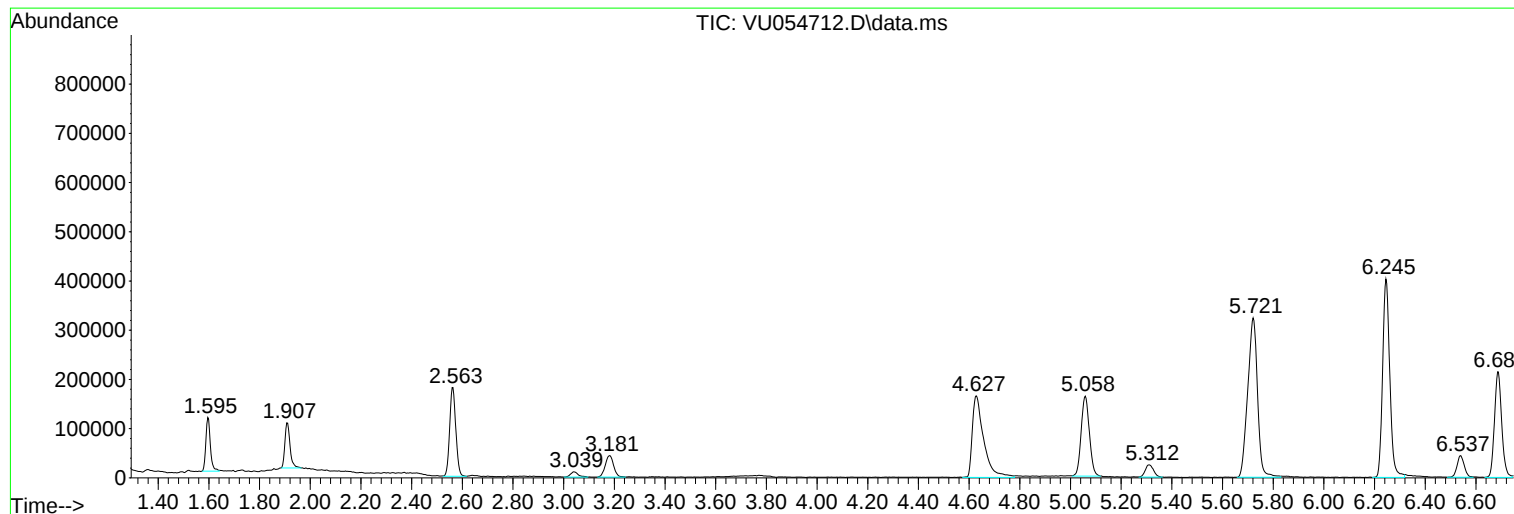

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054712.D
Acq On : 30 Jun 2023 11:03
Operator : MD/SY
Sample : 03477-07DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054712.D
Acq On : 30 Jun 2023 11:03
Operator : MD/SY
Sample : 03477-07DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------