

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054713.D
 Acq On : 30 Jun 2023 11:27
 Operator : MD/SY
 Sample : 03477-09DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HOA47DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	108	rVB	101607	123461	6.59%	1.229%
2	1.911	185	193	211	rVB	92370	130099	6.94%	1.295%
3	2.563	383	396	411	rBV2	180487	309752	16.53%	3.084%
4	3.039	535	544	558	rBV3	13101	23200	1.24%	0.231%
5	3.184	572	589	606	rBV2	35166	79689	4.25%	0.793%
6	4.624	1020	1037	1076	rBV	175238	509151	27.17%	5.069%
7	5.058	1157	1172	1192	rBV	166117	393968	21.02%	3.922%
8	5.312	1239	1251	1264	rVB3	12740	26486	1.41%	0.264%
9	5.721	1359	1378	1408	rBV3	318600	850680	45.39%	8.469%
10	6.245	1526	1541	1564	rBV	346839	674570	35.99%	6.716%
11	6.537	1617	1632	1647	rBV	147428	286505	15.29%	2.852%
12	6.685	1665	1678	1697	rBV2	214444	417977	22.30%	4.161%
13	7.563	1939	1951	1969	rBV	99831	185178	9.88%	1.844%
14	7.894	2038	2054	2072	rBV	363699	644269	34.38%	6.414%
15	8.177	2128	2142	2160	rBV	64871	113944	6.08%	1.134%
16	8.550	2244	2258	2273	rBV	1103214	1874082	100.00%	18.657%
17	8.631	2273	2283	2317	rVB2	546252	1062352	56.69%	10.576%
18	9.415	2513	2527	2546	rBV	466955	809251	43.18%	8.056%
19	10.753	2930	2943	2959	rBV	165456	270158	14.42%	2.690%
20	11.807	3260	3271	3286	rBV	431567	694377	37.05%	6.913%
21	12.190	3375	3390	3413	rBV	338546	565672	30.18%	5.631%




Sum of corrected areas: 10044821

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054713.D
Acq On : 30 Jun 2023 11:27
Operator : MD/SY
Sample : 03477-09DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA47DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

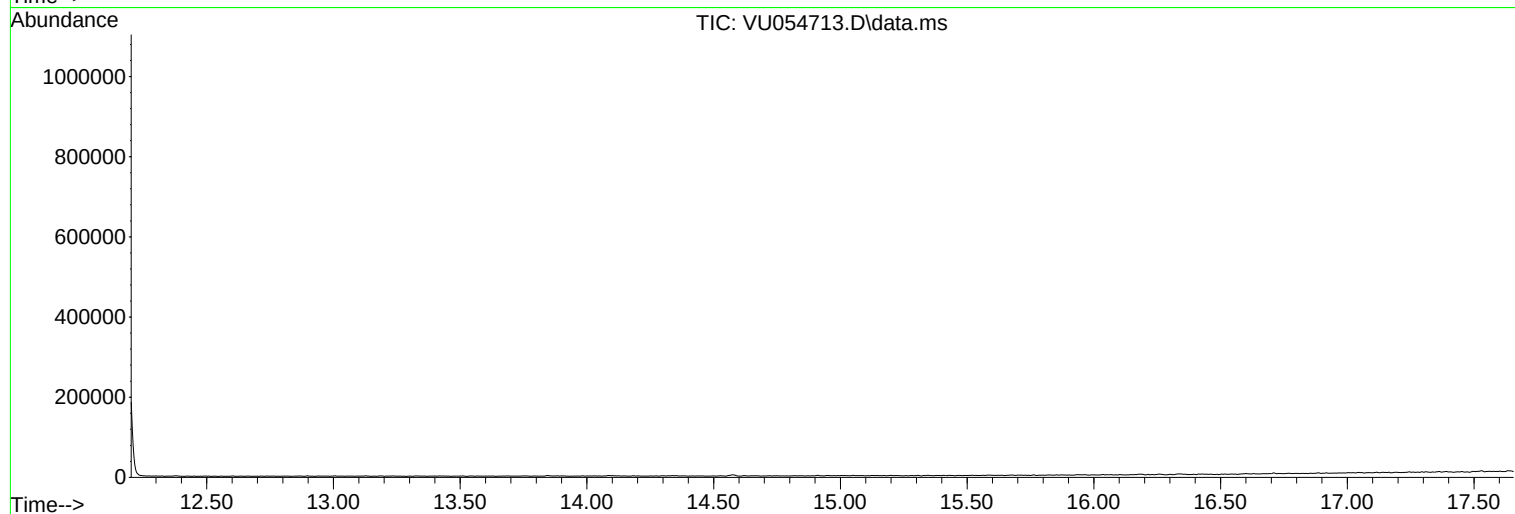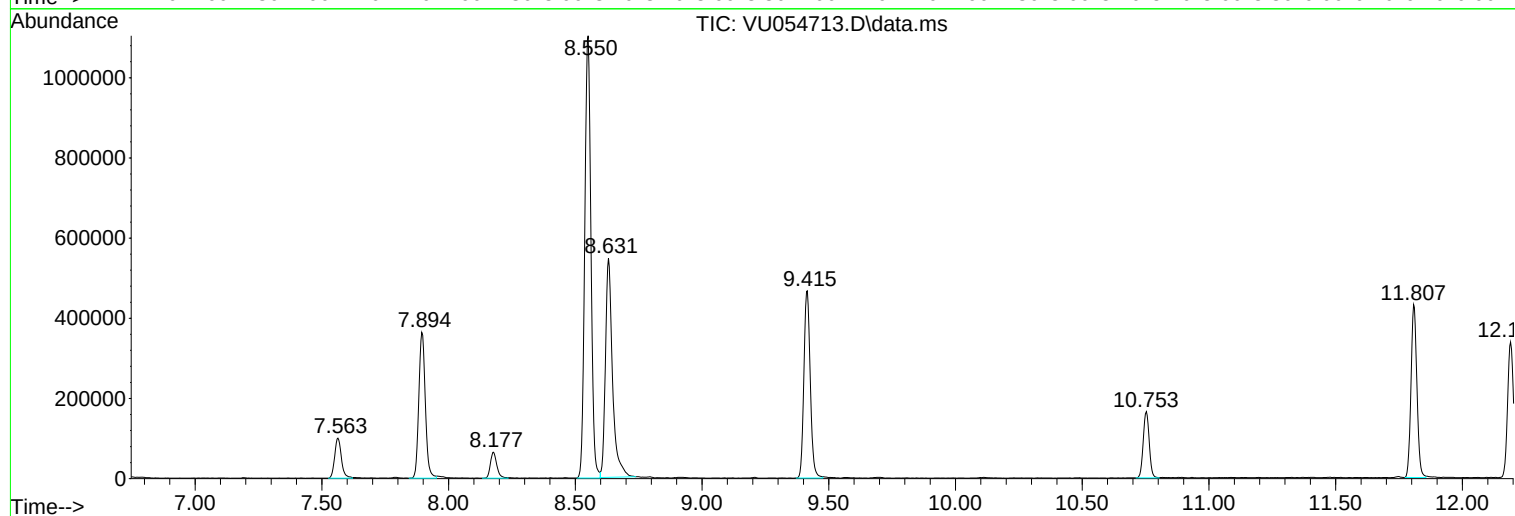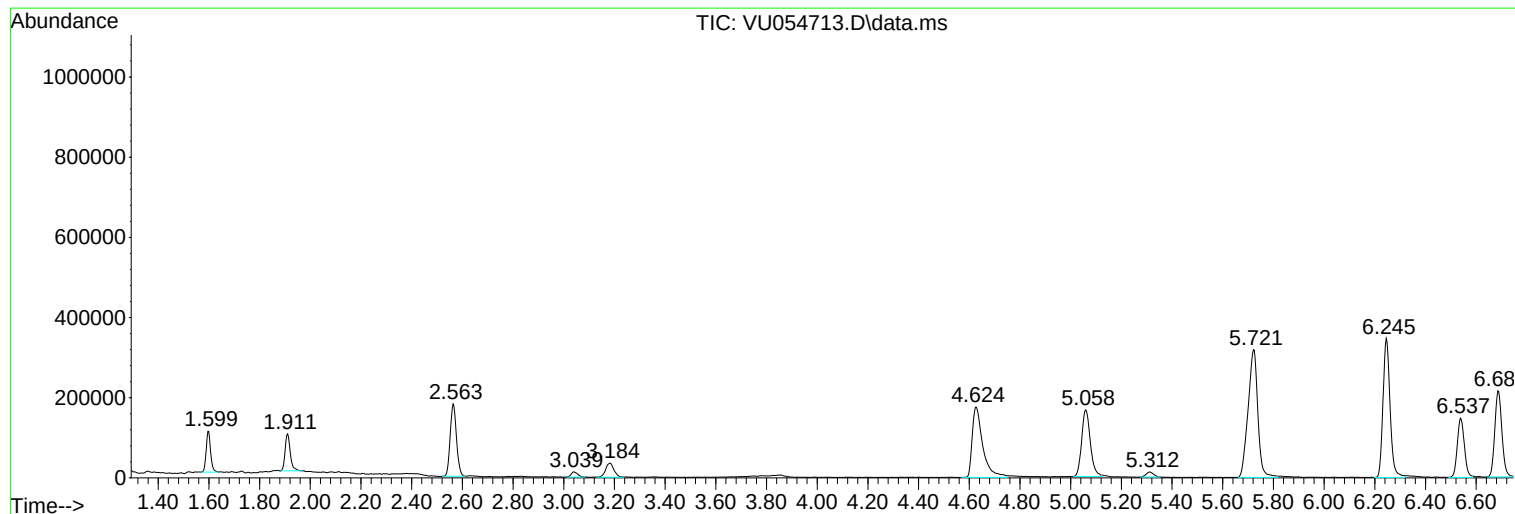

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054713.D
Acq On : 30 Jun 2023 11:27
Operator : MD/SY
Sample : 03477-09DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA47DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054713.D
Acq On : 30 Jun 2023 11:27
Operator : MD/SY
Sample : 03477-09DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA47DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc