

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054714.D
 Acq On : 30 Jun 2023 11:51
 Operator : MD/SY
 Sample : 03477-02DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HOA42DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054714.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	110	rBV	102697	123880	6.91%	1.274%
2	1.907	185	192	215	rVB	94443	149446	8.34%	1.537%
3	2.563	383	396	411	rBV2	182776	329644	18.40%	3.391%
4	3.181	573	588	609	rBV	16215	37599	2.10%	0.387%
5	4.624	1024	1037	1071	rBV	165289	453168	25.29%	4.662%
6	5.058	1157	1172	1196	rVB	167508	377721	21.08%	3.886%
7	5.721	1357	1378	1402	rBV2	321216	849118	47.39%	8.735%
8	6.245	1526	1541	1566	rBV	340372	664940	37.11%	6.840%
9	6.537	1619	1632	1650	rBV2	114085	221188	12.34%	2.275%
10	6.685	1665	1678	1698	rBV	211239	417343	23.29%	4.293%
11	7.563	1938	1951	1968	rBV2	101464	187398	10.46%	1.928%
12	7.894	2041	2054	2072	rBV	368931	646919	36.10%	6.655%
13	8.177	2129	2142	2166	rBV	64840	116013	6.47%	1.193%
14	8.550	2244	2258	2273	rBV	1064033	1791848	100.00%	18.432%
15	8.630	2273	2283	2317	rVB2	539332	1042404	58.17%	10.723%
16	9.415	2514	2527	2548	rBV	468680	799647	44.63%	8.226%
17	10.753	2927	2943	2960	rBV	166114	268558	14.99%	2.763%
18	11.807	3259	3271	3299	rBV	428720	693869	38.72%	7.138%
19	12.190	3377	3390	3408	rBV	332157	550449	30.72%	5.662%




Sum of corrected areas: 9721152

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054714.D
Acq On : 30 Jun 2023 11:51
Operator : MD/SY
Sample : 03477-02DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA42DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

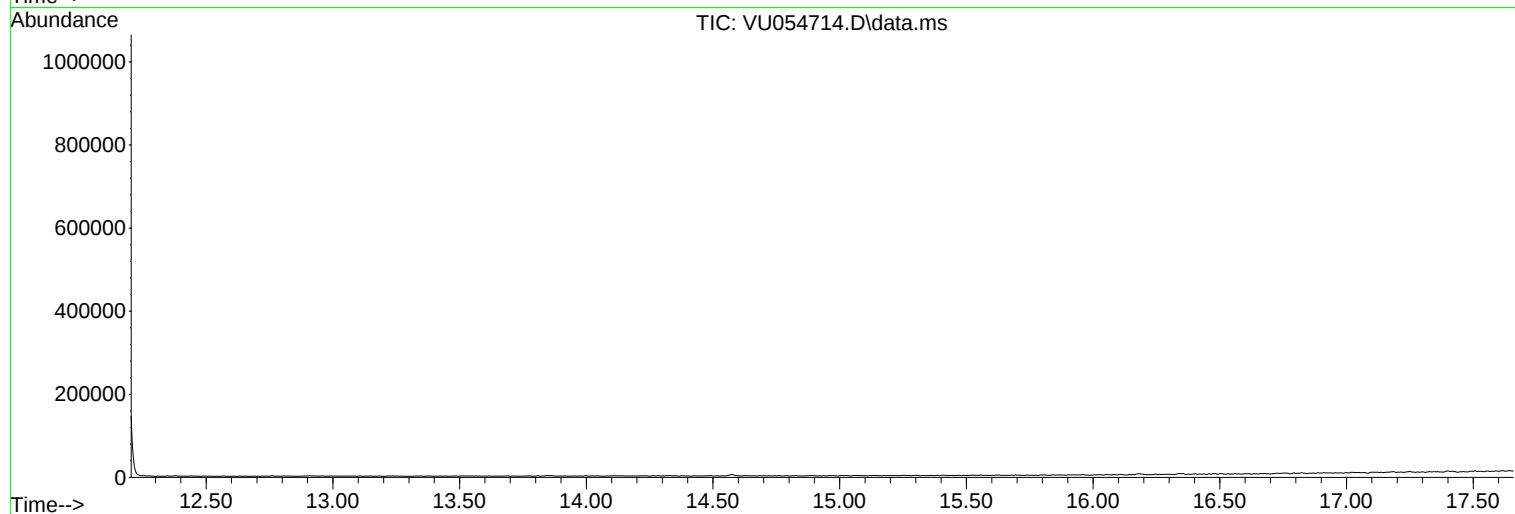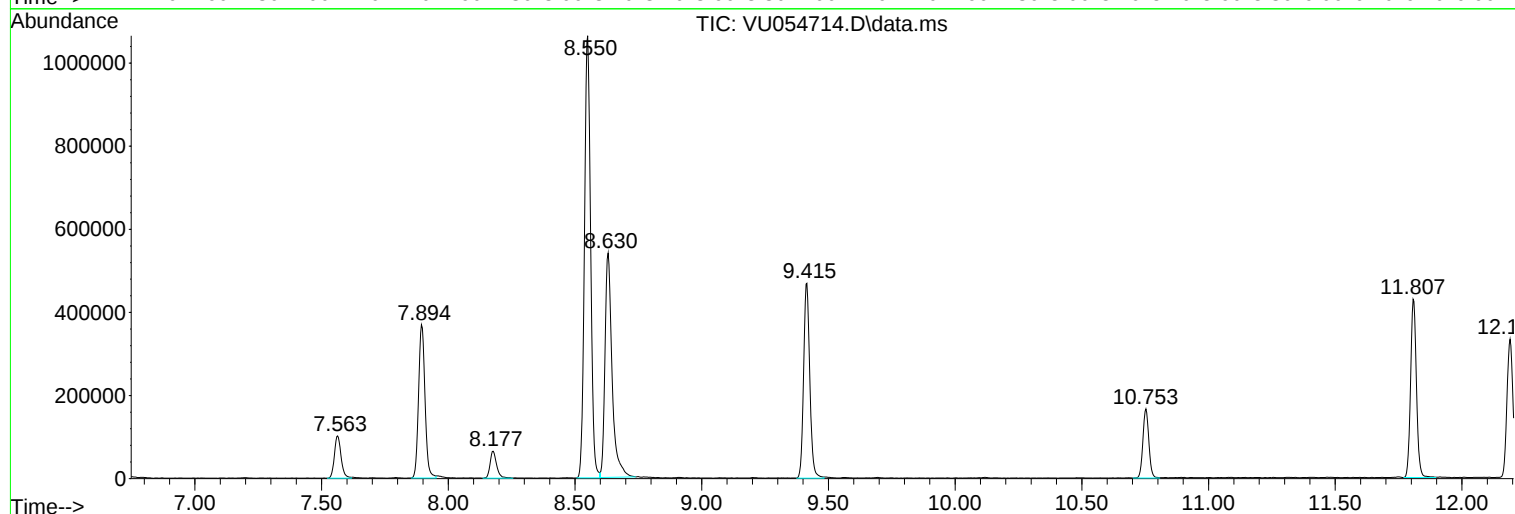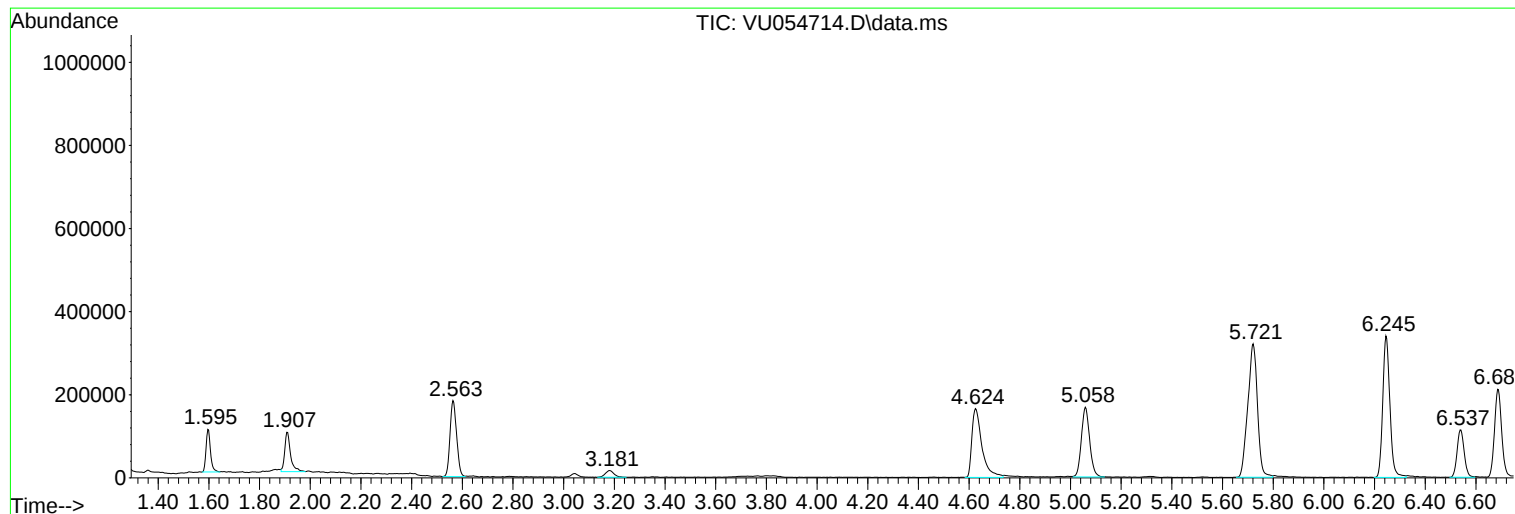

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054714.D
Acq On : 30 Jun 2023 11:51
Operator : MD/SY
Sample : 03477-02DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA42DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054714.D
Acq On : 30 Jun 2023 11:51
Operator : MD/SY
Sample : 03477-02DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA42DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc