

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054715.D
 Acq On : 30 Jun 2023 12:16
 Operator : MD/SY
 Sample : 03477-06DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HOA44DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054715.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	109	rBV	99836	120984	6.49%	1.236%
2	1.907	184	192	210	rVB	93322	144298	7.75%	1.474%
3	2.563	384	396	413	rBV2	188331	337309	18.11%	3.445%
4	3.181	576	588	605	rVB	22915	53117	2.85%	0.543%
5	4.624	1023	1037	1084	rBV	163670	462329	24.82%	4.722%
6	5.058	1156	1172	1190	rVB	160440	362913	19.48%	3.707%
7	5.721	1355	1378	1398	rBV2	312297	828263	44.46%	8.460%
8	6.245	1528	1541	1563	rBV	345161	671780	36.06%	6.861%
9	6.538	1620	1632	1648	rBV	119099	228755	12.28%	2.336%
10	6.689	1664	1679	1701	rBV	209210	414393	22.25%	4.233%
11	7.563	1939	1951	1966	rBV2	104340	183183	9.83%	1.871%
12	7.894	2041	2054	2075	rBV	357891	633902	34.03%	6.475%
13	8.177	2130	2142	2160	rBV	63518	112275	6.03%	1.147%
14	8.550	2244	2258	2273	rBV	1099415	1862750	100.00%	19.026%
15	8.631	2273	2283	2324	rVB2	524269	1026806	55.12%	10.488%
16	9.415	2512	2527	2551	rBV	484120	821116	44.08%	8.387%
17	10.753	2931	2943	2957	rBV	164935	264771	14.21%	2.704%
18	11.807	3259	3271	3297	rBV	435467	709913	38.11%	7.251%
19	12.190	3377	3390	3410	rBV	333096	551869	29.63%	5.637%




Sum of corrected areas: 9790726

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054715.D
Acq On : 30 Jun 2023 12:16
Operator : MD/SY
Sample : 03477-06DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

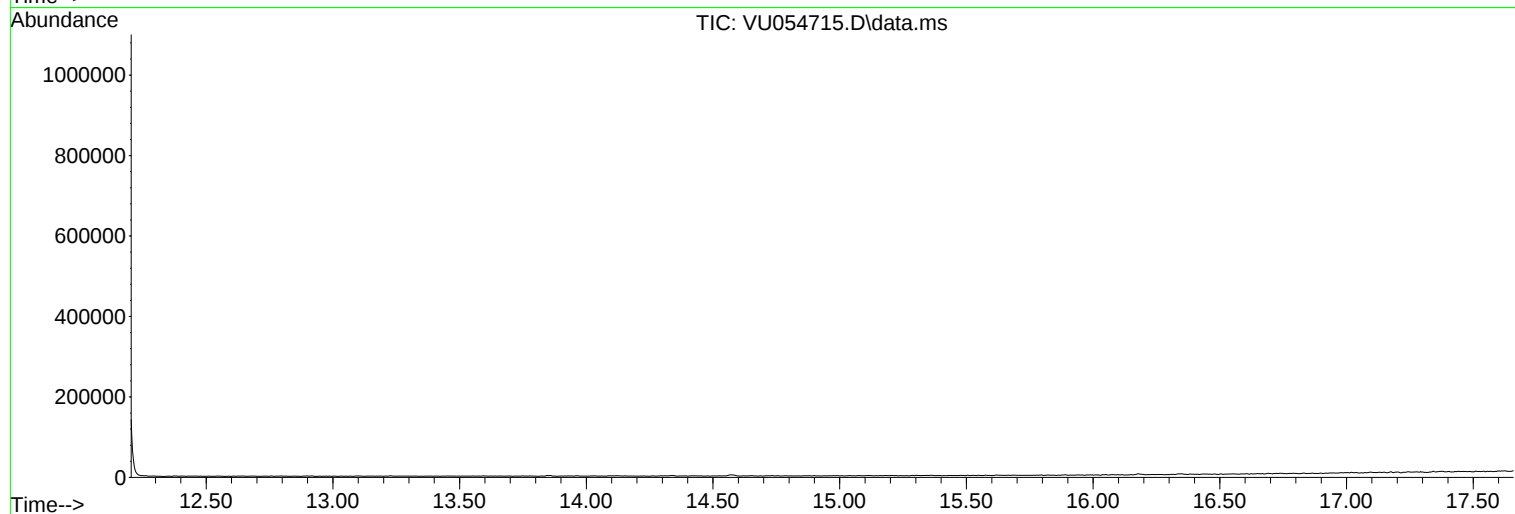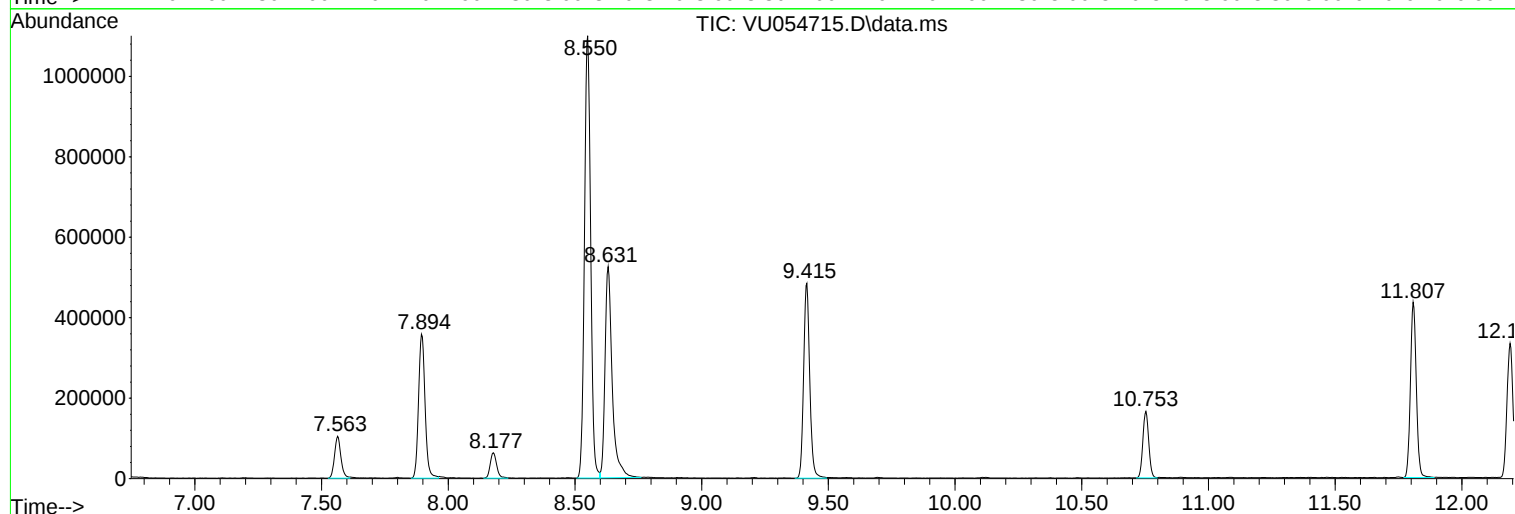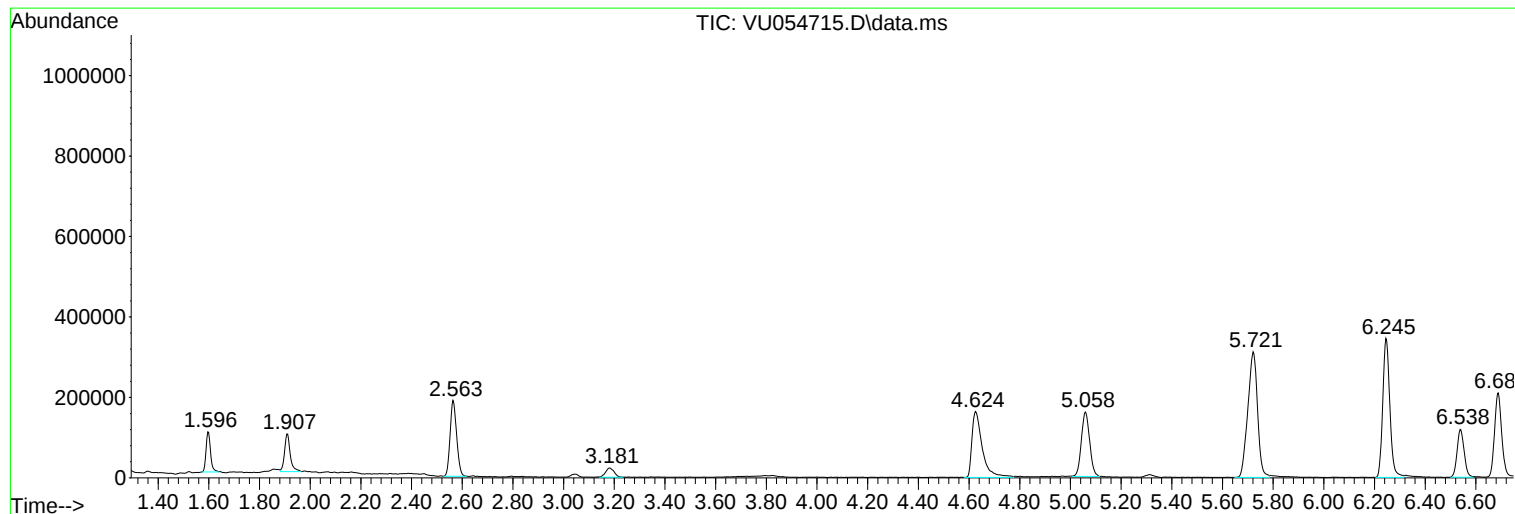

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054715.D
Acq On : 30 Jun 2023 12:16
Operator : MD/SY
Sample : 03477-06DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054715.D
Acq On : 30 Jun 2023 12:16
Operator : MD/SY
Sample : 03477-06DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc