

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054716.D
 Acq On : 30 Jun 2023 12:39
 Operator : MD/SY
 Sample : 03477-01DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HOA41DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054716.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	112	rVB	96606	120707	8.10%	1.308%
2	1.907	185	192	204	rVB	85452	117413	7.88%	1.273%
3	2.563	384	396	412	rVB2	169547	297610	19.98%	3.226%
4	3.039	535	544	558	rVB4	7855	16252	1.09%	0.176%
5	3.181	576	588	603	rVB2	9627	21074	1.41%	0.228%
6	4.624	1023	1037	1066	rBV	155451	412754	27.71%	4.474%
7	5.058	1156	1172	1198	rVB	157542	363838	24.42%	3.944%
8	5.721	1357	1378	1403	rBV2	308059	812072	54.52%	8.803%
9	6.245	1528	1541	1569	rBV	360568	704417	47.29%	7.636%
10	6.537	1620	1632	1647	rBV	91254	176911	11.88%	1.918%
11	6.685	1663	1678	1705	rBV	206598	408459	27.42%	4.428%
12	7.563	1939	1951	1965	rBV	99059	175144	11.76%	1.899%
13	7.894	2041	2054	2074	rBV	345064	612023	41.09%	6.634%
14	8.177	2128	2142	2160	rBV2	60577	107673	7.23%	1.167%
15	8.550	2244	2258	2272	rBV	878906	1489624	100.00%	16.148%
16	8.631	2272	2283	2320	rVB2	514860	998574	67.04%	10.825%
17	9.412	2512	2526	2548	rBV	494910	848907	56.99%	9.202%
18	10.753	2928	2943	2960	rBV	157606	262449	17.62%	2.845%
19	11.807	3259	3271	3293	rBV	463777	743376	49.90%	8.058%
20	12.190	3376	3390	3407	rBV	329237	535616	35.96%	5.806%




Sum of corrected areas: 9224893

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054716.D
Acq On : 30 Jun 2023 12:39
Operator : MD/SY
Sample : 03477-01DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA41DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

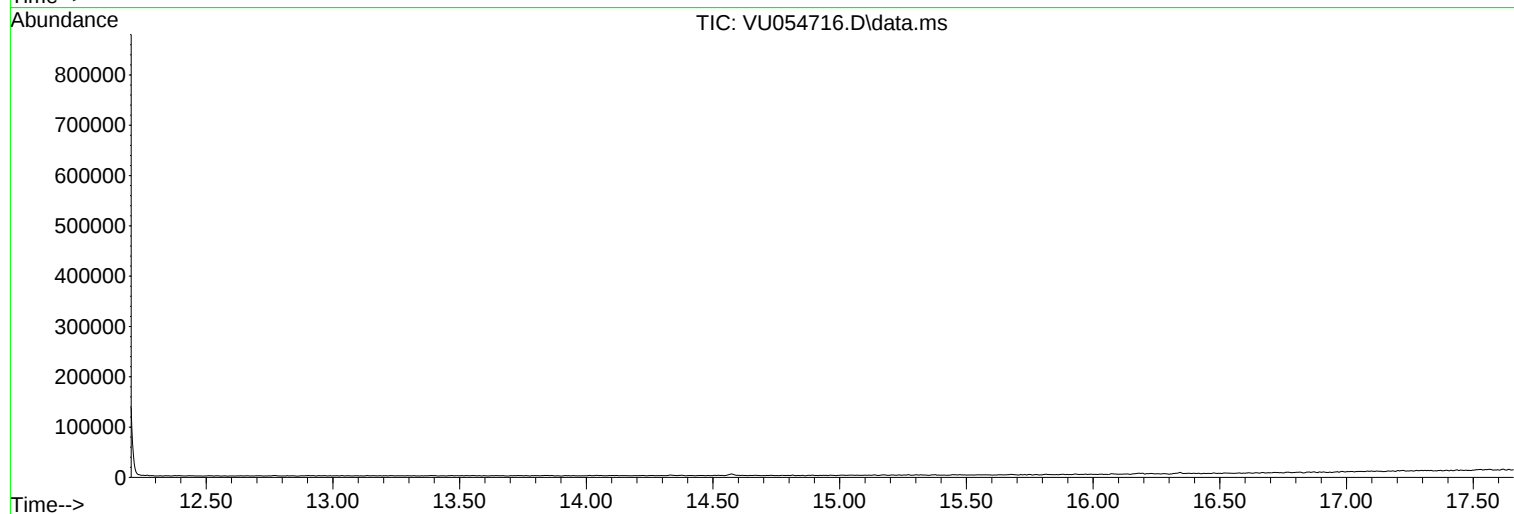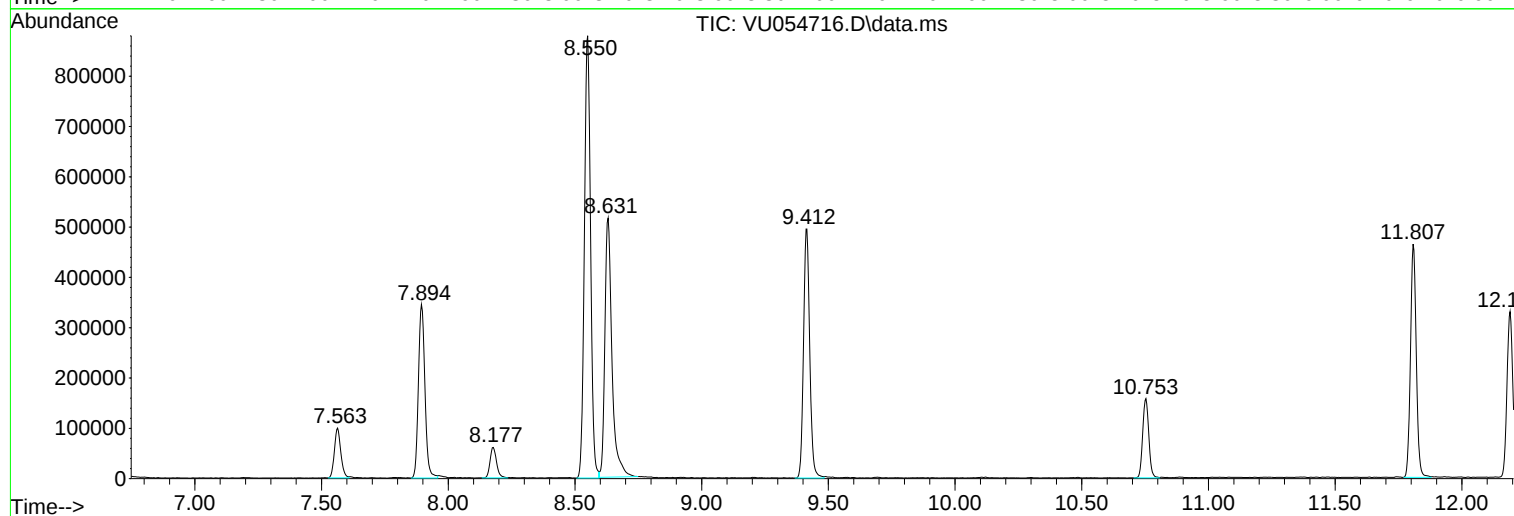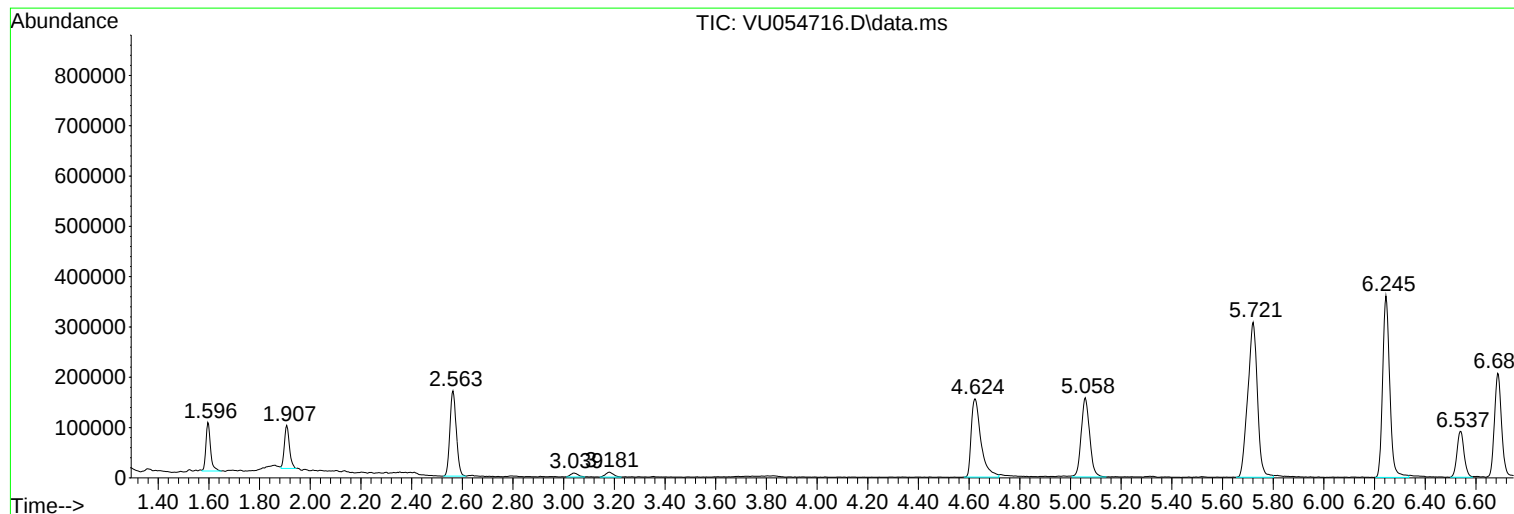

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054716.D
Acq On : 30 Jun 2023 12:39
Operator : MD/SY
Sample : 03477-01DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA41DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054716.D
Acq On : 30 Jun 2023 12:39
Operator : MD/SY
Sample : 03477-01DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA41DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------