

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054717.D
 Acq On : 30 Jun 2023 13:04
 Operator : MD/SY
 Sample : 03477-05DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HOA43DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	112	rBV	100484	124602	9.77%	1.327%
2	1.907	184	192	207	rVB	95427	138049	10.83%	1.470%
3	2.560	382	395	411	rVB	167853	275015	21.57%	2.929%
4	3.042	536	545	555	rVB3	7486	13102	1.03%	0.140%
5	3.181	576	588	606	rVB2	9249	22282	1.75%	0.237%
6	4.624	1025	1037	1066	rBV	169028	447382	35.09%	4.765%
7	5.058	1144	1172	1197	rBV	171029	402322	31.56%	4.285%
8	5.316	1239	1252	1261	rBV5	6180	13784	1.08%	0.147%
9	5.721	1354	1378	1405	rBV2	333165	873894	68.55%	9.307%
10	6.245	1527	1541	1561	rBV	370017	716877	56.23%	7.635%
11	6.541	1620	1633	1650	rBV2	91127	172409	13.52%	1.836%
12	6.685	1665	1678	1700	rBV	217354	426282	33.44%	4.540%
13	7.563	1939	1951	1968	rBV	102770	188108	14.75%	2.003%
14	7.894	2040	2054	2075	rBV	372723	657204	51.55%	6.999%
15	8.177	2130	2142	2161	rBV	63819	113046	8.87%	1.204%
16	8.550	2245	2258	2272	rBV	746854	1274900	100.00%	13.577%
17	8.630	2272	2283	2311	rVB2	555454	1048728	82.26%	11.169%
18	9.415	2511	2527	2553	rBV	516269	878210	68.88%	9.353%
19	10.753	2931	2943	2961	rBV	174516	279183	21.90%	2.973%
20	11.807	3258	3271	3297	rBV	468880	756558	59.34%	8.057%
21	12.190	3377	3390	3414	rBV	346878	567872	44.54%	6.048%




Sum of corrected areas: 9389809

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054717.D
Acq On : 30 Jun 2023 13:04
Operator : MD/SY
Sample : 03477-05DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

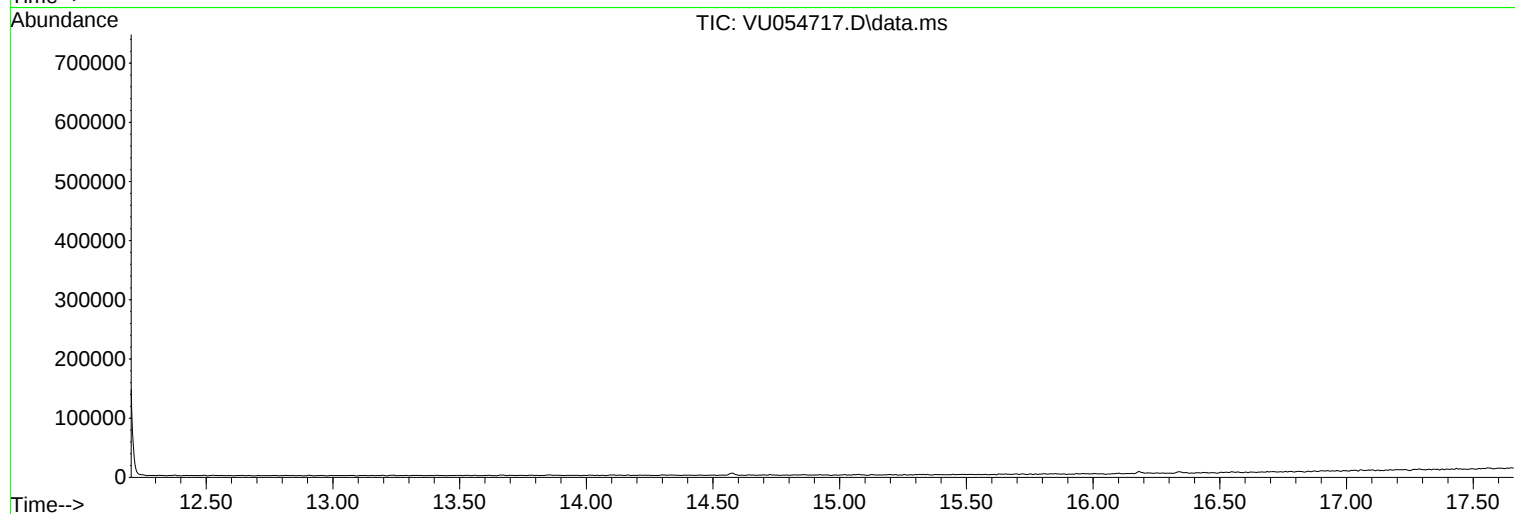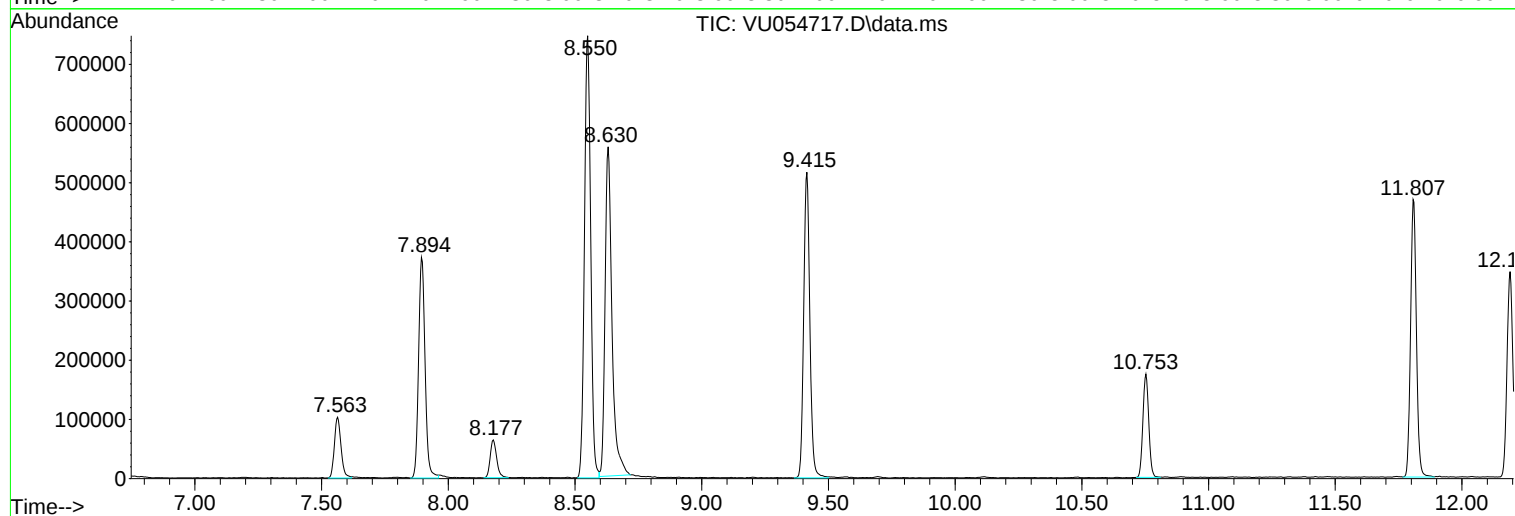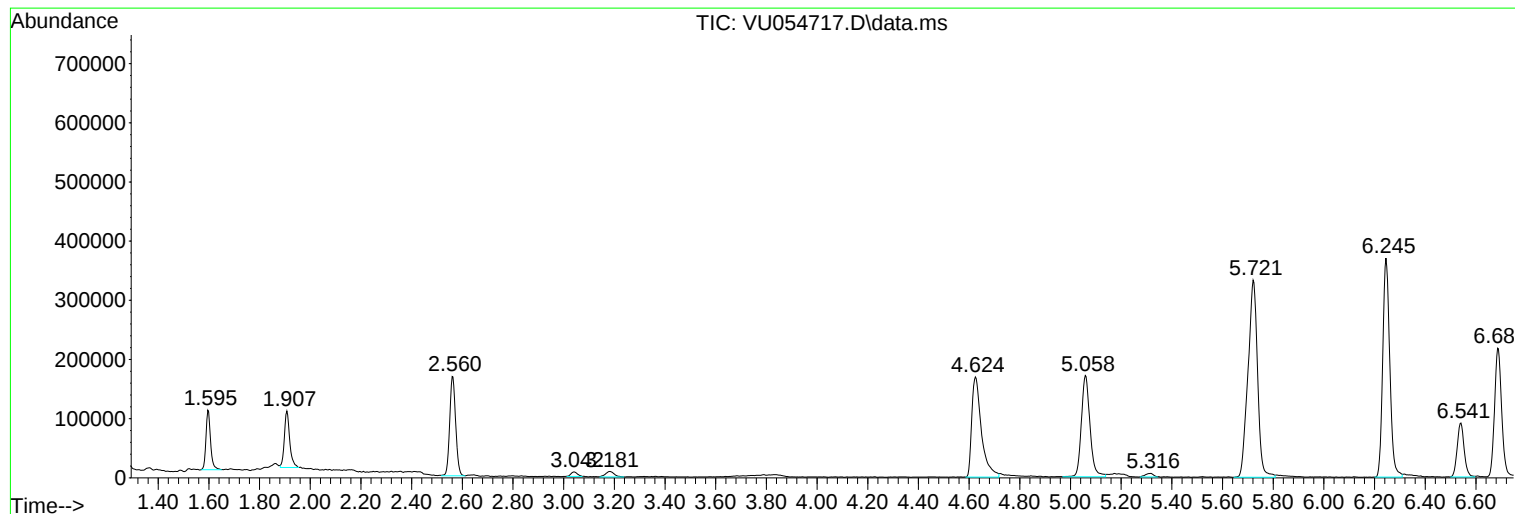

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054717.D
Acq On : 30 Jun 2023 13:04
Operator : MD/SY
Sample : 03477-05DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054717.D
Acq On : 30 Jun 2023 13:04
Operator : MD/SY
Sample : 03477-05DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc