

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054718.D
 Acq On : 30 Jun 2023 13:29
 Operator : MD/SY
 Sample : 03477-10DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HOA48DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054718.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	109	rBV	93993	117469	11.49%	1.381%
2	1.907	185	192	209	rVB	89102	129230	12.64%	1.519%
3	2.560	383	395	410	rVB	154718	251160	24.56%	2.952%
4	3.039	532	544	556	rBV2	21327	41791	4.09%	0.491%
5	3.181	574	588	603	rBV4	5719	13355	1.31%	0.157%
6	4.624	1025	1037	1072	rBV	154403	419217	41.00%	4.928%
7	5.058	1157	1172	1197	rVB	160900	377070	36.88%	4.432%
8	5.309	1237	1250	1264	rBV7	5875	13725	1.34%	0.161%
9	5.721	1359	1378	1406	rBV2	305546	806098	78.84%	9.476%
10	6.245	1527	1541	1568	rBV	342157	658193	64.37%	7.737%
11	6.541	1619	1633	1649	rBV2	56848	110305	10.79%	1.297%
12	6.685	1665	1678	1700	rBV	199378	399519	39.07%	4.696%
13	7.563	1936	1951	1971	rBV	96476	174386	17.05%	2.050%
14	7.894	2041	2054	2078	rBV	343633	602730	58.95%	7.085%
15	8.177	2130	2142	2157	rBV2	60821	107539	10.52%	1.264%
16	8.550	2242	2258	2273	rBV	589837	1022492	100.00%	12.019%
17	8.631	2273	2283	2325	rVB2	527615	998865	97.69%	11.742%
18	9.415	2514	2527	2553	rBV	466973	785288	76.80%	9.231%
19	10.753	2931	2943	2959	rBV	161454	263320	25.75%	3.095%
20	11.807	3259	3271	3287	rBV	429710	681601	66.66%	8.012%
21	12.190	3377	3390	3408	rBV2	322953	533742	52.20%	6.274%




Sum of corrected areas: 8507095

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054718.D
Acq On : 30 Jun 2023 13:29
Operator : MD/SY
Sample : 03477-10DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA48DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

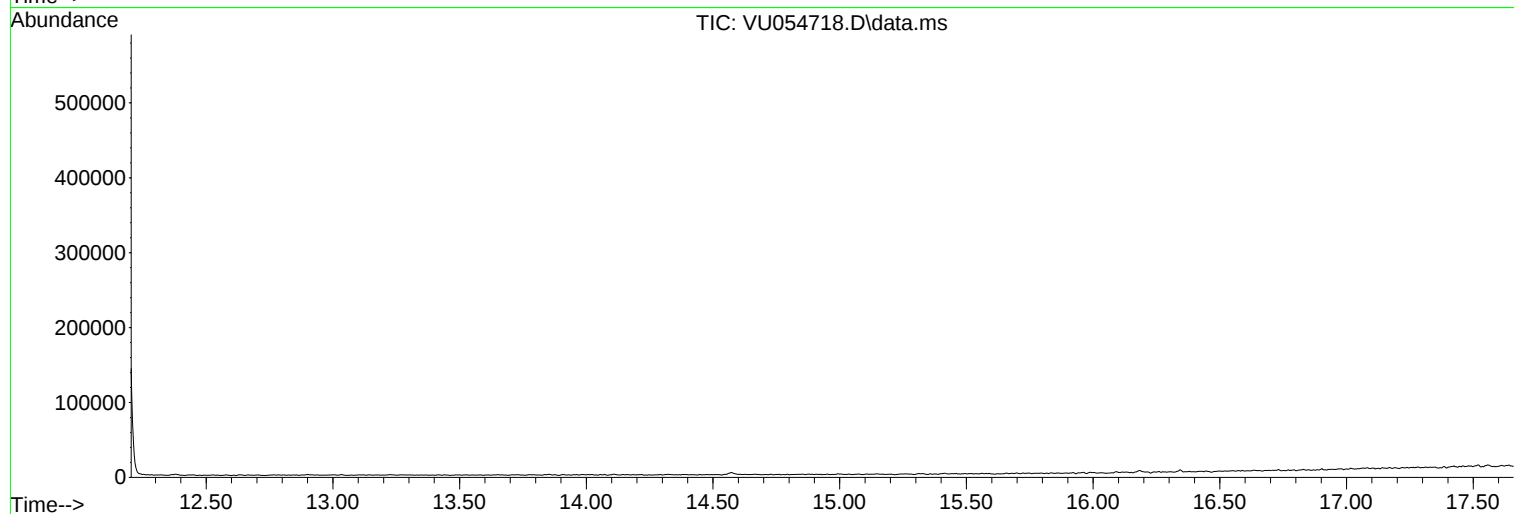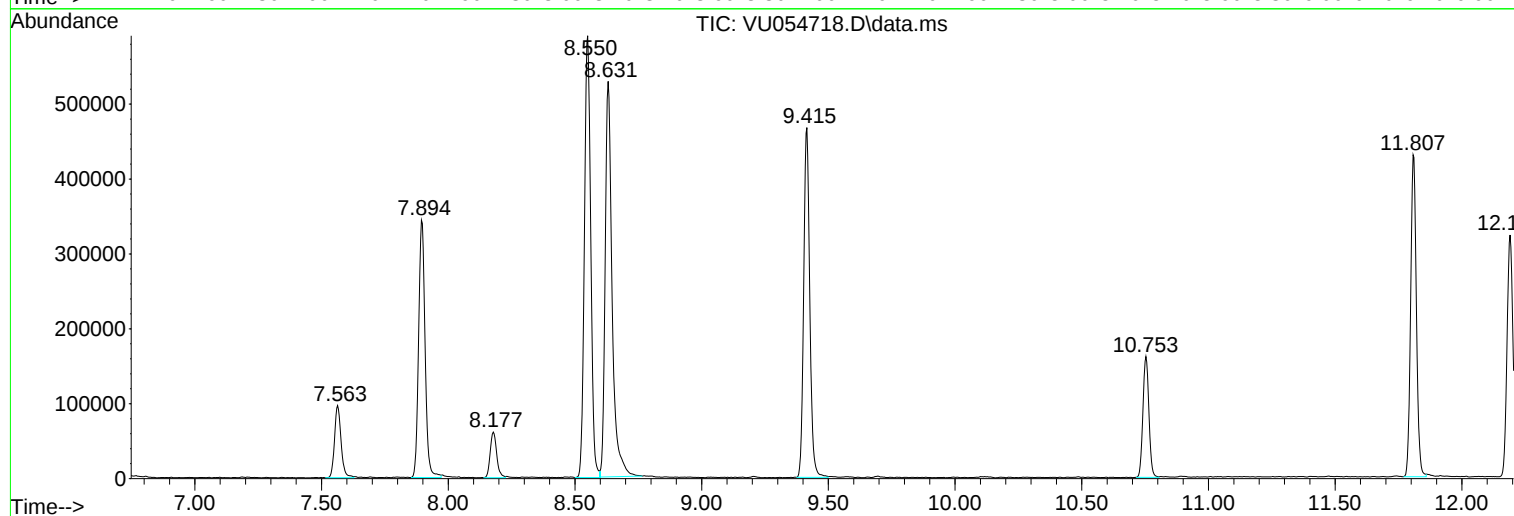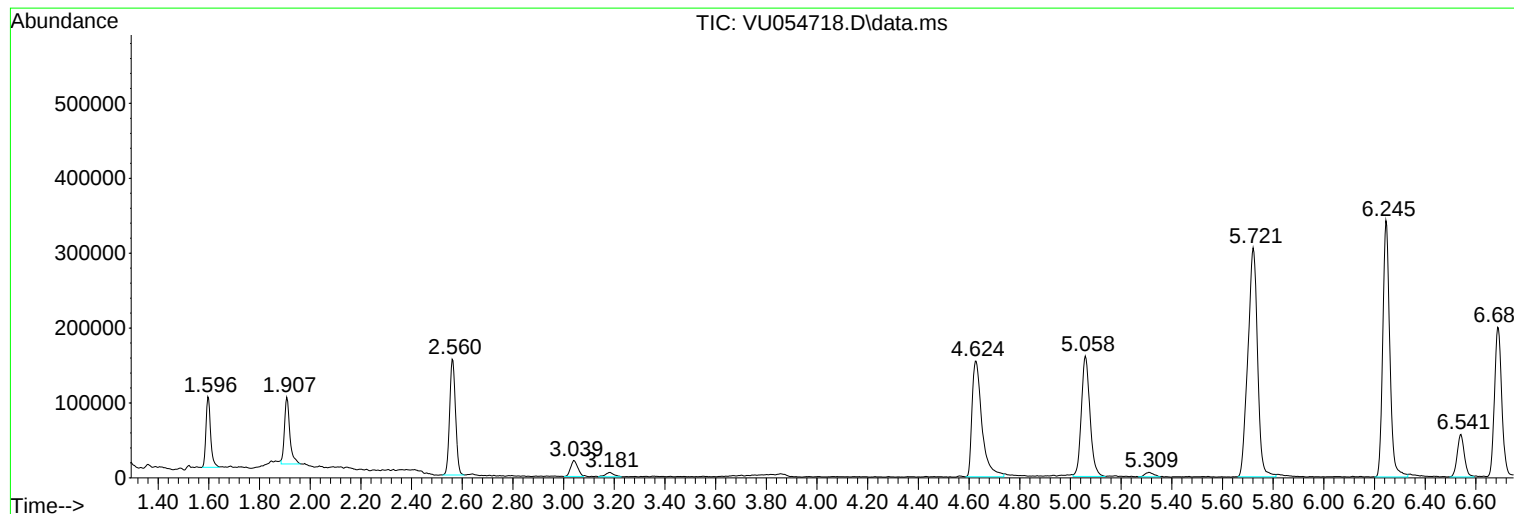

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054718.D
Acq On : 30 Jun 2023 13:29
Operator : MD/SY
Sample : 03477-10DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA48DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054718.D
Acq On : 30 Jun 2023 13:29
Operator : MD/SY
Sample : 03477-10DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA48DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc