

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054720.D
 Acq On : 30 Jun 2023 14:18
 Operator : MD/SY
 Sample : 03477-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HOA49

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	110	rVB	104459	129362	11.99%	1.636%
2	1.908	184	192	205	rVB	93227	134021	12.42%	1.695%
3	2.561	383	395	410	rVB	175516	283118	26.24%	3.580%
4	3.043	535	545	558	rVB2	16180	30396	2.82%	0.384%
5	3.178	578	587	602	rVB2	7385	15034	1.39%	0.190%
6	4.625	1024	1037	1069	rBV	170090	452583	41.94%	5.723%
7	5.059	1155	1172	1191	rBV	174837	384370	35.62%	4.861%
8	5.721	1356	1378	1407	rBV2	332868	891359	82.60%	11.272%
9	6.245	1528	1541	1562	rBV	345124	669648	62.05%	8.469%
10	6.686	1665	1678	1695	rBV	220297	438966	40.68%	5.551%
11	7.564	1938	1951	1969	rBV	105990	191432	17.74%	2.421%
12	7.895	2038	2054	2074	rBV	379564	673494	62.41%	8.517%
13	8.178	2129	2142	2164	rBV2	67799	119274	11.05%	1.508%
14	8.548	2247	2257	2270	rVB2	22768	39525	3.66%	0.500%
15	8.631	2270	2283	2314	rBV	566491	1079145	100.00%	13.647%
16	9.412	2512	2526	2547	rBV	475372	803706	74.48%	10.164%
17	10.753	2927	2943	2961	rBV	174641	288736	26.76%	3.651%
18	11.808	3259	3271	3301	rBV	434962	700909	64.95%	8.864%
19	12.190	3377	3390	3409	rBV	352767	582404	53.97%	7.365%




Sum of corrected areas: 7907482

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054720.D
Acq On : 30 Jun 2023 14:18
Operator : MD/SY
Sample : 03477-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

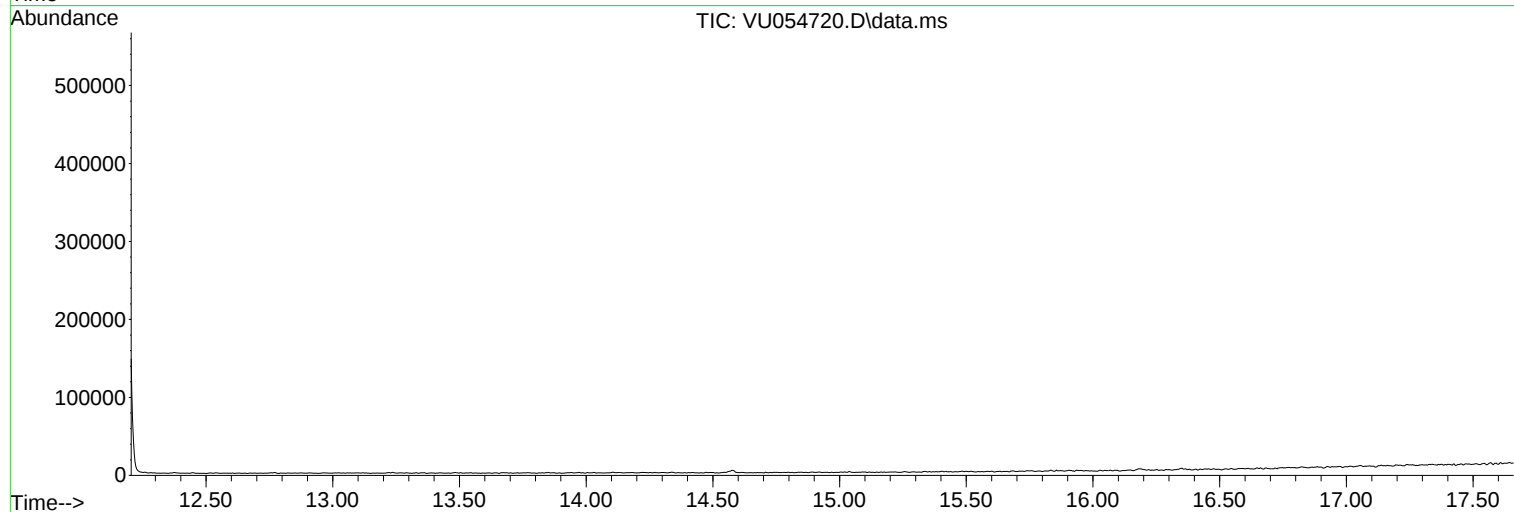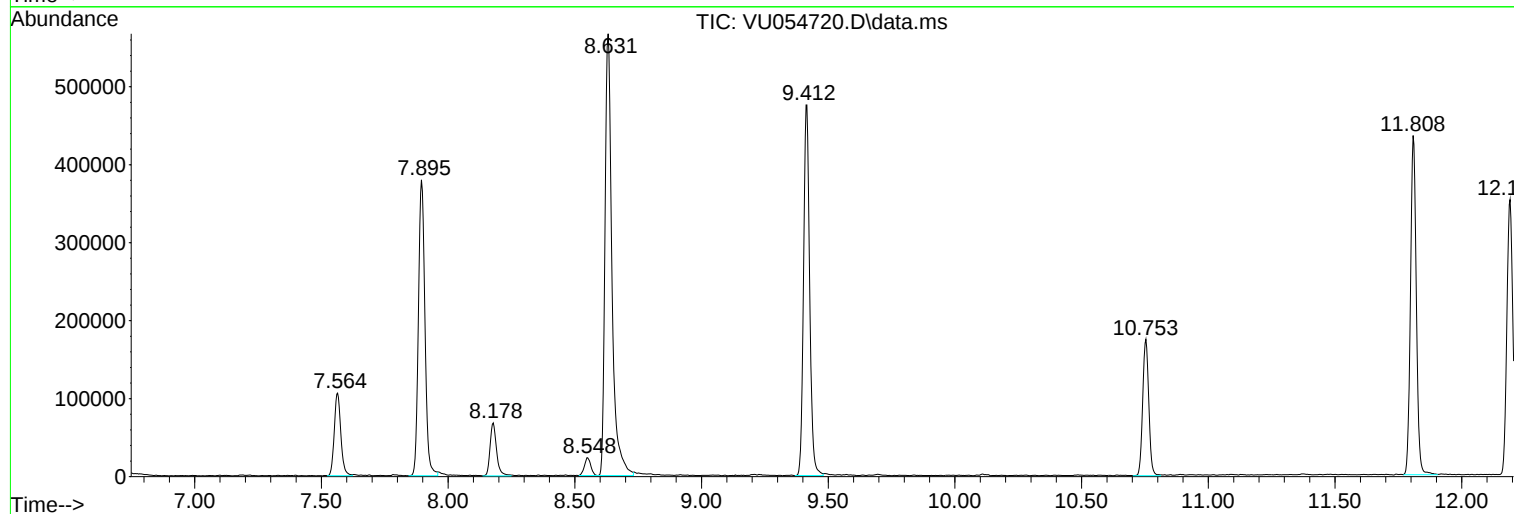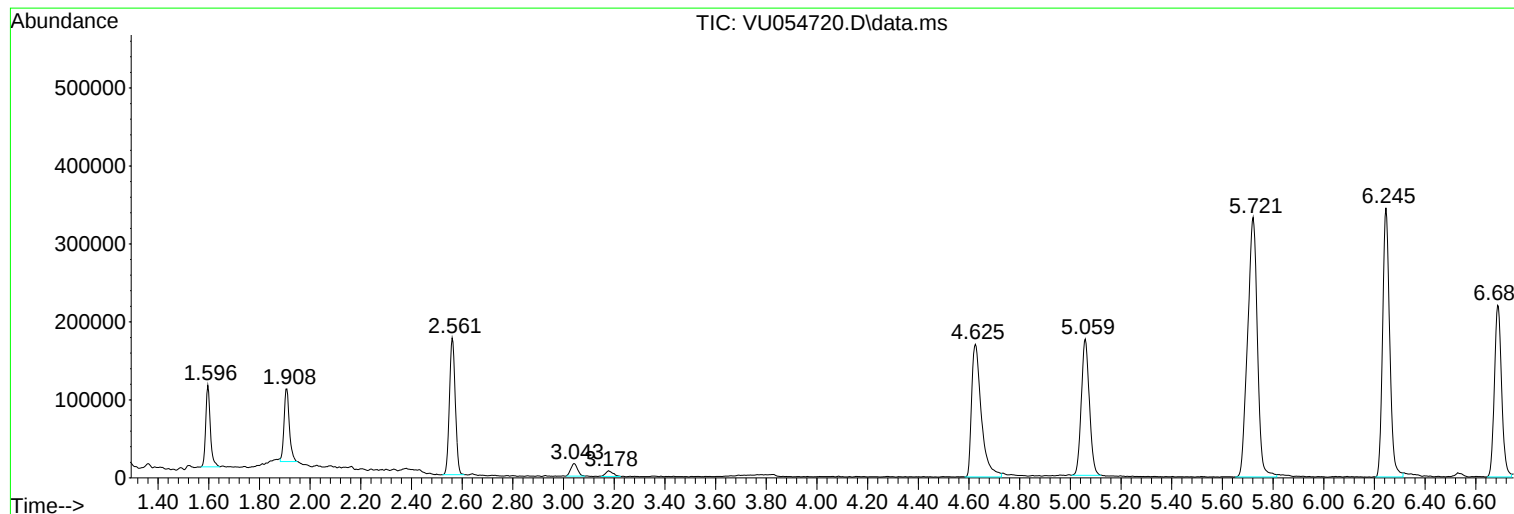

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054720.D
Acq On : 30 Jun 2023 14:18
Operator : MD/SY
Sample : 03477-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054720.D
Acq On : 30 Jun 2023 14:18
Operator : MD/SY
Sample : 03477-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOA49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc