

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054724.D
 Acq On : 30 Jun 2023 15:54
 Operator : MD/SY
 Sample : 03478-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054724.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	110	rBV	97557	118628	11.48%	1.565%
2	1.904	184	191	211	rVB	90902	136844	13.24%	1.806%
3	2.560	383	395	412	rBV	162478	265401	25.68%	3.502%
4	3.039	533	544	565	rVB2	20018	39015	3.77%	0.515%
5	3.177	577	587	602	rVB3	6478	14386	1.39%	0.190%
6	4.624	1021	1037	1062	rBV	162250	419883	40.62%	5.540%
7	5.058	1154	1172	1199	rVB	162494	370286	35.82%	4.886%
8	5.721	1355	1378	1405	rBV2	321634	840582	81.32%	11.091%
9	6.245	1527	1541	1563	rBV	336150	650109	62.89%	8.578%
10	6.685	1662	1678	1699	rBV	210418	417506	40.39%	5.509%
11	7.563	1939	1951	1972	rBV2	98986	180003	17.41%	2.375%
12	7.894	2041	2054	2071	rBV	359413	628404	60.79%	8.291%
13	8.177	2130	2142	2160	rBV2	64616	111371	10.77%	1.469%
14	8.467	2221	2232	2246	rVB2	6109	11287	1.09%	0.149%
15	8.550	2246	2258	2270	rBV5	16958	29883	2.89%	0.394%
16	8.630	2270	2283	2329	rBV	535817	1033647	100.00%	13.638%
17	9.415	2513	2527	2548	rBV	464461	794755	76.89%	10.486%
18	10.753	2928	2943	2957	rBV	165515	269078	26.03%	3.550%
19	10.888	2975	2985	2995	rBV2	10087	17483	1.69%	0.231%
20	11.810	3259	3272	3290	rBV	424498	685078	66.28%	9.039%
21	12.190	3378	3390	3410	rBV	337258	545520	52.78%	7.198%




Sum of corrected areas: 7579149

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054724.D
Acq On : 30 Jun 2023 15:54
Operator : MD/SY
Sample : 03478-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

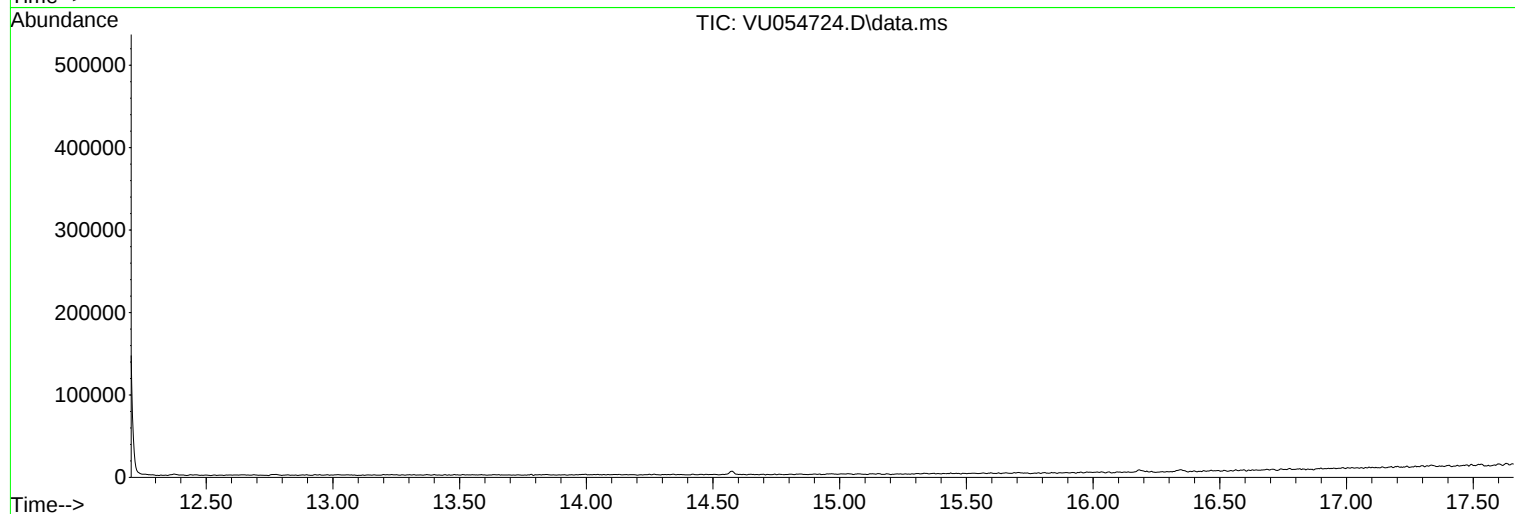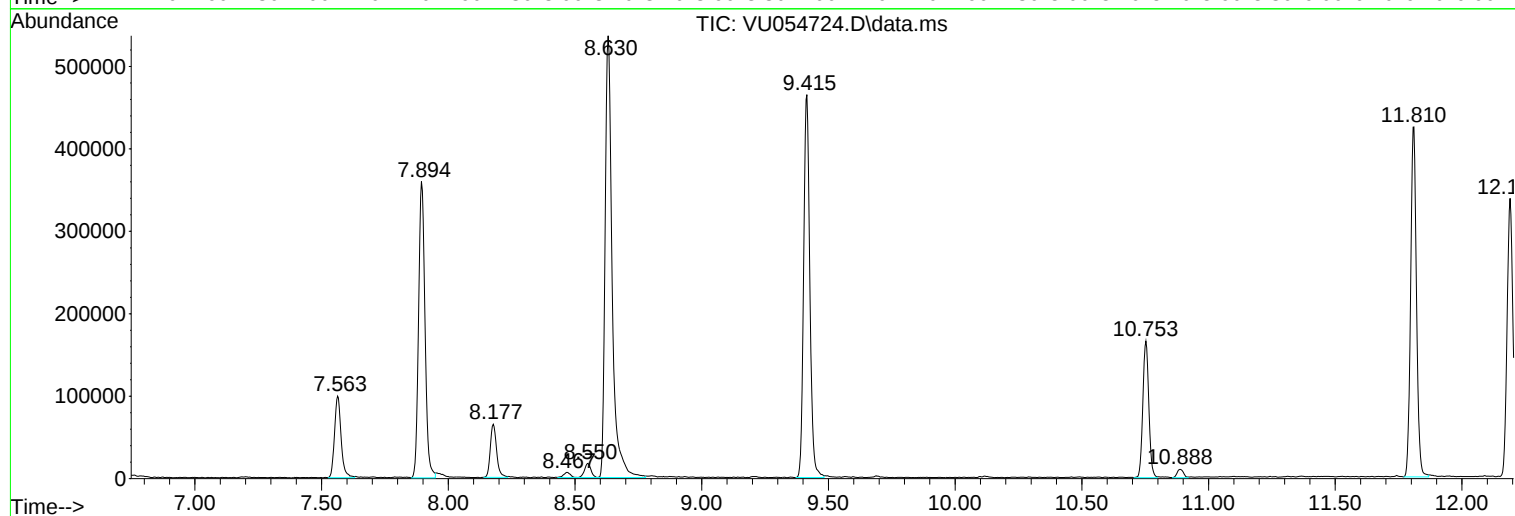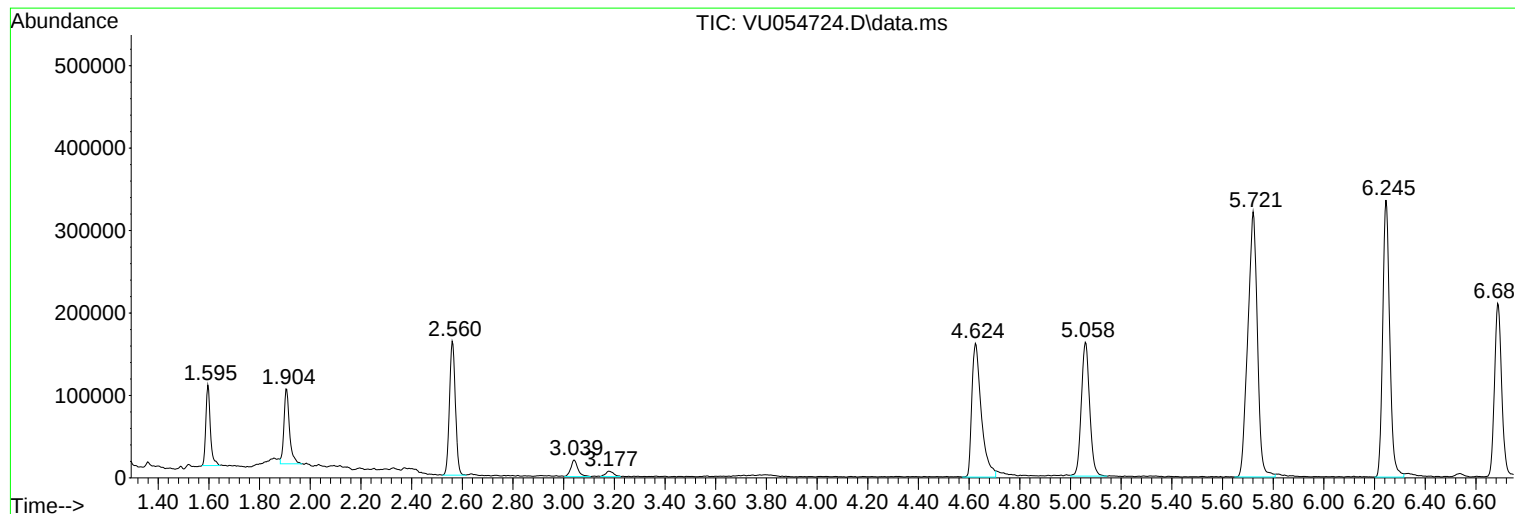

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054724.D
Acq On : 30 Jun 2023 15:54
Operator : MD/SY
Sample : 03478-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054724.D
Acq On : 30 Jun 2023 15:54
Operator : MD/SY
Sample : 03478-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc