

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054727.D
 Acq On : 30 Jun 2023 17:06
 Operator : MD/SY
 Sample : 03495-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0FA3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	66	71	79	rBV	17938	22206	1.15%	0.237%
2	1.596	88	95	109	rVB	91497	114406	5.93%	1.223%
3	1.907	185	192	213	rVB	83027	122891	6.37%	1.313%
4	2.560	383	395	410	rBV	154131	249512	12.93%	2.667%
5	4.624	1024	1037	1071	rBV	161855	427019	22.12%	4.564%
6	5.062	1157	1173	1199	rVB2	168573	438385	22.71%	4.685%
7	5.721	1358	1378	1399	rBV2	304896	798040	41.34%	8.529%
8	6.245	1528	1541	1562	rBV	332452	647403	33.54%	6.919%
9	6.537	1623	1632	1645	rBV4	10846	21630	1.12%	0.231%
10	6.685	1664	1678	1695	rBV	201492	398866	20.66%	4.263%
11	7.563	1937	1951	1968	rBV	93991	171230	8.87%	1.830%
12	7.894	2041	2054	2073	rBV	336836	596167	30.88%	6.372%
13	8.177	2127	2142	2159	rBV2	58344	106084	5.50%	1.134%
14	8.550	2244	2258	2273	rBV	1123871	1930360	100.00%	20.631%
15	8.631	2273	2283	2321	rVB	524578	1015825	52.62%	10.857%
16	9.415	2514	2527	2553	rBV	460832	786589	40.75%	8.407%
17	10.753	2931	2943	2962	rBV2	163871	265895	13.77%	2.842%
18	10.891	2976	2986	2997	rVB	15960	25243	1.31%	0.270%
19	11.811	3259	3272	3292	rBV	423317	689031	35.69%	7.364%
20	12.190	3378	3390	3410	rBV	323273	529608	27.44%	5.660%




Sum of corrected areas: 9356390

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054727.D
Acq On : 30 Jun 2023 17:06
Operator : MD/SY
Sample : 03495-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

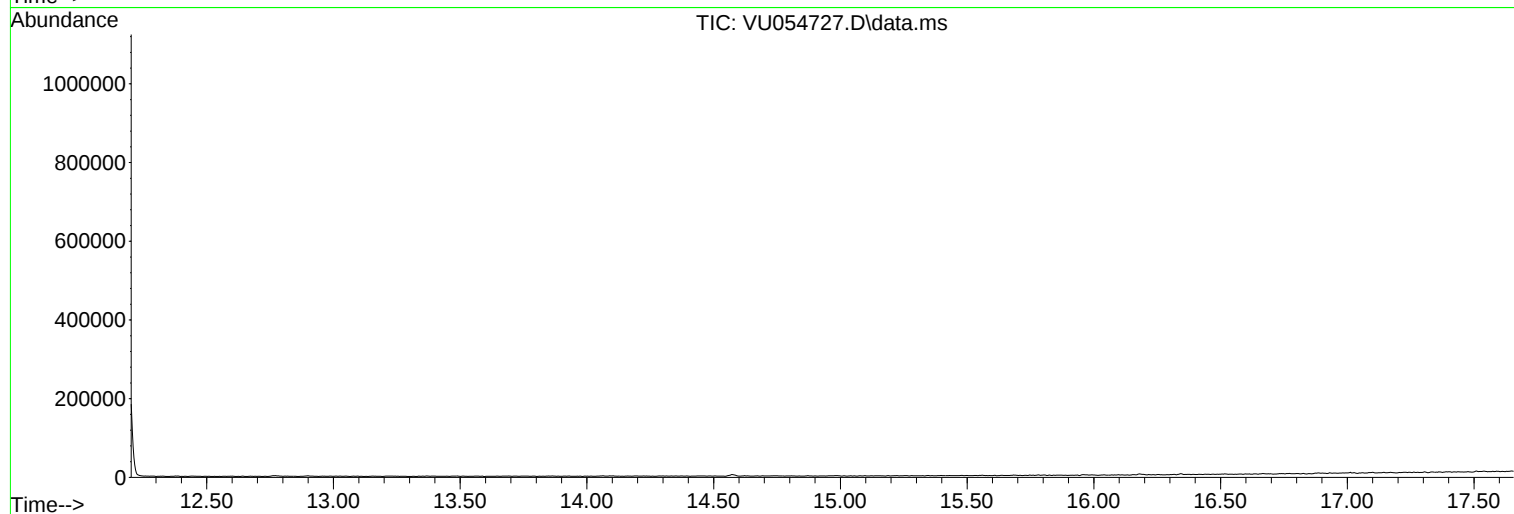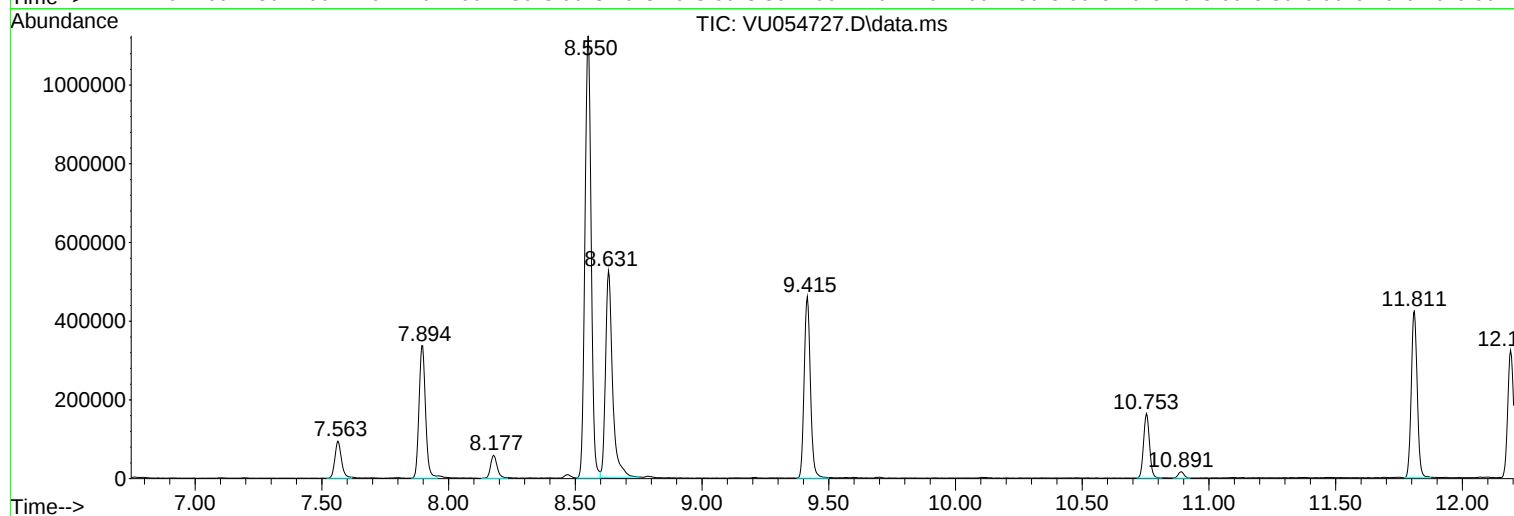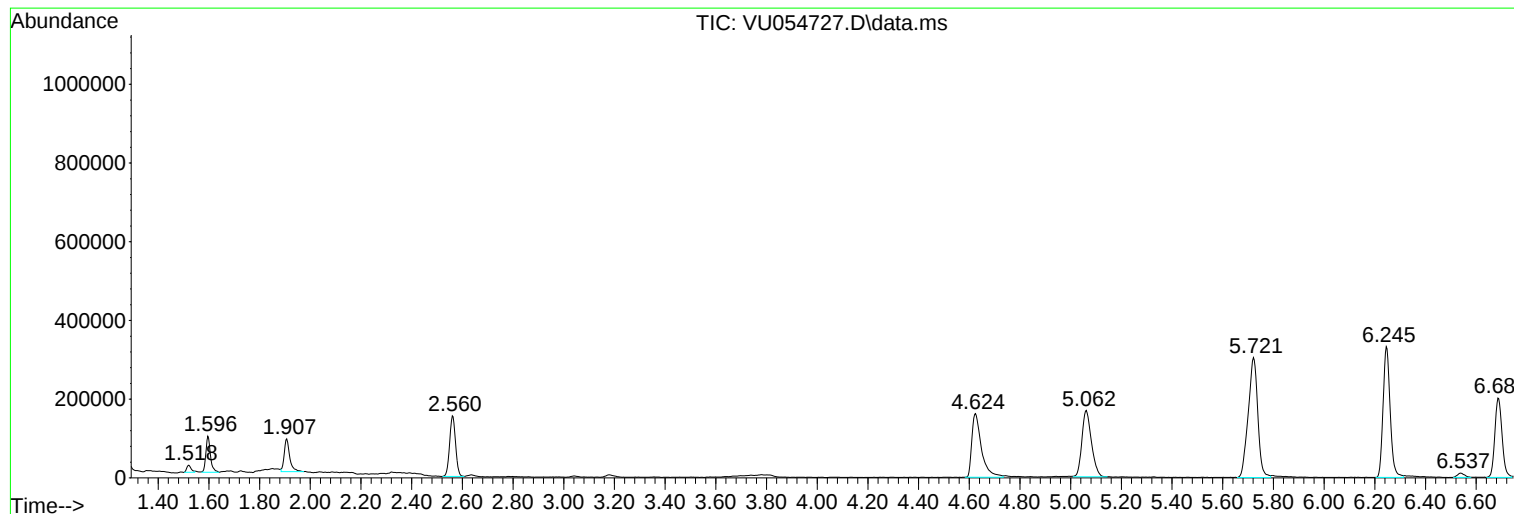

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054727.D
Acq On : 30 Jun 2023 17:06
Operator : MD/SY
Sample : 03495-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054727.D
Acq On : 30 Jun 2023 17:06
Operator : MD/SY
Sample : 03495-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc