

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054730.D
 Acq On : 30 Jun 2023 18:20
 Operator : MD/SY
 Sample : 03495-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0FA8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054730.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	66	71	82	rBV	19792	26245	2.66%	0.347%
2	1.596	88	95	108	rVB	90731	113003	11.43%	1.495%
3	1.908	185	192	203	rVB	82122	109343	11.06%	1.447%
4	2.563	384	396	409	rBV	151500	247676	25.06%	3.278%
5	3.184	578	589	604	rBV3	6972	15109	1.53%	0.200%
6	4.624	1026	1037	1081	rBV	155625	420652	42.56%	5.567%
7	5.059	1156	1172	1199	rVB3	169304	430725	43.58%	5.700%
8	5.721	1359	1378	1404	rBV2	302864	800956	81.04%	10.599%
9	6.245	1528	1541	1564	rBV2	345189	670062	67.80%	8.867%
10	6.685	1664	1678	1703	rBV	198384	398237	40.29%	5.270%
11	7.563	1939	1951	1973	rBV2	91952	168854	17.08%	2.235%
12	7.894	2037	2054	2073	rBV	343029	596466	60.35%	7.893%
13	8.177	2128	2142	2161	rBV	58424	104799	10.60%	1.387%
14	8.550	2247	2258	2271	rBV2	61318	107277	10.85%	1.420%
15	8.631	2271	2283	2316	rBV	511735	988352	100.00%	13.079%
16	9.415	2514	2527	2558	rBV	487616	824420	83.41%	10.910%
17	10.753	2930	2943	2958	rBV	160175	262880	26.60%	3.479%
18	10.891	2976	2986	2994	rBV2	9388	14905	1.51%	0.197%
19	11.807	3259	3271	3290	rBV	444790	723727	73.23%	9.577%
20	12.190	3378	3390	3410	rBV	328852	532870	53.92%	7.052%




Sum of corrected areas: 7556558

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054730.D
Acq On : 30 Jun 2023 18:20
Operator : MD/SY
Sample : 03495-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

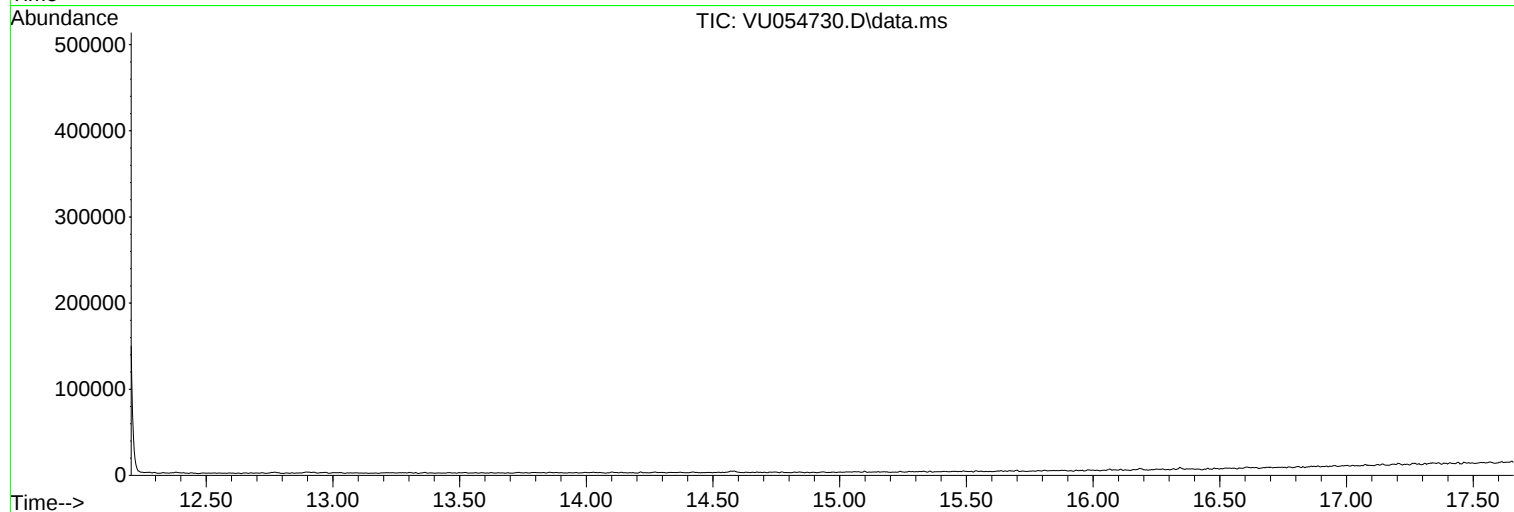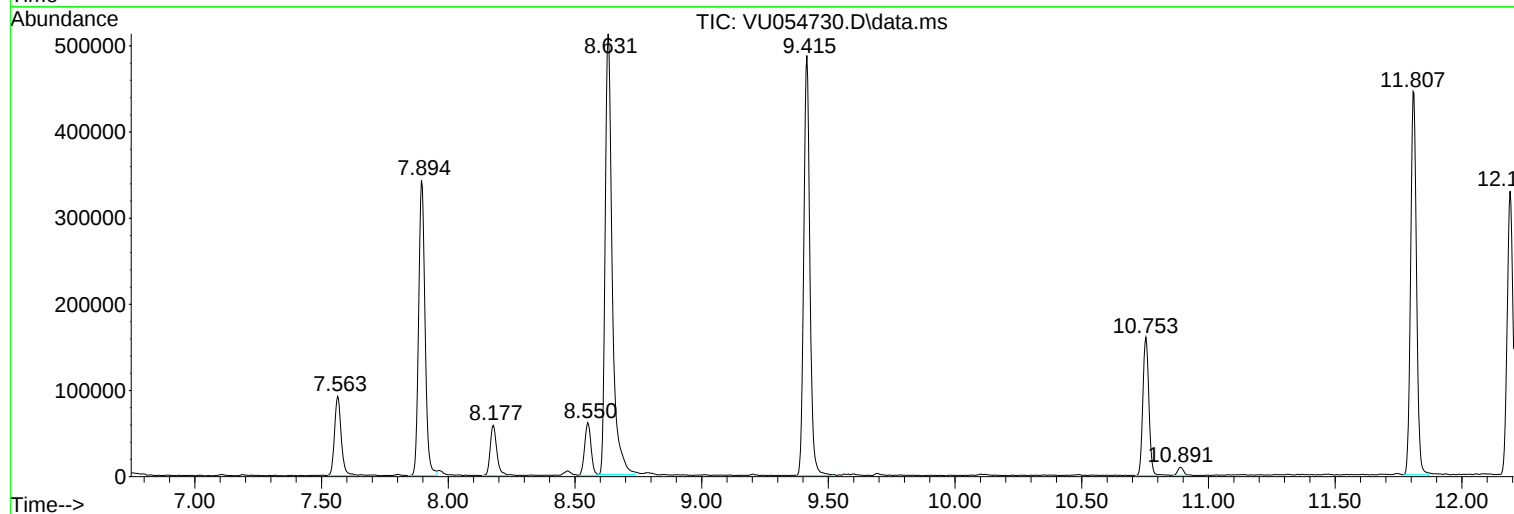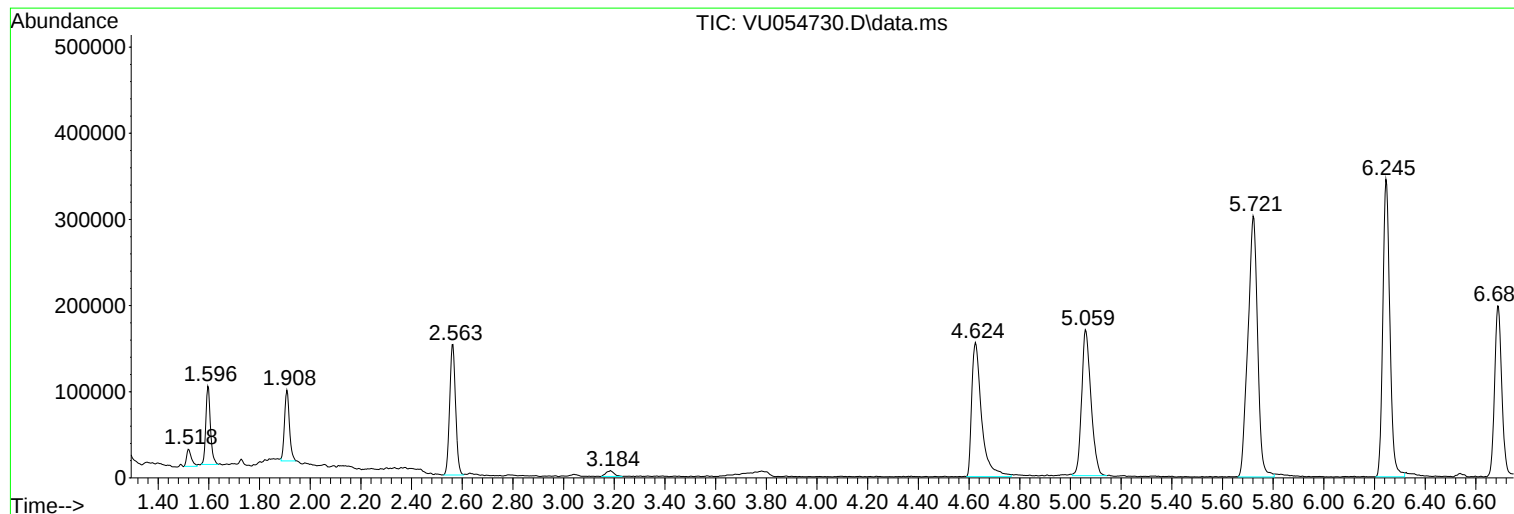

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054730.D
Acq On : 30 Jun 2023 18:20
Operator : MD/SY
Sample : 03495-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054730.D
Acq On : 30 Jun 2023 18:20
Operator : MD/SY
Sample : 03495-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------