

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054731.D
 Acq On : 30 Jun 2023 18:45
 Operator : MD/SY
 Sample : 03495-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0FB0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054731.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	66	71	80	rVV	25796	30324	3.10%	0.414%
2	1.596	88	95	111	rVB	92443	114759	11.73%	1.565%
3	1.727	131	136	144	rVB	10157	11515	1.18%	0.157%
4	1.907	184	192	210	rVB	85705	125003	12.78%	1.705%
5	2.560	384	395	409	rBV	147541	241986	24.73%	3.300%
6	3.181	576	588	601	rBV	10172	23010	2.35%	0.314%
7	4.624	1025	1037	1062	rBV	155770	408145	41.71%	5.566%
8	5.062	1157	1173	1198	rVB2	163962	403629	41.25%	5.504%
9	5.721	1357	1378	1405	rBV2	300817	793773	81.12%	10.825%
10	6.245	1525	1541	1568	rBV	320675	632301	64.62%	8.623%
11	6.685	1664	1678	1698	rBV	200335	395114	40.38%	5.388%
12	7.563	1937	1951	1979	rBV2	90220	169834	17.36%	2.316%
13	7.894	2041	2054	2073	rBV	337997	587927	60.09%	8.017%
14	8.177	2129	2142	2160	rBV2	57527	101349	10.36%	1.382%
15	8.550	2245	2258	2271	rBV2	43864	75308	7.70%	1.027%
16	8.631	2271	2283	2313	rBV	507977	978473	100.00%	13.343%
17	9.415	2512	2527	2549	rBV	451899	772345	78.93%	10.532%
18	10.753	2929	2943	2959	rBV	158457	258680	26.44%	3.528%
19	10.888	2976	2985	2996	rVB2	7032	11319	1.16%	0.154%
20	11.807	3259	3271	3291	rBV	417280	673854	68.87%	9.189%
21	12.190	3376	3390	3409	rBV	317996	524435	53.60%	7.152%




Sum of corrected areas: 7333083

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054731.D
Acq On : 30 Jun 2023 18:45
Operator : MD/SY
Sample : 03495-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

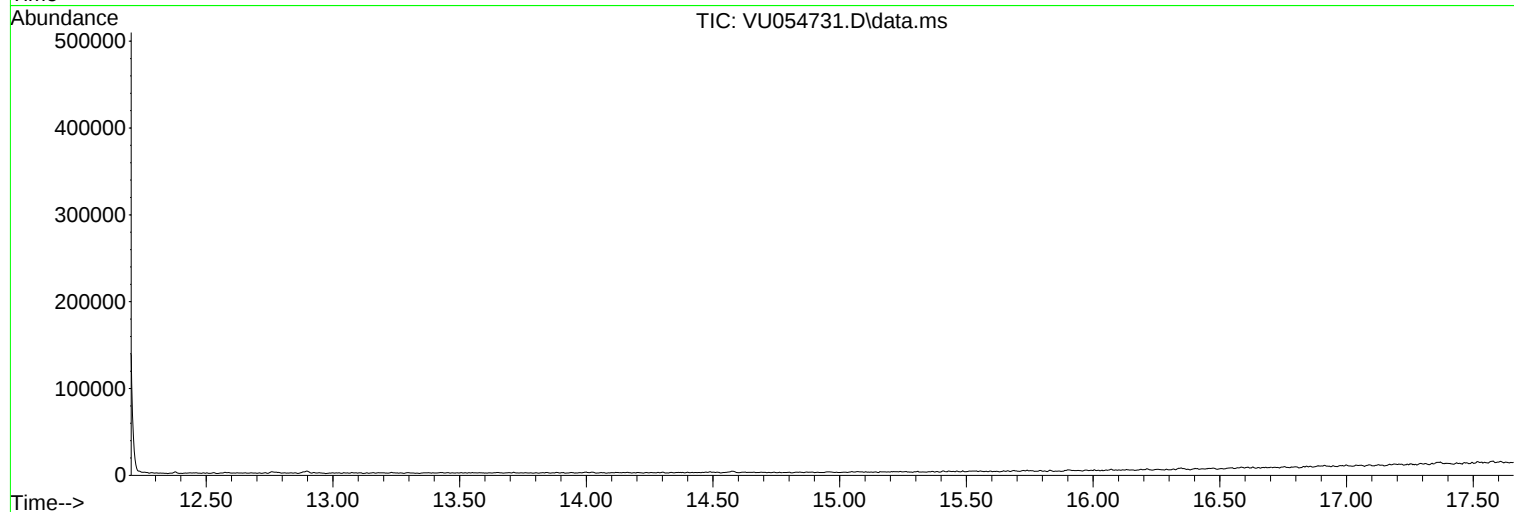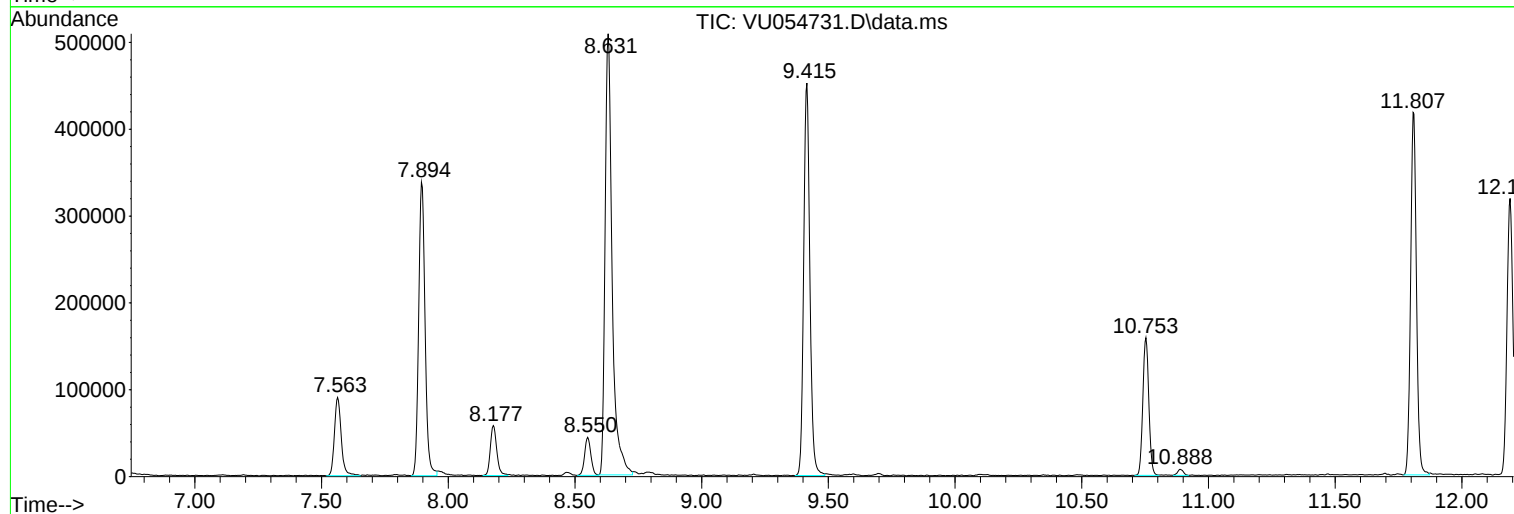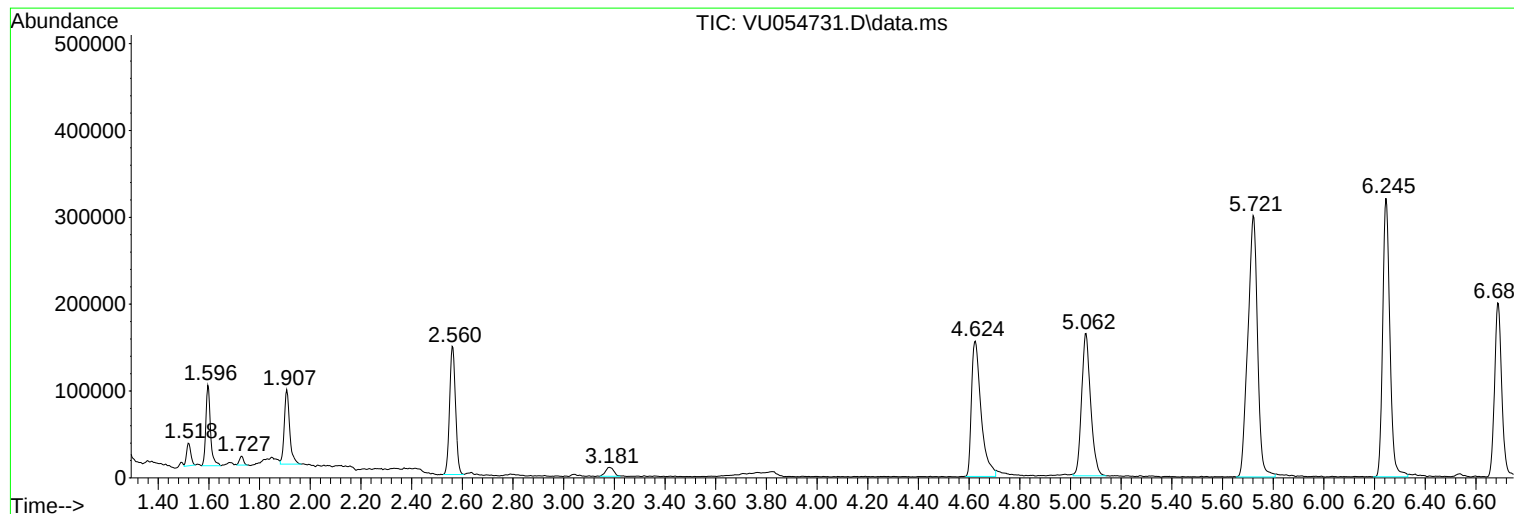

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054731.D
Acq On : 30 Jun 2023 18:45
Operator : MD/SY
Sample : 03495-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054731.D
Acq On : 30 Jun 2023 18:45
Operator : MD/SY
Sample : 03495-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------