

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054734.D
 Acq On : 30 Jun 2023 19:59
 Operator : MD/SY
 Sample : VIBLK170
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK170

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054734.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	114	rVB	93410	115077	11.54%	1.501%
2	1.907	185	192	213	rVB	86580	128198	12.85%	1.673%
3	2.563	384	396	411	rVB	148599	244303	24.50%	3.187%
4	3.039	533	544	563	rBV2	18080	37048	3.71%	0.483%
5	3.181	576	588	603	rVB3	6363	14688	1.47%	0.192%
6	4.624	1025	1037	1082	rBV	150215	423264	42.44%	5.522%
7	5.058	1157	1172	1191	rBV	148358	336447	33.74%	4.389%
8	5.721	1358	1378	1413	rBV2	291847	781829	78.39%	10.200%
9	6.245	1527	1541	1561	rBV	345732	661296	66.31%	8.627%
10	6.537	1620	1632	1645	rVB10	6830	13520	1.36%	0.176%
11	6.689	1665	1679	1695	rBV	189946	378925	37.99%	4.944%
12	7.563	1935	1951	1970	rBV	92169	169739	17.02%	2.214%
13	7.791	2011	2022	2041	rBV3	12804	25732	2.58%	0.336%
14	7.894	2041	2054	2071	rBV	335475	589786	59.14%	7.695%
15	7.965	2073	2076	2087	rVB3	8002	12140	1.22%	0.158%
16	8.177	2131	2142	2164	rBV	56217	102875	10.32%	1.342%
17	8.550	2245	2258	2271	rVB4	22848	41064	4.12%	0.536%
18	8.631	2271	2283	2319	rBV2	506990	997317	100.00%	13.011%
19	9.415	2514	2527	2551	rBV	476000	814099	81.63%	10.621%
20	9.569	2567	2575	2590	rVB	7535	12106	1.21%	0.158%
21	9.692	2603	2613	2626	rBV4	6630	12331	1.24%	0.161%
22	10.110	2726	2743	2754	rBV6	9159	21342	2.14%	0.278%
23	10.483	2848	2859	2867	rBV3	6636	11046	1.11%	0.144%
24	10.753	2931	2943	2959	rBV	153895	254438	25.51%	3.319%
25	10.888	2975	2985	3000	rVB2	8993	14846	1.49%	0.194%
26	11.466	3154	3165	3177	rBV3	9758	14870	1.49%	0.194%
27	11.746	3244	3252	3260	rBV5	9473	15766	1.58%	0.206%
28	11.807	3260	3271	3295	rVV	442524	733230	73.52%	9.566%
29	12.190	3377	3390	3407	rBV	316515	538475	53.99%	7.025%
30	13.219	3701	3710	3724	rBV3	16551	26132	2.62%	0.341%
31	13.839	3894	3903	3914	rBV3	25801	39714	3.98%	0.518%
32	14.087	3971	3980	3994	rBV3	21136	38412	3.85%	0.501%
33	14.328	4044	4055	4071	rBV2	27849	44964	4.51%	0.587%




Sum of corrected areas: 7665019

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054734.D
Acq On : 30 Jun 2023 19:59
Operator : MD/SY
Sample : VIBLK170
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK170

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

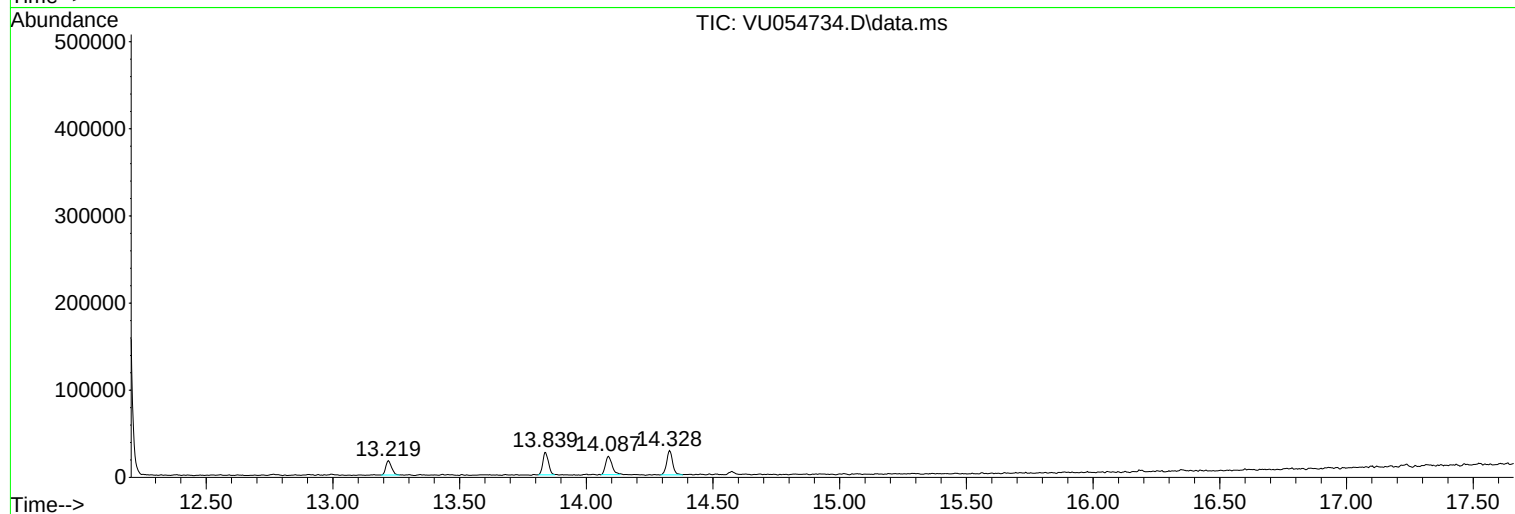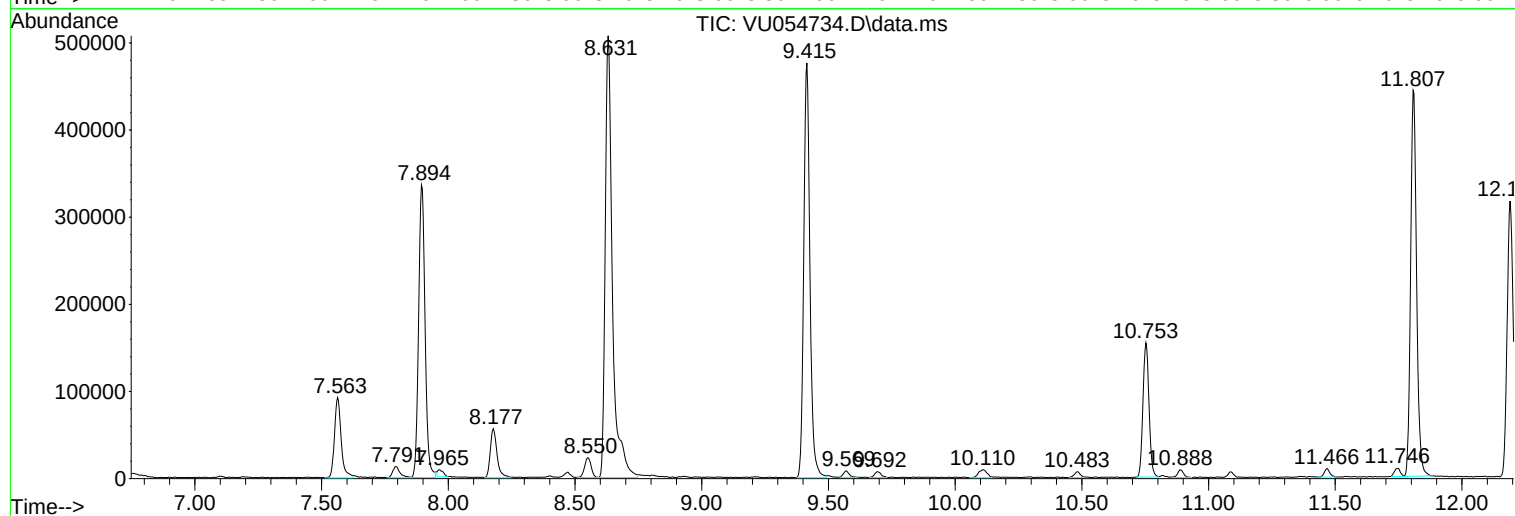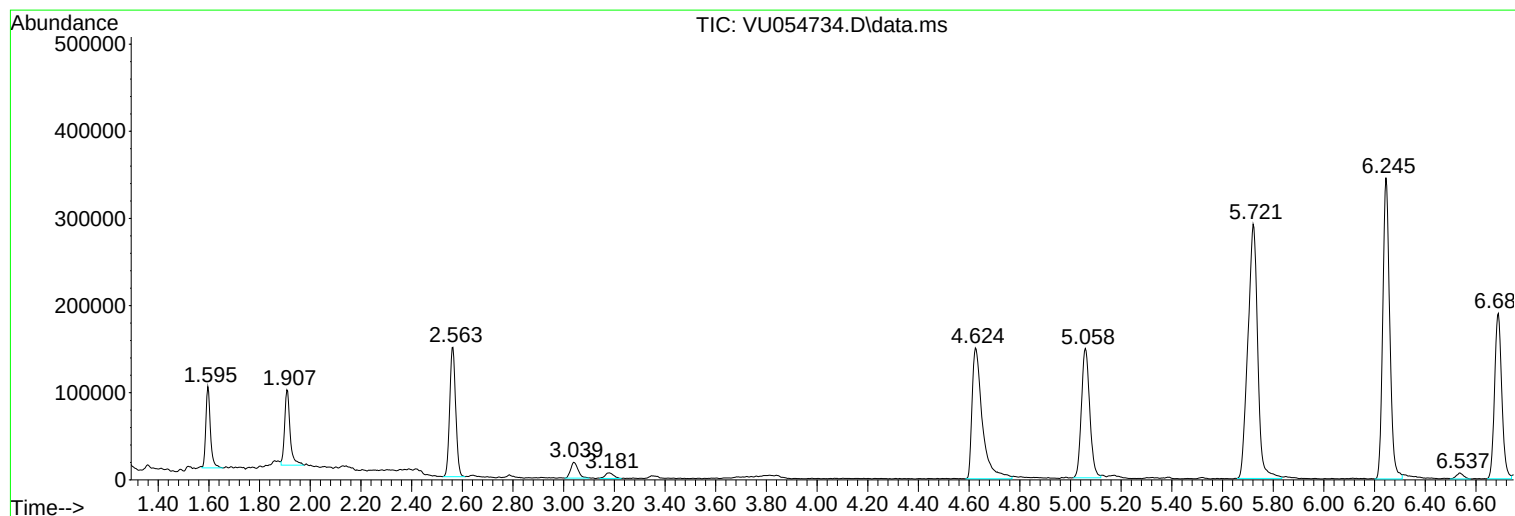

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054734.D
Acq On : 30 Jun 2023 19:59
Operator : MD/SY
Sample : VIBLK170
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK170

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
Data File : VU054734.D
Acq On : 30 Jun 2023 19:59
Operator : MD/SY
Sample : VIBLK170
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK170

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------