


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU063023\
 Data File : VU054708.D
 Acq On : 30 Jun 2023 08:39
 Operator : MD/SY
 Sample : BFB028
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB028

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jul 05 04:39:25 2023

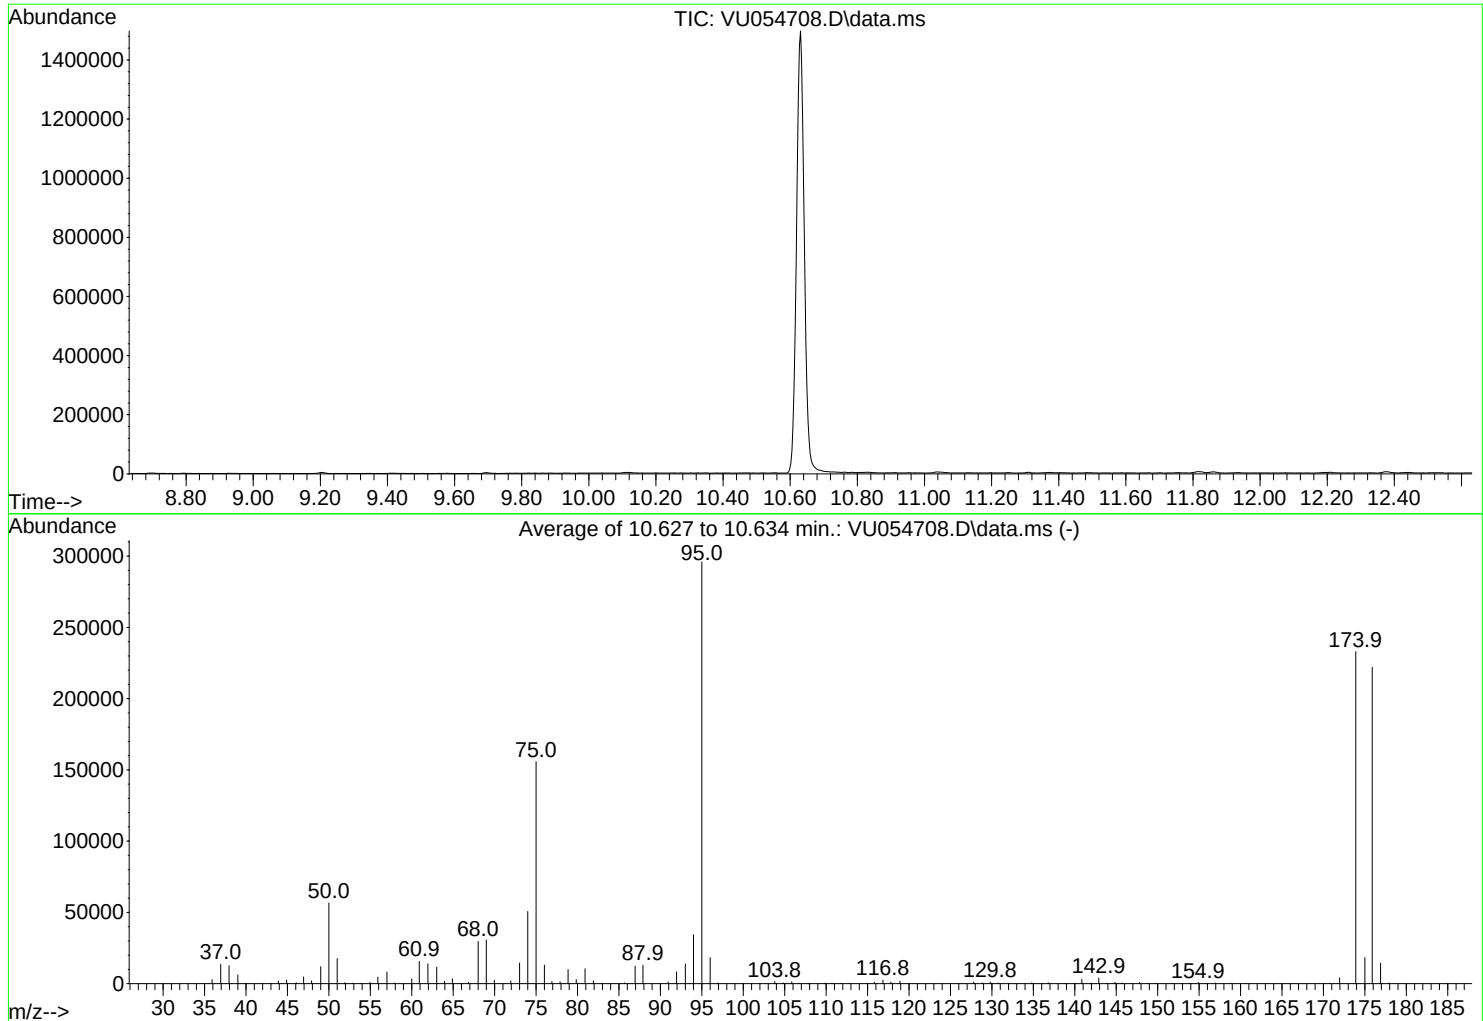

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	56560	PASS
75	95	30	80	52.6	155755	PASS
95	95	100	100	100.0	296000	PASS
96	95	5	9	6.2	18288	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.7	233003	PASS
175	174	5	9	7.9	18299	PASS
176	174	95	101	95.3	222059	PASS
177	176	5	9	6.5	14423	PASS

m/z	Abundance
35.90	1263.0
37.90	381.0
39.90	170.0
43.80	728.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
36.00	3946.0
36.90	13658.0
38.00	12930.0
39.00	6027.0
40.00	389.0
41.70	103.0
42.90	235.0
44.00	2705.0
44.90	2662.0
46.00	631.0
47.00	4659.0
47.90	1996.0
49.00	12325.0
50.00	57208.0
51.00	17744.0
51.90	646.0
52.90	263.0
53.80	122.0
55.00	856.0
55.90	4709.0
57.00	8144.0
57.90	482.0
60.00	3265.0
60.90	15691.0
61.90	13842.0
63.00	11811.0
64.00	1673.0
64.90	3533.0
66.10	308.0
66.80	935.0
68.00	29704.0
69.00	30904.0
69.90	2412.0
72.00	2146.0
73.00	14531.0
74.00	50456.0
75.00	157696.0
76.00	13254.0
76.90	1572.0
77.90	1320.0
78.90	9985.0
79.90	2997.0
80.90	10691.0
81.90	2010.0
83.00	297.0
85.70	577.0
87.00	12469.0
87.90	13188.0
90.90	1126.0
91.90	8071.0
93.00	13617.0
94.00	34688.0
95.00	296384.0
96.00	18904.0
96.90	480.0
102.60	145.0
103.80	1381.0
104.80	522.0
105.90	1237.0
106.70	273.0
107.80	125.0
109.90	255.0
110.70	282.0
111.80	264.0
112.80	270.0
115.00	251.0
115.80	1180.0
116.80	2317.0
117.80	1108.0
118.90	1989.0
124.00	170.0
125.90	112.0
127.80	1156.0
128.90	680.0
129.80	1147.0
130.70	454.0
134.80	603.0
136.80	688.0
138.90	105.0
140.00	255.0
140.80	2959.0
142.00	368.0
142.90	3726.0
143.90	324.0
144.90	913.0
145.70	403.0
146.90	224.0
147.80	783.0
148.80	175.0
149.80	247.0
151.80	123.0
152.80	196.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

153.80	202.0
154.90	784.0
156.00	196.0
157.00	468.0
158.90	325.0
160.60	326.0
169.50	123.0
170.00	101.0
170.70	346.0
172.00	4070.0
173.90	230144.0
175.00	17848.0
175.90	218944.0
176.90	14333.0
177.90	462.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
35.90	4073.0
37.00	13938.0
38.00	13329.0
39.00	6216.0
40.00	421.0
41.70	105.0
42.90	274.0
43.90	2659.0
44.90	2489.0
46.00	681.0
46.90	4912.0
47.90	1939.0
49.00	12281.0
50.00	58352.0
51.00	18296.0
51.90	722.0
52.80	310.0
53.80	102.0
55.00	1007.0
55.90	4867.0
57.00	8442.0
57.90	474.0
60.00	3324.0
60.90	16307.0
62.00	14284.0
63.00	11721.0
63.90	1726.0
64.90	3487.0
66.00	268.0
66.90	973.0
68.00	30832.0
69.00	31736.0
70.00	2385.0
72.00	2073.0
73.00	15239.0
74.00	52120.0
75.00	161152.0
76.00	13557.0
76.90	1637.0
77.90	1309.0
78.80	10218.0
79.90	2874.0
80.90	10687.0
81.90	2175.0
83.00	290.0
85.70	591.0
87.00	12591.0
87.90	13256.0
90.90	1088.0
92.00	8681.0
93.00	14361.0
94.00	35104.0
95.00	305600.0
96.00	18800.0
97.00	448.0
102.70	181.0
103.80	1471.0
104.80	568.0
105.90	1410.0
106.70	310.0
109.90	332.0
110.70	337.0
111.70	241.0
112.80	313.0
115.00	281.0
115.80	1087.0
116.90	2517.0
117.80	1195.0
118.90	1902.0
124.00	109.0
125.90	120.0
127.80	1117.0
128.80	603.0
129.80	1143.0
130.80	498.0
134.80	594.0
136.80	743.0
138.90	145.0
140.00	311.0
140.80	3123.0
142.00	395.0
142.90	4198.0
143.90	368.0
144.90	892.0
145.70	426.0
146.90	246.0
147.80	867.0
148.80	222.0
149.70	269.0
151.80	211.0
152.90	200.0
153.80	272.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

154.90	855.0
156.00	247.0
156.90	468.0
158.00	122.0
158.90	224.0
160.70	295.0
169.50	101.0
170.00	130.0
170.70	315.0
172.00	4161.0
173.90	241344.0
175.00	18952.0
175.90	229120.0
176.90	14940.0
177.90	467.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
35.90	3907.0
37.00	13182.0
38.00	12469.0
39.00	5869.0
40.00	406.0
42.90	250.0
43.90	2364.0
44.90	2144.0
46.10	568.0
46.90	4475.0
47.90	1760.0
49.00	11170.0
50.00	54120.0
51.00	16912.0
51.90	652.0
52.80	404.0
54.90	981.0
55.90	4187.0
57.00	7947.0
57.90	392.0
60.00	3063.0
60.90	14988.0
62.00	13554.0
63.00	11029.0
63.90	1571.0
64.90	3167.0
65.80	260.0
66.90	904.0
68.00	28432.0
69.00	29384.0
70.00	2172.0
71.90	1694.0
73.00	13875.0
74.00	49200.0
75.00	148416.0
76.00	12436.0
76.90	1601.0
77.90	1139.0
78.80	9413.0
79.80	2473.0
80.90	9928.0
81.90	2077.0
82.90	314.0
85.70	520.0
86.90	11681.0
87.90	12314.0
91.00	1035.0
92.00	8306.0
93.00	13453.0
94.00	32952.0
95.00	286016.0
96.00	17160.0
97.00	521.0
102.70	161.0
103.80	1375.0
104.80	503.0
105.80	1466.0
106.70	306.0
109.80	302.0
110.70	364.0
111.70	185.0
112.80	274.0
114.90	256.0
115.80	918.0
116.90	2466.0
117.80	1215.0
118.90	1654.0
125.90	110.0
127.80	975.0
128.80	467.0
129.80	1080.0
130.80	504.0
134.80	618.0
136.80	721.0
138.90	174.0
140.00	244.0
140.90	3114.0
142.00	368.0
142.90	4063.0
143.80	348.0
144.80	803.0
145.70	450.0
146.90	194.0
147.80	828.0
148.70	231.0
149.80	241.0
151.80	249.0
152.80	175.0
153.80	268.0
154.90	839.0
155.90	217.0
156.90	413.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

158.00	102.0
158.70	144.0
160.70	248.0
170.10	153.0
170.80	289.0
171.90	3930.0
173.90	227520.0
175.00	18096.0
175.90	218112.0
176.90	13996.0
177.90	403.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028