

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070119\
 Data File : VU033120.D
 Acq On : 01 Jul 2019 17:24
 Operator : JC/SP
 Sample : K3599-07
 Misc : 7.92g/10mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAM16

Manual Integrations
 APPROVED

MMDadoda
 7/3/2019 9:03:00 AM

Quant Time: Jul 02 07:18:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 02 04:16:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.87	114	226973	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	223391	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	110781	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	53809	34.69	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.38%
7) Chloroethane-d5	1.64	69	35477	28.68	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	57.36%#
11) 1,1-Dichloroethene-d2	2.22	63	97387	31.16	ug/L	-0.05
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.32%
21) 2-Butanone-d5	4.19	46	145005	112.31	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	112.31%
24) Chloroform-d	4.63	84	138624	45.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.94%
26) 1,2-Dichloroethane-d4	5.30	65	101244	50.40	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.80%
32) Benzene-d6	5.32	84	261328	44.88	ug/L	-0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.76%
36) 1,2-Dichloropropane-d6	6.32	67	87679	47.26	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.52%
41) Toluene-d8	7.56	98	236483	43.36	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.72%
43) trans-1,3-Dichloropropene-	7.85	79	42296	43.83	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.66%
47) 2-Hexanone-d5	8.32	63	88742	102.45	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.45%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	142675	49.75	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.50%
64) 1,2-Dichlorobenzene-d4	11.86	152	99190	46.27	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.54%

Target Compounds				Ovalue
22) 2-Butanone	4.28	43	19445m	10.520 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU070119\
Data File : VU033120.D
Acq On : 01 Jul 2019 17:24
Operator : JC/SP
Sample : K3599-07
Misc : 7.92g/10mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 23 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
GAM16

Manual Integrations
APPROVED

MMDadoda
7/3/2019 9:03:00 AM

Quant Time: Jul 02 07:18:28 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 02 04:16:18 2019
Response via : Initial Calibration

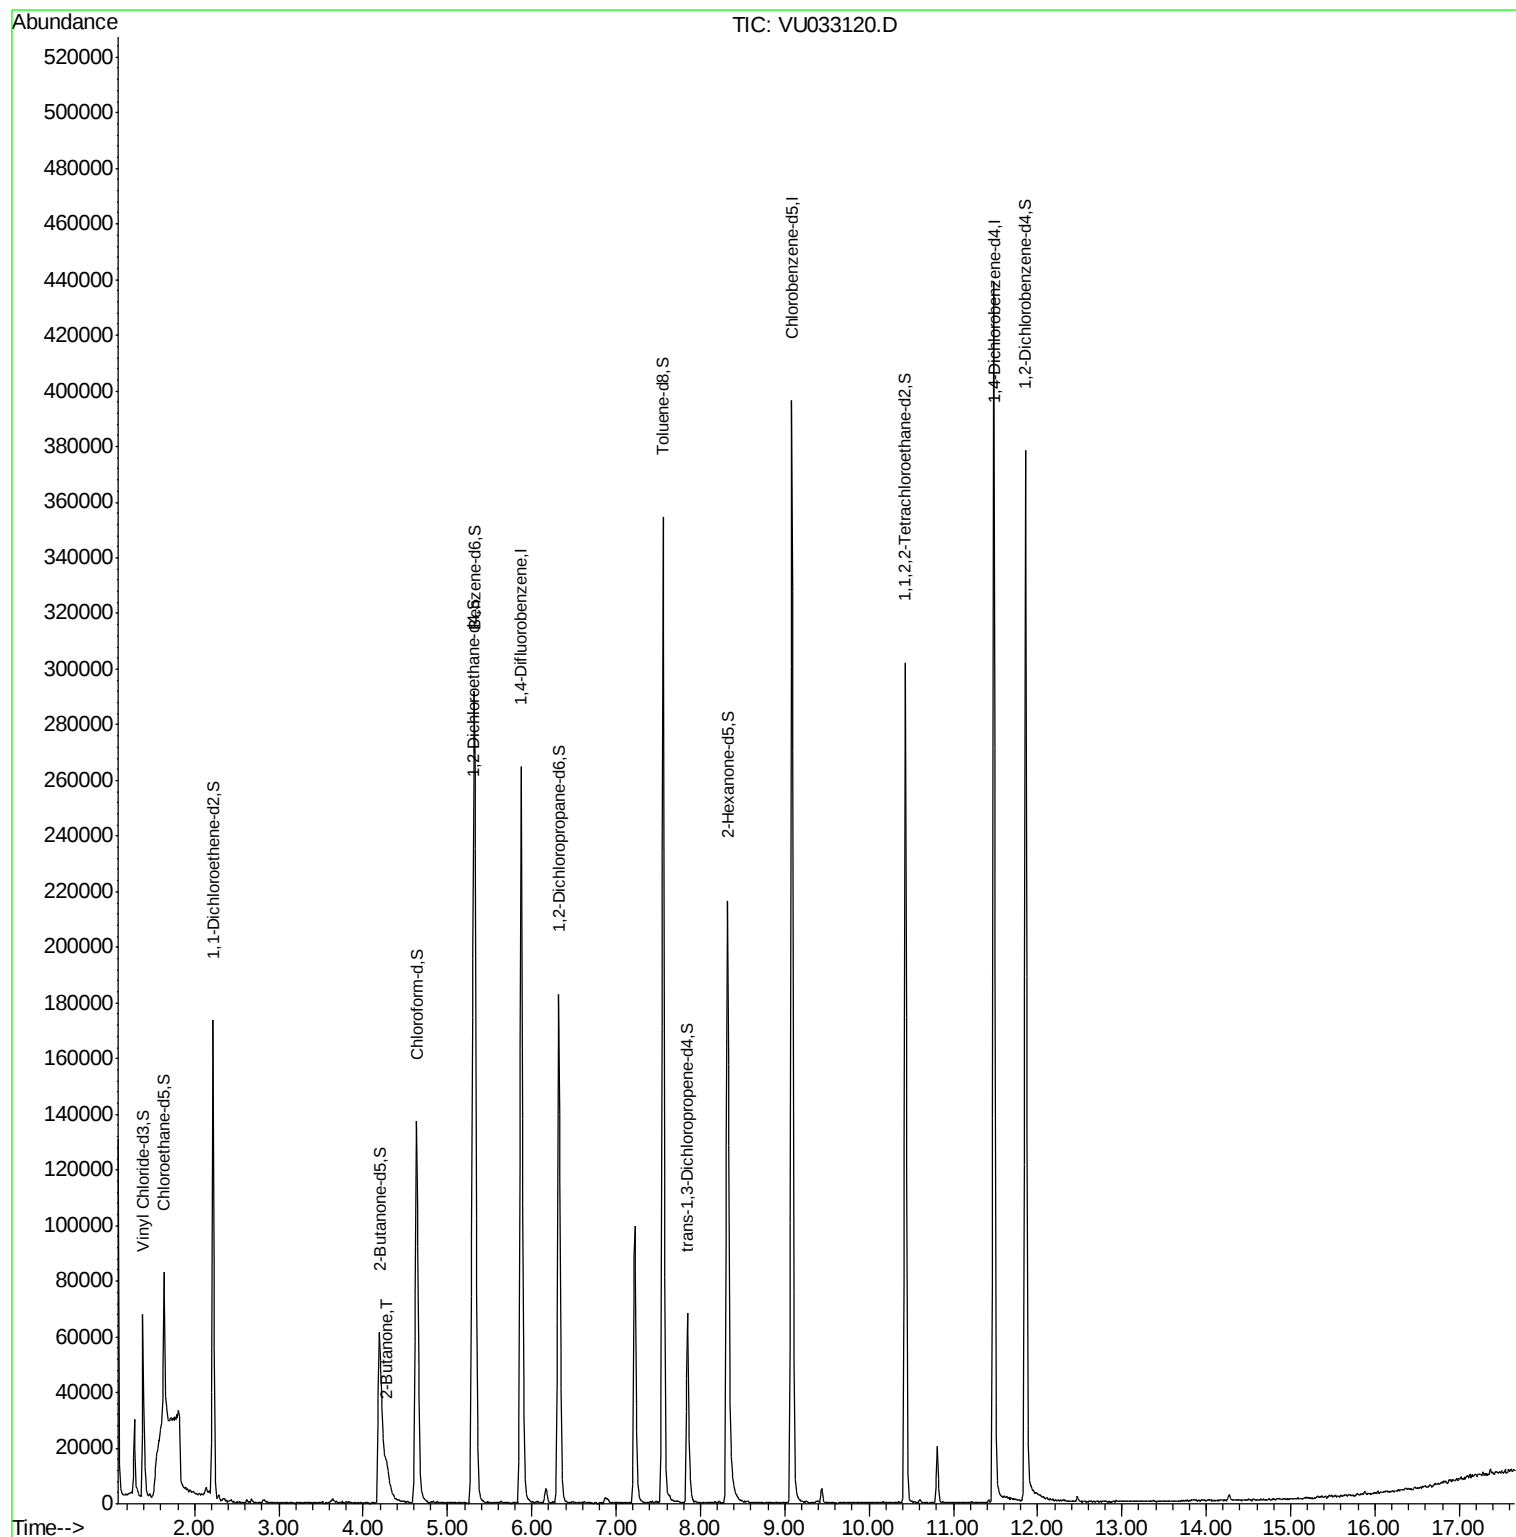

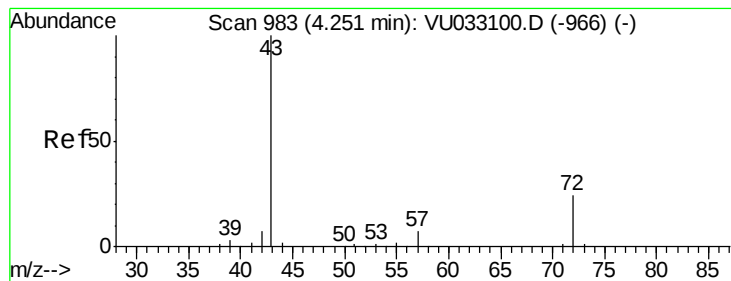

#22

2-Butanone

Concen: 10.520 ug/L m

RT: 4.28 min Scan# 993

Delta R.T. 0.03 min

Lab File: VU033120.D

Acq: 01 Jul 2019 17:24

Tot Ion: 43 Resp: 19445

Ion Ratio Lower Upper

43 100

72 10.2 12.9 38.6#

Instrument :

MSVOA_U

ClientSampleId :

GAM16

Manual Integrations

APPROVED

MMDadoda

7/3/2019 9:03:00 AM

