


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU070119\
Data File : VU033099.D
Acq On : 01 Jul 2019 08:29
Operator : JC/SP
Sample : BFB32
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB32

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Title : VOC Analysis
Last Update : Tue Jul 02 04:16:18 2019

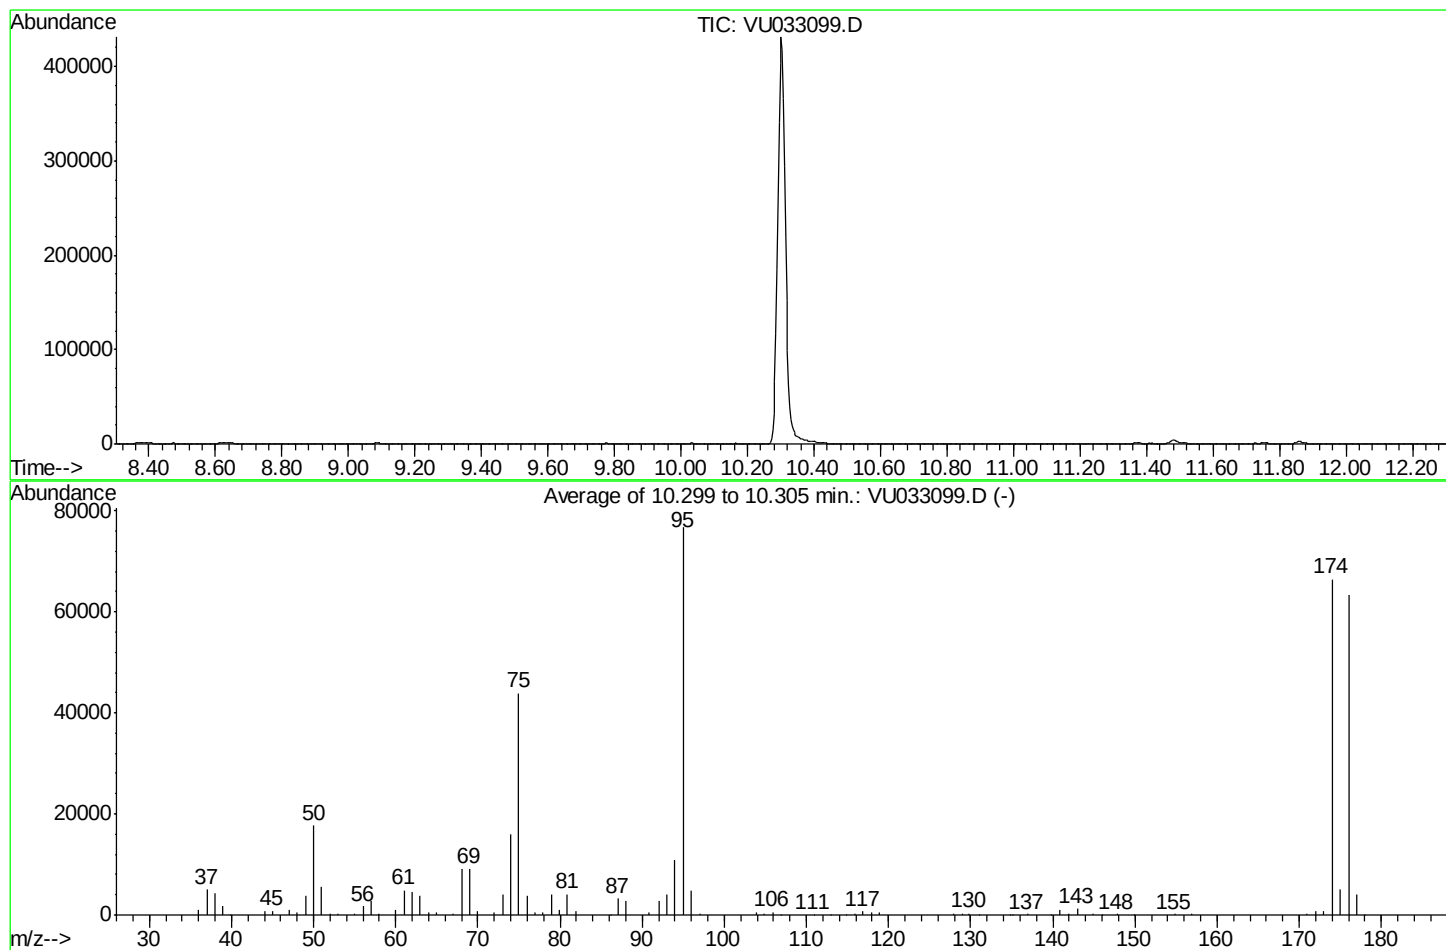

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	17653	PASS
75	95	30	80	57.1	43832	PASS
95	95	100	100	100.0	76709	PASS
96	95	5	9	6.4	4939	PASS
173	174	0.00	2	1.3	887	PASS
174	95	50	120	86.6	66392	PASS
175	174	5	9	7.7	5098	PASS
176	174	95	101	95.6	63445	PASS
177	176	5	9	6.5	4105	PASS

Scan 2853 (10.263 min): VU033099.D
BFB32

m/z	Abundance
39.90	164.0
44.00	234.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
36.00	958.0
37.00	4935.0
38.00	4361.0
39.00	1790.0
39.90	278.0
44.00	991.0
45.00	749.0
47.10	1049.0
47.90	599.0
49.00	3832.0
50.00	17256.0
51.00	5378.0
52.10	277.0
53.00	114.0
55.00	329.0
56.00	1641.0
57.00	2738.0
58.00	167.0
60.00	947.0
61.00	4778.0
62.00	4516.0
63.00	3650.0
64.00	527.0
65.00	431.0
67.00	270.0
68.00	8644.0
69.00	8928.0
70.00	667.0
72.00	511.0
73.00	4140.0
74.00	15647.0
75.00	42896.0
76.00	3933.0
77.00	565.0
78.00	362.0
78.90	3898.0
79.90	918.0
80.90	4161.0
81.90	863.0
87.00	3091.0
87.90	2755.0
90.90	431.0
92.00	2591.0
93.00	4080.0
94.00	10456.0
95.00	74448.0
96.00	4821.0
97.00	144.0
103.90	458.0
104.80	208.0
105.90	545.0
110.90	124.0
113.00	129.0
114.80	102.0
116.00	333.0
116.90	595.0
118.00	407.0
118.90	601.0
127.90	292.0
128.90	126.0
129.90	306.0
131.00	133.0
134.80	163.0
136.90	159.0
139.80	112.0
140.90	1033.0
142.00	112.0
143.00	1157.0
144.90	205.0
145.90	124.0
147.80	180.0
149.90	117.0
154.80	163.0
157.00	176.0
171.00	112.0
171.90	699.0
173.00	941.0
174.00	63008.0
175.00	4857.0
176.00	59512.0
177.00	3871.0
177.90	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
36.00	985.0
37.00	5221.0
38.00	4415.0
39.00	1844.0
39.90	305.0
44.00	1007.0
45.00	796.0
47.10	1106.0
47.90	591.0
49.00	3891.0
50.00	18248.0
51.00	5653.0
52.00	268.0
53.00	161.0
55.00	372.0
56.00	1753.0
57.00	2794.0
58.00	175.0
60.00	958.0
61.00	4910.0
62.00	4646.0
63.00	3880.0
64.00	522.0
65.00	498.0
67.00	252.0
68.00	9389.0
69.00	9432.0
70.00	725.0
72.00	593.0
73.00	4255.0
74.00	16488.0
75.00	45424.0
76.00	3963.0
77.00	545.0
78.00	416.0
78.90	4129.0
79.90	972.0
80.90	4287.0
81.90	926.0
86.10	128.0
87.00	3356.0
88.00	3000.0
90.80	420.0
92.00	2731.0
93.00	4326.0
94.00	11170.0
95.00	79400.0
96.00	5100.0
97.00	144.0
103.90	505.0
104.80	189.0
105.90	584.0
106.80	116.0
110.90	125.0
113.00	103.0
114.80	123.0
115.90	404.0
116.90	719.0
118.00	427.0
118.90	649.0
127.90	310.0
129.00	149.0
129.90	317.0
131.00	117.0
134.80	138.0
136.90	174.0
139.80	101.0
140.90	1124.0
142.00	178.0
143.00	1266.0
144.90	218.0
146.00	148.0
147.90	173.0
149.90	141.0
154.80	244.0
156.90	172.0
170.90	138.0
172.00	868.0
173.00	899.0
174.00	68704.0
175.00	5288.0
176.00	65512.0
177.00	4256.0
177.90	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
36.00	902.0
37.00	4879.0
38.00	4128.0
39.00	1769.0
39.90	268.0
44.00	944.0
45.00	790.0
47.10	1005.0
47.90	536.0
49.00	3598.0
50.00	17456.0
51.00	5391.0
52.10	232.0
53.00	164.0
54.90	374.0
56.00	1616.0
57.00	2681.0
58.00	155.0
60.00	899.0
61.00	4770.0
62.00	4551.0
63.00	3873.0
64.00	484.0
65.00	516.0
67.10	260.0
68.00	9180.0
69.00	9058.0
70.00	678.0
72.00	577.0
73.00	4071.0
74.00	15686.0
75.00	43176.0
76.00	3695.0
77.00	475.0
77.90	399.0
78.90	4028.0
80.00	922.0
80.90	4026.0
81.90	855.0
86.10	120.0
87.00	3272.0
88.00	2986.0
90.80	387.0
92.00	2689.0
93.00	4106.0
94.00	10813.0
95.00	76280.0
96.00	4897.0
97.00	140.0
103.90	473.0
104.80	131.0
105.90	533.0
106.80	128.0
110.90	121.0
114.80	120.0
115.90	381.0
116.90	752.0
118.00	413.0
118.90	625.0
127.90	284.0
128.90	183.0
129.80	311.0
135.10	133.0
136.90	159.0
140.90	1120.0
142.00	178.0
143.00	1255.0
144.90	225.0
146.00	126.0
147.90	194.0
149.80	118.0
154.80	263.0
156.90	180.0
170.80	147.0
171.10	146.0
172.00	916.0
173.00	821.0
174.00	67464.0
175.00	5149.0
176.00	65312.0
177.00	4189.0
177.90	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32