
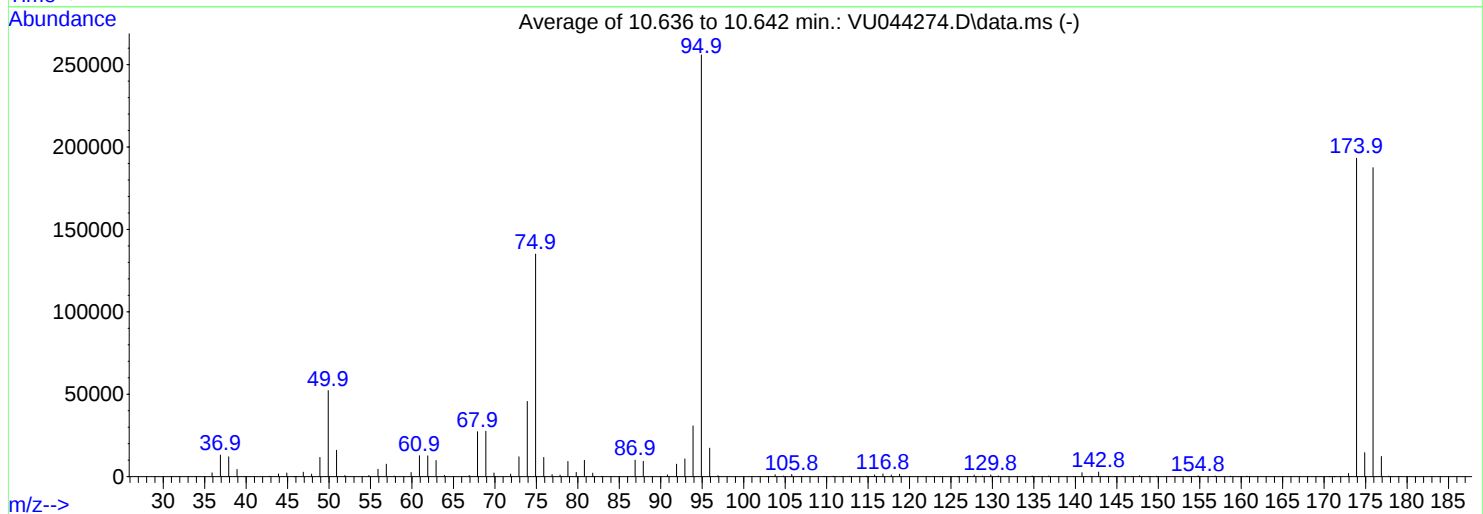


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070121\
 Data File : VU044274.D
 Acq On : 01 Jul 2021 09:03
 Operator : SY/MD
 Sample : BFB48
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB508

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR062121WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Jul 03 04:56:00 2021

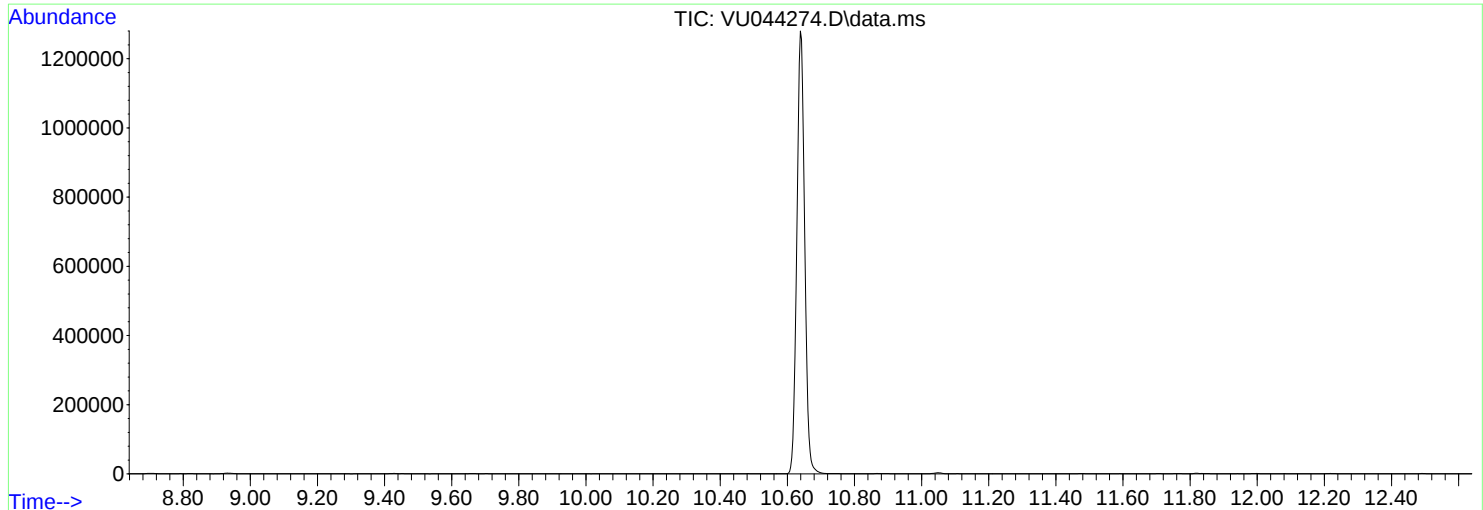

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	52197	PASS
75	95	30	80	52.8	135085	PASS
95	95	100	100	100.0	255957	PASS
96	95	5	9	6.7	17267	PASS
173	174	0.00	2	1.0	1989	PASS
174	95	50	120	75.5	193259	PASS
175	174	5	9	7.6	14604	PASS
176	174	95	101	97.0	187499	PASS
177	176	5	9	6.5	12252	PASS

m/z	Abundance
35.90	2442.0
36.90	13468.0
37.90	12454.0
38.90	4547.0
39.80	238.0
41.00	111.0
42.80	208.0
43.90	2097.0
44.90	2287.0
46.10	194.0
46.90	2883.0
47.90	1635.0
48.90	12062.0
49.90	53928.0
50.90	16520.0
51.90	671.0
54.80	747.0
55.90	4648.0
56.90	7827.0
57.90	419.0
59.90	2600.0
60.90	13054.0
61.90	12894.0
62.90	10186.0
63.90	808.0
66.90	736.0
67.90	28136.0
68.90	28424.0
69.90	2315.0
71.90	1592.0
72.90	12361.0
73.90	47104.0
74.90	139200.0
75.90	12084.0
76.90	1326.0
77.80	1035.0
78.80	9586.0
79.80	2714.0
80.80	10202.0
81.80	2229.0
82.80	249.0
86.00	274.0
86.90	10421.0
87.90	9543.0
90.80	1079.0
91.90	7835.0
92.90	11072.0
93.90	31680.0
94.90	264384.0
95.90	17864.0
96.90	604.0
102.70	122.0
103.80	1253.0
104.80	384.0
105.80	1400.0
106.80	257.0
109.70	230.0
110.80	295.0
111.80	146.0
112.80	316.0
114.80	255.0
115.80	1095.0
116.80	1691.0
117.80	1057.0
118.80	1482.0
123.70	124.0
126.80	112.0
127.80	978.0
128.80	453.0
129.80	1069.0
130.70	496.0
134.80	365.0
136.80	464.0
139.80	194.0
140.80	2446.0
141.80	311.0
142.80	2881.0
143.80	174.0
144.80	233.0
145.80	342.0
146.80	192.0
147.70	537.0
148.80	199.0
149.80	313.0
151.70	141.0
152.80	187.0
153.80	182.0
154.80	646.0
156.90	402.0
158.70	267.0
160.70	266.0
172.90	2056.0

Instrument :
MSVOA_U
ClientSampleId :
BFB508

173.90	199616.0
174.90	15143.0
175.90	193280.0
176.90	12636.0
177.80	363.0

Instrument :
MSVOA_U
ClientSampleId :
BFB508

m/z	Abundance
35.90	2365.0
36.90	13129.0
37.90	12166.0
38.90	4312.0
39.80	262.0
42.80	198.0
43.90	2075.0
44.90	2097.0
45.80	171.0
46.90	2722.0
47.90	1648.0
48.90	11682.0
49.90	51952.0
50.90	15925.0
51.90	608.0
54.80	726.0
55.90	4469.0
56.90	7477.0
57.90	337.0
59.90	2578.0
60.90	12700.0
61.90	12655.0
62.90	9844.0
63.90	781.0
66.90	703.0
67.90	27072.0
68.90	27440.0
69.90	2083.0
71.90	1575.0
72.90	12182.0
73.90	45648.0
74.90	135232.0
75.90	11383.0
76.90	1354.0
77.80	1033.0
78.80	9236.0
79.80	2634.0
80.80	10102.0
81.80	2205.0
82.80	245.0
86.00	248.0
86.90	9938.0
87.90	9237.0
90.80	1122.0
91.90	7687.0
92.90	11177.0
93.90	30912.0
94.90	257792.0
95.90	17168.0
96.90	514.0
102.80	134.0
103.80	1216.0
104.80	385.0
105.80	1357.0
106.80	272.0
109.70	251.0
110.80	306.0
111.70	173.0
112.80	287.0
114.80	260.0
115.80	1011.0
116.80	1620.0
117.80	1045.0
118.80	1457.0
123.70	104.0
126.80	115.0
127.80	892.0
128.80	440.0
129.80	1129.0
130.70	483.0
134.80	399.0
136.80	436.0
139.80	213.0
140.80	2468.0
141.80	288.0
142.80	2860.0
143.80	134.0
144.80	270.0
145.70	335.0
146.80	186.0
147.80	589.0
148.80	154.0
149.80	297.0
151.70	144.0
152.80	199.0
153.80	177.0
154.80	622.0
156.90	396.0
158.70	315.0
160.70	269.0
170.60	100.0
173.00	2028.0

Instrument :
MSVOA_U
ClientSampleId :
BFB508

173.90	199040.0
174.90	14567.0
175.90	194432.0
176.90	12408.0
177.80	352.0

Instrument :
MSVOA_U
ClientSampleId :
BFB508

m/z	Abundance
39.80	132.0
43.90	344.0

Instrument :
MSVOA_U
ClientSampleId :
BFB508

m/z	Abundance
35.90	2277.0
36.90	12704.0
37.90	11566.0
38.90	4393.0
39.80	233.0
41.00	100.0
42.80	213.0
43.90	1985.0
44.90	2275.0
46.00	200.0
46.90	2669.0
47.90	1485.0
48.90	11265.0
49.90	50712.0
50.90	15762.0
51.90	650.0
54.80	704.0
55.90	4326.0
56.90	7492.0
57.80	421.0
59.90	2432.0
60.90	12359.0
61.90	12258.0
62.90	9572.0
63.90	847.0
66.90	720.0
67.90	26584.0
68.90	26808.0
69.90	2281.0
71.90	1479.0
72.90	11497.0
73.90	44296.0
74.90	130824.0
75.90	11574.0
76.90	1284.0
77.90	965.0
78.80	8994.0
79.80	2468.0
80.80	9547.0
81.80	2051.0
82.90	231.0
86.00	228.0
86.90	9668.0
87.90	9211.0
90.80	945.0
91.90	7160.0
92.90	10168.0
93.90	29616.0
94.90	245696.0
95.90	16768.0
96.90	623.0
102.70	124.0
103.80	1168.0
104.80	355.0
105.80	1269.0
106.80	228.0
109.70	189.0
110.80	260.0
111.90	115.0
112.80	289.0
114.80	252.0
115.80	1044.0
116.80	1604.0
117.80	957.0
118.80	1363.0
123.70	138.0
125.80	105.0
127.80	967.0
128.80	417.0
129.80	920.0
130.70	406.0
134.80	348.0
136.80	434.0
139.80	171.0
140.80	2273.0
141.90	307.0
142.80	2646.0
143.80	197.0
144.80	166.0
145.80	326.0
146.80	177.0
147.70	516.0
148.80	233.0
149.80	294.0
151.80	137.0
152.70	175.0
153.80	162.0
154.80	545.0
156.80	374.0
158.70	211.0
160.70	238.0
171.20	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB508

172.90	1883.0
173.90	181120.0
174.90	14101.0
175.90	174784.0
176.90	11711.0
177.80	317.0

Instrument :
MSVOA_U
ClientSampleId :
BFB508