


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070122\
Data File : VU049579.D
Acq On : 01 Jul 2022 12:57
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Title : SW846 8260
Last Update : Tue Jun 28 10:35:43 2022

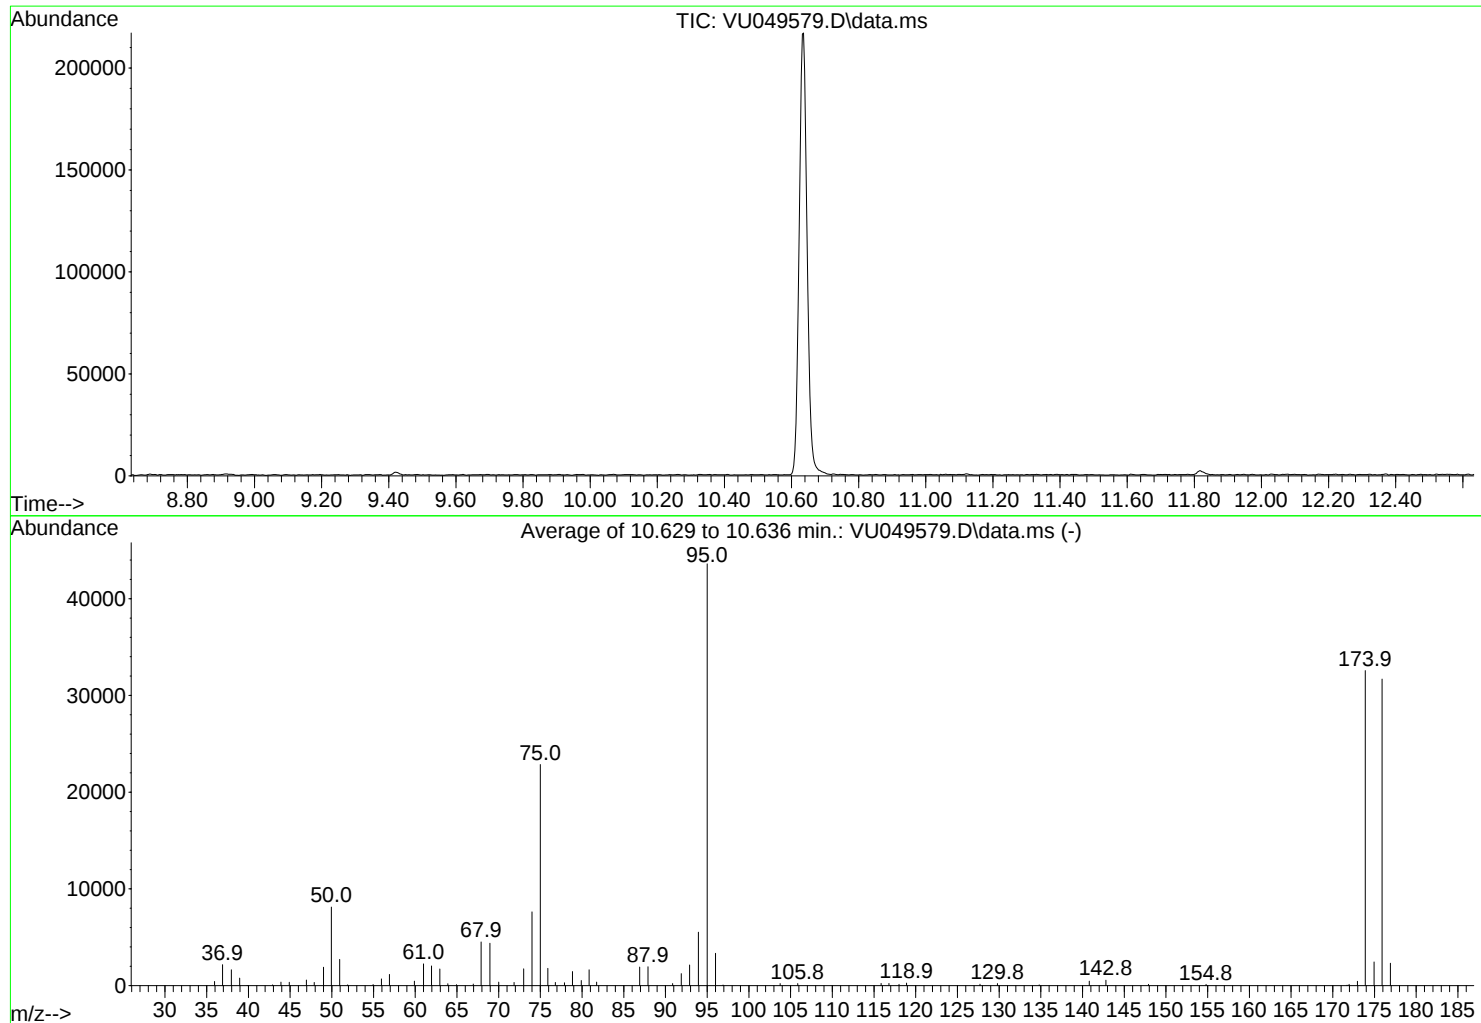

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	8125	PASS
75	95	30	60	52.4	22856	PASS
95	95	100	100	100.0	43603	PASS
96	95	5	9	7.7	3349	PASS
173	174	0.00	2	1.4	445	PASS
174	95	50	100	74.7	32568	PASS
175	174	5	9	7.5	2449	PASS
176	174	95	101	97.3	31693	PASS
177	176	5	9	7.3	2319	PASS