


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU070124\  
Data File : VU059692.D  
Acq On : 01 Jul 2024 18:05  
Operator : MD/SY  
Sample : P3084-05  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
E1GC8

Manual IntegrationsAPPROVED

Quant Time: Jul 02 01:40:08 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR061724WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Jun 29 01:51:23 2024  
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024  
Supervised By :Semsettin Yesilyurt 07/05/2024

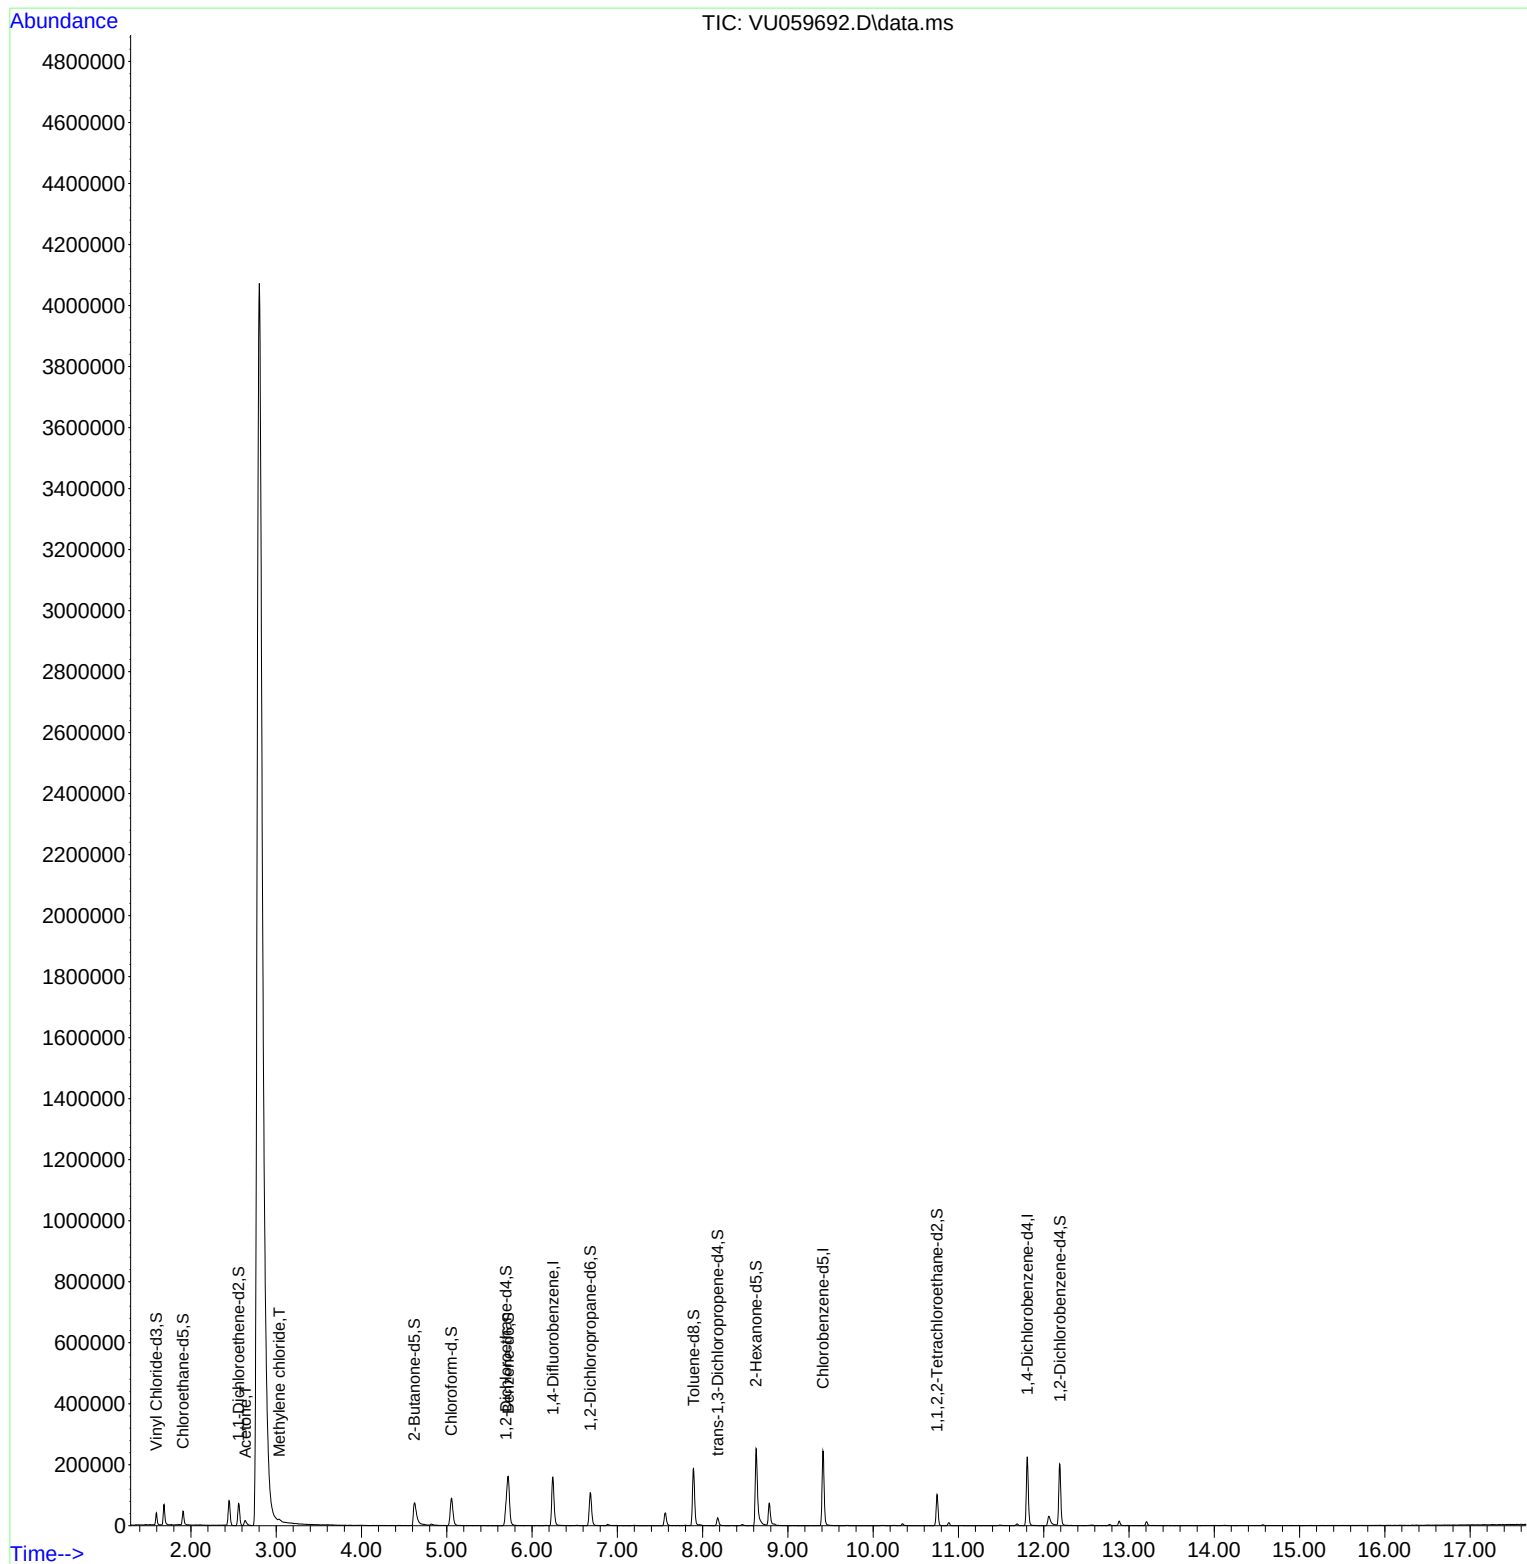




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU070124\  
Data File : VU059692.D  
Acq On : 01 Jul 2024 18:05  
Operator : MD/SY  
Sample : P3084-05  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
E1GC8

Manual IntegrationsAPPROVED

Quant Time: Jul 02 01:40:08 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR061724WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Jun 29 01:51:23 2024  
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024  
Supervised By :Semsettin Yesilyurt 07/05/2024

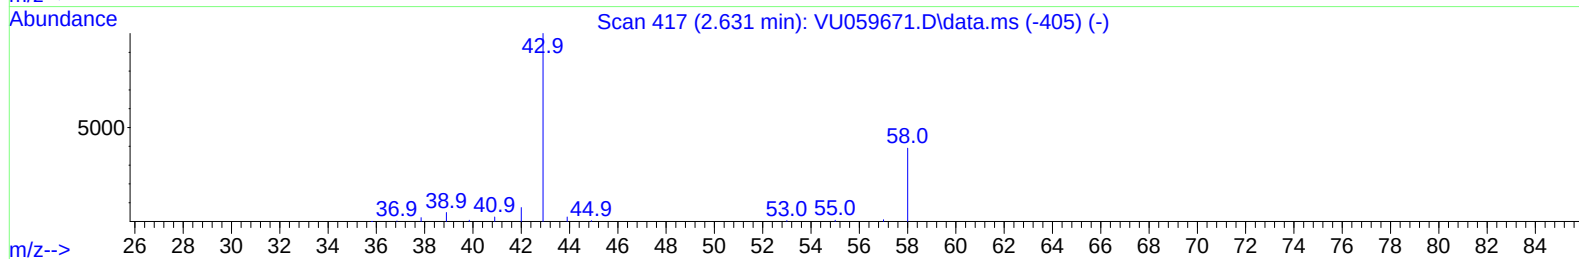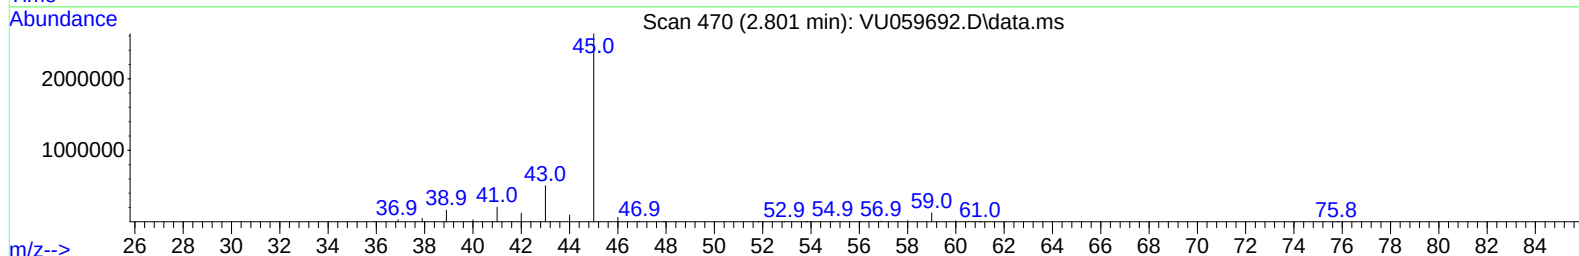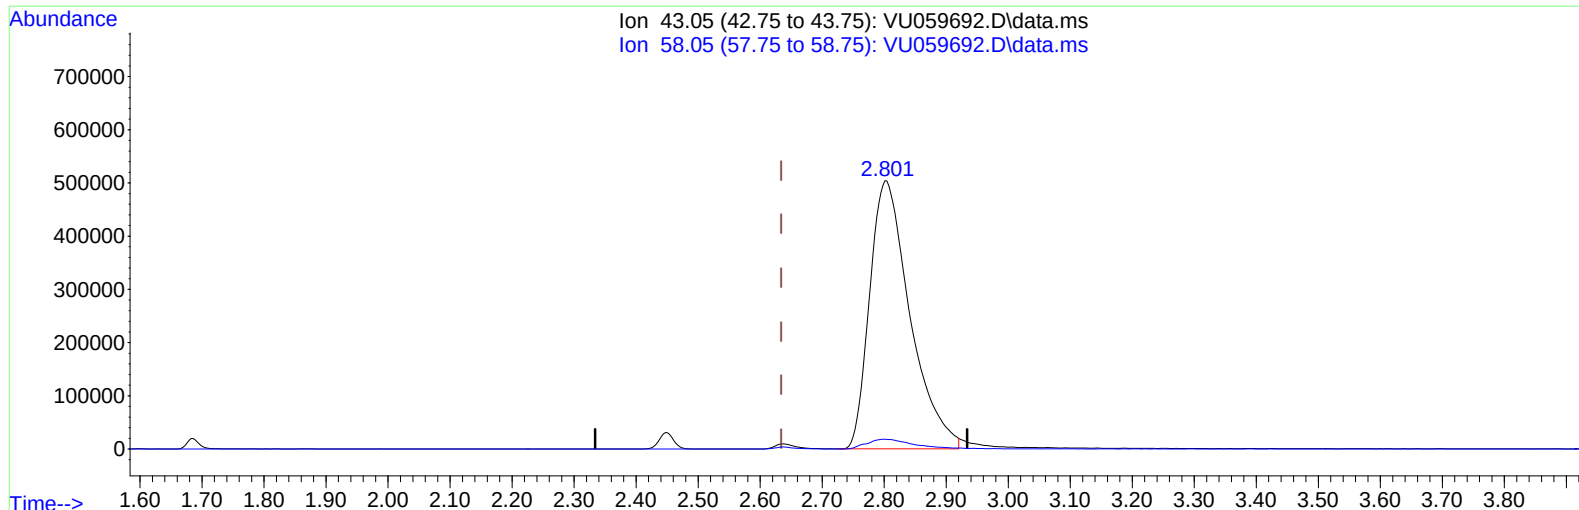

TIC: VU059692.D\data.ms

(13) Acetone (T)

2.801min (+ 0.167) 1814.25 ug/L

response 2272263

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 34.00  | 4.21   |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU070124\  
Data File : VU059692.D  
Acq On : 01 Jul 2024 18:05  
Operator : MD/SY  
Sample : P3084-05  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
E1GC8

Manual IntegrationsAPPROVED

Quant Time: Jul 02 01:40:08 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR061724WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Jun 29 01:51:23 2024  
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024  
Supervised By :Semsettin Yesilyurt 07/05/2024

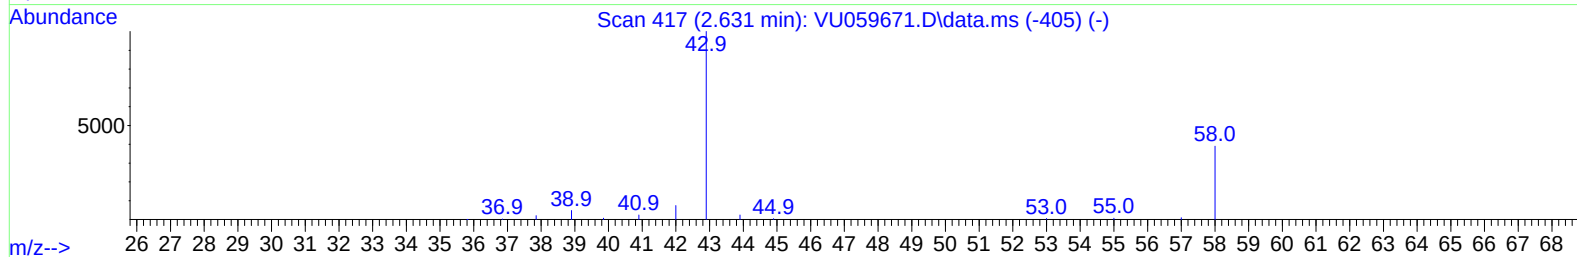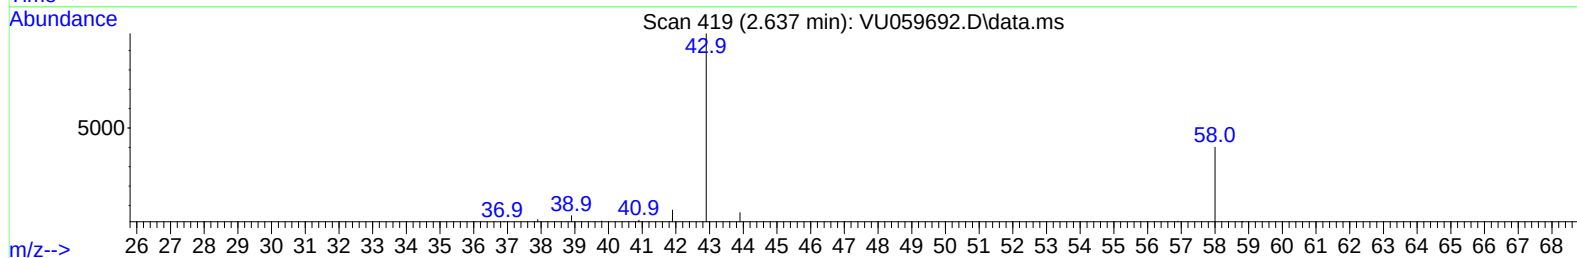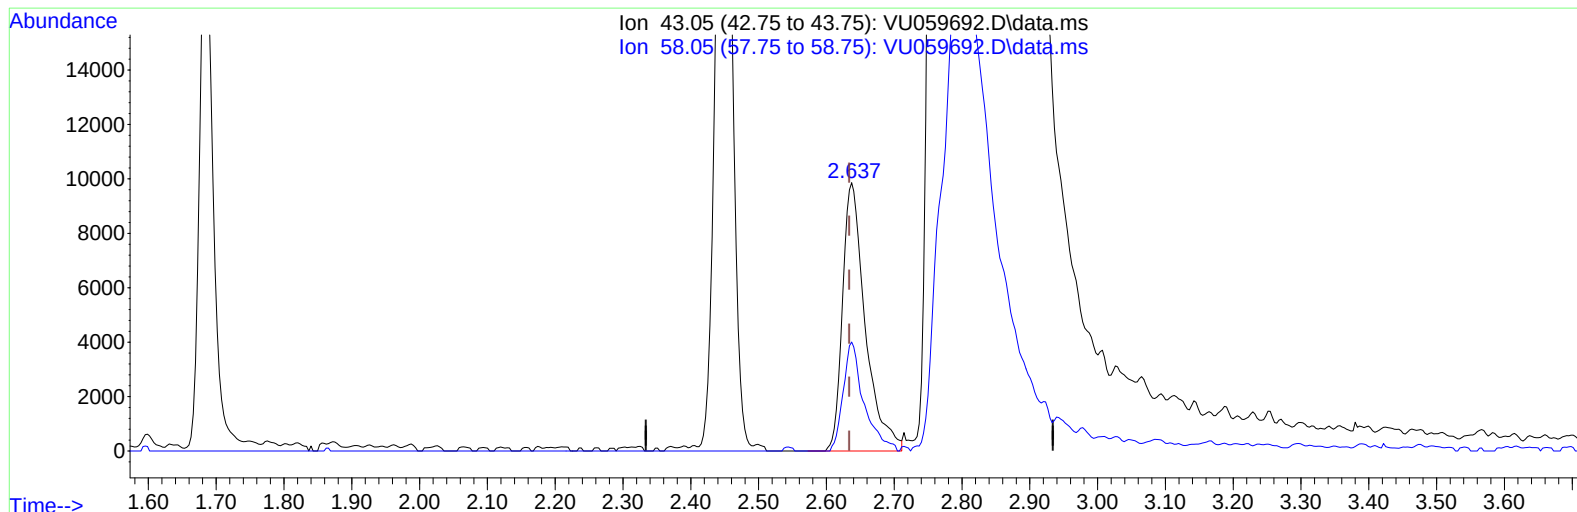

TIC: VU059692.D\data.ms

(13) Acetone (T)

2.637min (+ 0.003) 18.35 ug/L m

response 22977

| Ion   | Exp%   | Act%    |
|-------|--------|---------|
| 43.05 | 100.00 | 100.00  |
| 58.05 | 34.00  | 416.02# |
| 0.00  | 0.00   | 0.00    |
| 0.00  | 0.00   | 0.00    |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU070124\  
 Data File : VU059692.D  
 Acq On : 01 Jul 2024 18:05  
 Operator : MD/SY  
 Sample : P3084-05  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 E1GC8

Manual IntegrationsAPPROVED

Quant Time: Jul 02 01:40:08 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR061724WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Jun 29 01:51:23 2024  
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024  
 Supervised By :Semsettin Yesilyurt 07/05/2024

| Compound                      | R.T.   | QIon           | Response | Conc   | Units    | Dev(Min) |
|-------------------------------|--------|----------------|----------|--------|----------|----------|
| Internal Standards            |        |                |          |        |          |          |
| 1) 1,4-Difluorobenzene        | 6.245  | 114            | 134799   | 5.000  | ug/L     | 0.00     |
| 28) Chlorobenzene-d5          | 9.412  | 117            | 145233   | 5.000  | ug/L     | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.807 | 152            | 65014    | 5.000  | ug/L     | 0.00     |
| System Monitoring Compounds   |        |                |          |        |          |          |
| 4) Vinyl Chloride-d3          | 1.595  | 65             | 29393    | 3.136  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 40 - 130 | Recovery | =      | 62.800%  |          |
| 7) Chloroethane-d5            | 1.907  | 69             | 34625    | 3.839  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 130 | Recovery | =      | 76.800%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.560  | 65             | 13845    | 3.560  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 125 | Recovery | =      | 71.200%  |          |
| 20) 2-Butanone-d5             | 4.621  | 46             | 116755   | 60.471 | ug/L     | 0.00     |
| Spiked Amount                 | 50.000 | Range 40 - 130 | Recovery | =      | 120.940% |          |
| 24) Chloroform-d              | 5.055  | 84             | 87283    | 4.537  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 90.800%  |          |
| 26) 1,2-Dichloroethane-d4     | 5.695  | 65             | 43343    | 4.677  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 93.600%  |          |
| 32) Benzene-d6                | 5.721  | 84             | 161353   | 4.037  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 80.800%  |          |
| 36) 1,2-Dichloropropane-d6    | 6.685  | 67             | 54741    | 4.469  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 140 | Recovery | =      | 89.400%  |          |
| 41) Toluene-d8                | 7.894  | 98             | 133124   | 3.583  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 71.600%  |          |
| 43) trans-1,3-Dichloroprop... | 8.177  | 79             | 15754    | 4.108  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 55 - 130 | Recovery | =      | 82.200%  |          |
| 46) 2-Hexanone-d5             | 8.627  | 63             | 86844    | 54.497 | ug/L     | 0.00     |
| Spiked Amount                 | 50.000 | Range 45 - 130 | Recovery | =      | 109.000% |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.749 | 84             | 52595    | 5.197  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 120 | Recovery | =      | 104.000% |          |
| 66) 1,2-Dichlorobenzene-d4    | 12.190 | 152            | 56838    | 4.912  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 80 - 120 | Recovery | =      | 98.200%  |          |
| Target Compounds              |        |                |          |        |          |          |
| 13) Acetone                   | 2.637  | 43             | 22977m   | 18.346 | ug/L     |          |
| 16) Methylene chloride        | 3.036  | 84             | 2083     | 0.184  | ug/L     | 90       |

(#) = qualifier out of range (m) = manual integration (+) = signals summed