

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059694.D
Acq On : 01 Jul 2024 18:53
Operator : MD/SY
Sample : P3084-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE4


Manual IntegrationsAPPROVED

Quant Time: Jul 02 01:40:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

07/05/2024
Supervised By :Semsettin
Yesilyurt

07/05/2024

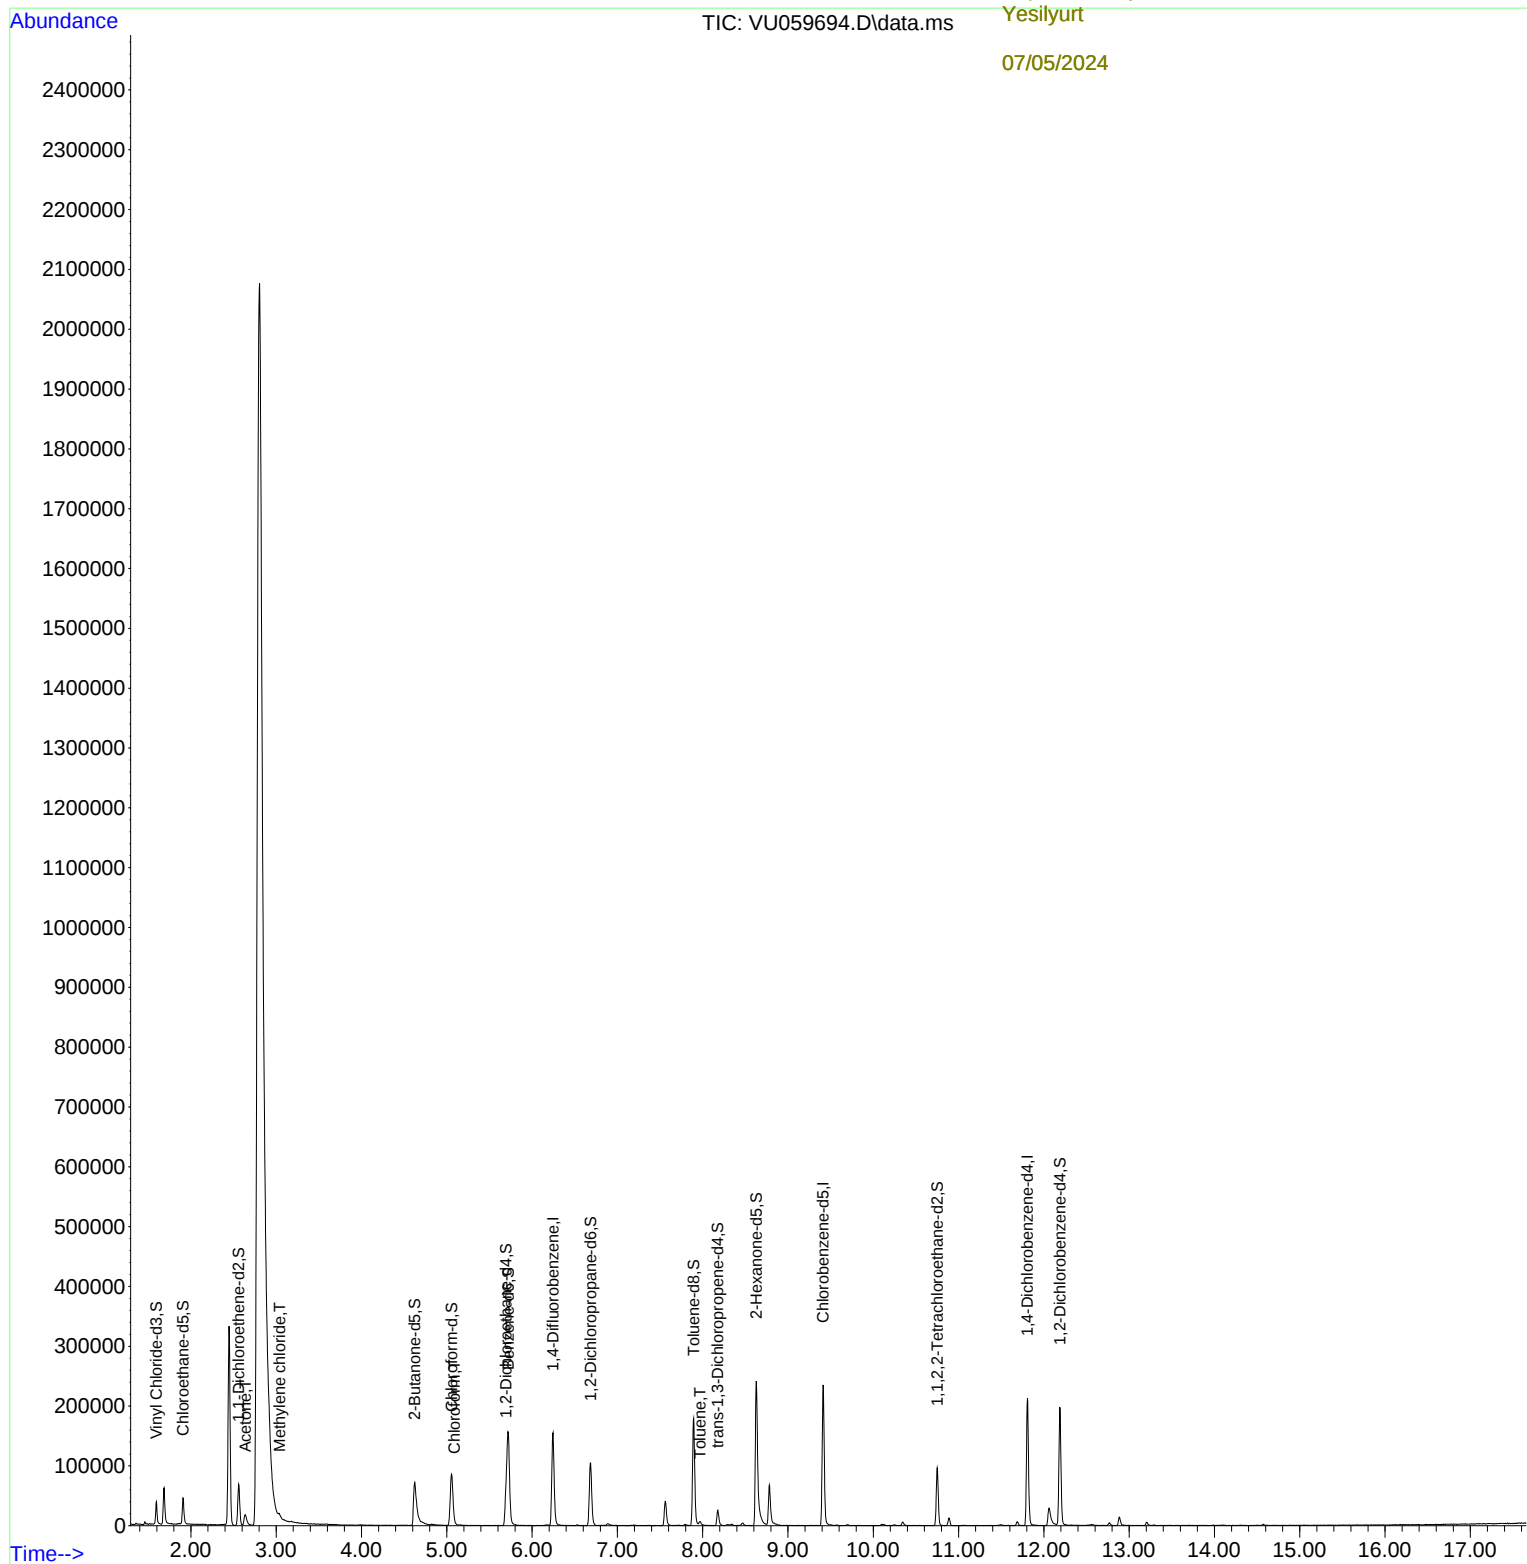

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059694.D
Acq On : 01 Jul 2024 18:53
Operator : MD/SY
Sample : P3084-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1




Instrument :
MSVOA_U
ClientSampleId :
E1GE4

Manual IntegrationsAPPROVED

Quant Time: Jul 02 01:40:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

07/05/2024
Supervised By :Semsettin
Yesilyurt

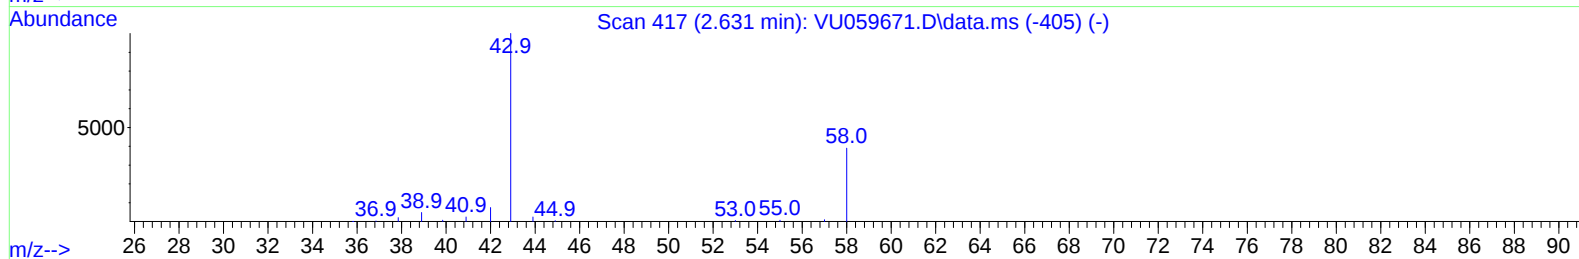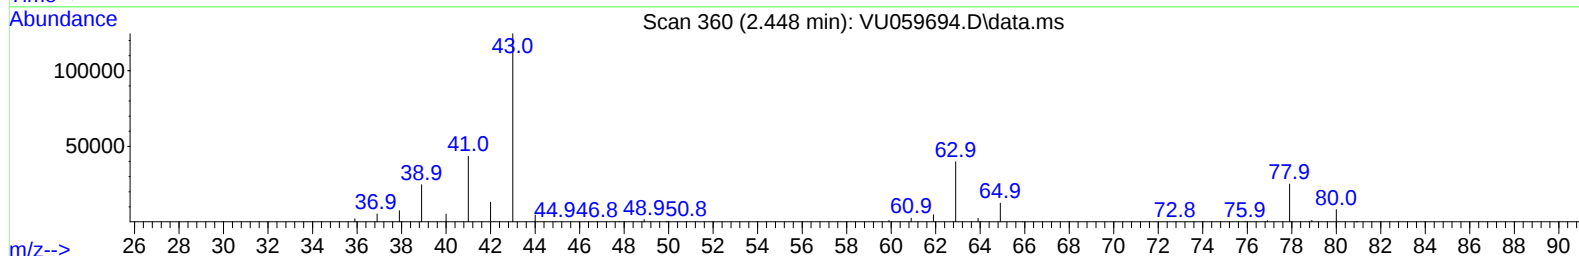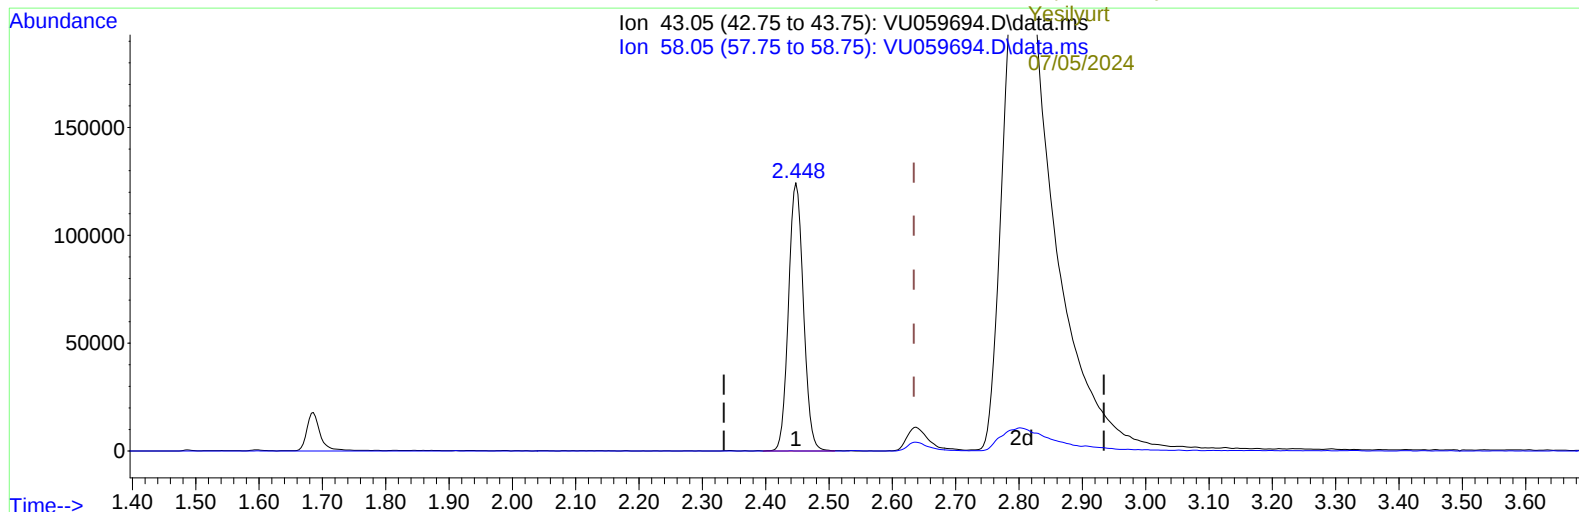

TIC: VU059694.D\data.ms

(13) Acetone (T)

2.448min (-0.186) 167.85 ug/L

response 203821

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	4.86
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059694.D
Acq On : 01 Jul 2024 18:53
Operator : MD/SY
Sample : P3084-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1




Instrument :
MSVOA_U
ClientSampleId :
E1GE4

Manual IntegrationsAPPROVED

Quant Time: Jul 02 01:40:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

07/05/2024
Supervised By :Semsettin
Yesilyurt

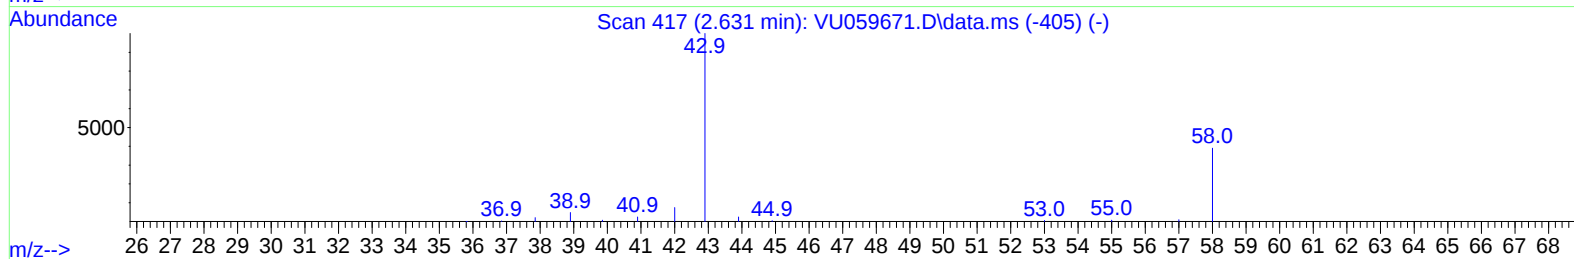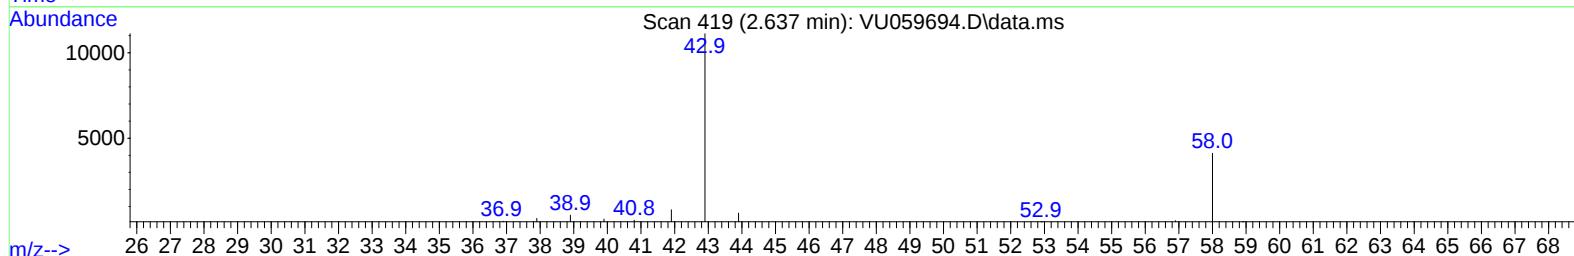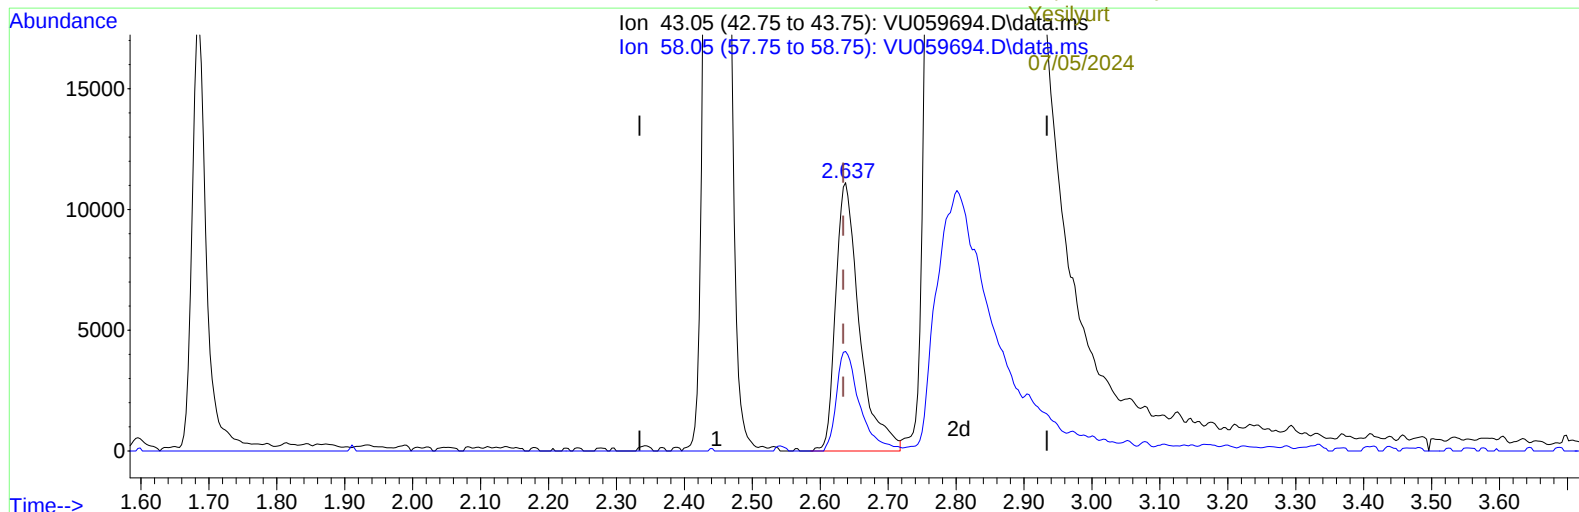

TIC: VU059694.D\data.ms

(13) Acetone (T)

2.637min (+ 0.003) 22.28 ug/L m

response 27054

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	36.59
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
 Data File : VU059694.D
 Acq On : 01 Jul 2024 18:53
 Operator : MD/SY
 Sample : P3084-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GE4

Manual IntegrationsAPPROVED

Quant Time: Jul 02 01:40:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 29 01:51:23 2024
 Response via : Initial Calibration

Reviewed By :Mahesh
 Dadoda

07/05/2024
 Supervised By :Semsettin
 Yesilyurt

07/05/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	130694	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	139694	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	61578	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	27977	3.079	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	61.600%
7) Chloroethane-d5	1.907	69	31920	3.650	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	73.000%
11) 1,1-Dichloroethene-d2	2.560	65	12984	3.444	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.800%
20) 2-Butanone-d5	4.624	46	115658	61.784	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	123.560%
24) Chloroform-d	5.055	84	82953	4.447	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
26) 1,2-Dichloroethane-d4	5.695	65	42596	4.741	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
32) Benzene-d6	5.721	84	156382	4.068	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.400%
36) 1,2-Dichloropropane-d6	6.685	67	53370	4.530	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.600%
41) Toluene-d8	7.894	98	127655	3.572	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.400%
43) trans-1,3-Dichloroprop...	8.177	79	15418	4.179	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.600%
46) 2-Hexanone-d5	8.627	63	82755	53.990	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.980%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	51083	5.248	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.000%
66) 1,2-Dichlorobenzene-d4	12.187	152	56832	5.185	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.800%
Target Compounds						
					Qvalue	
13) Acetone	2.637	43	27054m	22.279	ug/L	
16) Methylene chloride	3.039	84	2397	0.218	ug/L	96
25) Chloroform	5.087	83	4178	0.223	ug/L	88
42) Toluene	7.968	91	5467	0.122	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed