


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059717.D
Acq On : 02 Jul 2024 04:28
Operator : MD/SY
Sample : P3121-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COBM6

Manual IntegrationsAPPROVED

Quant Time: Jul 02 07:22:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

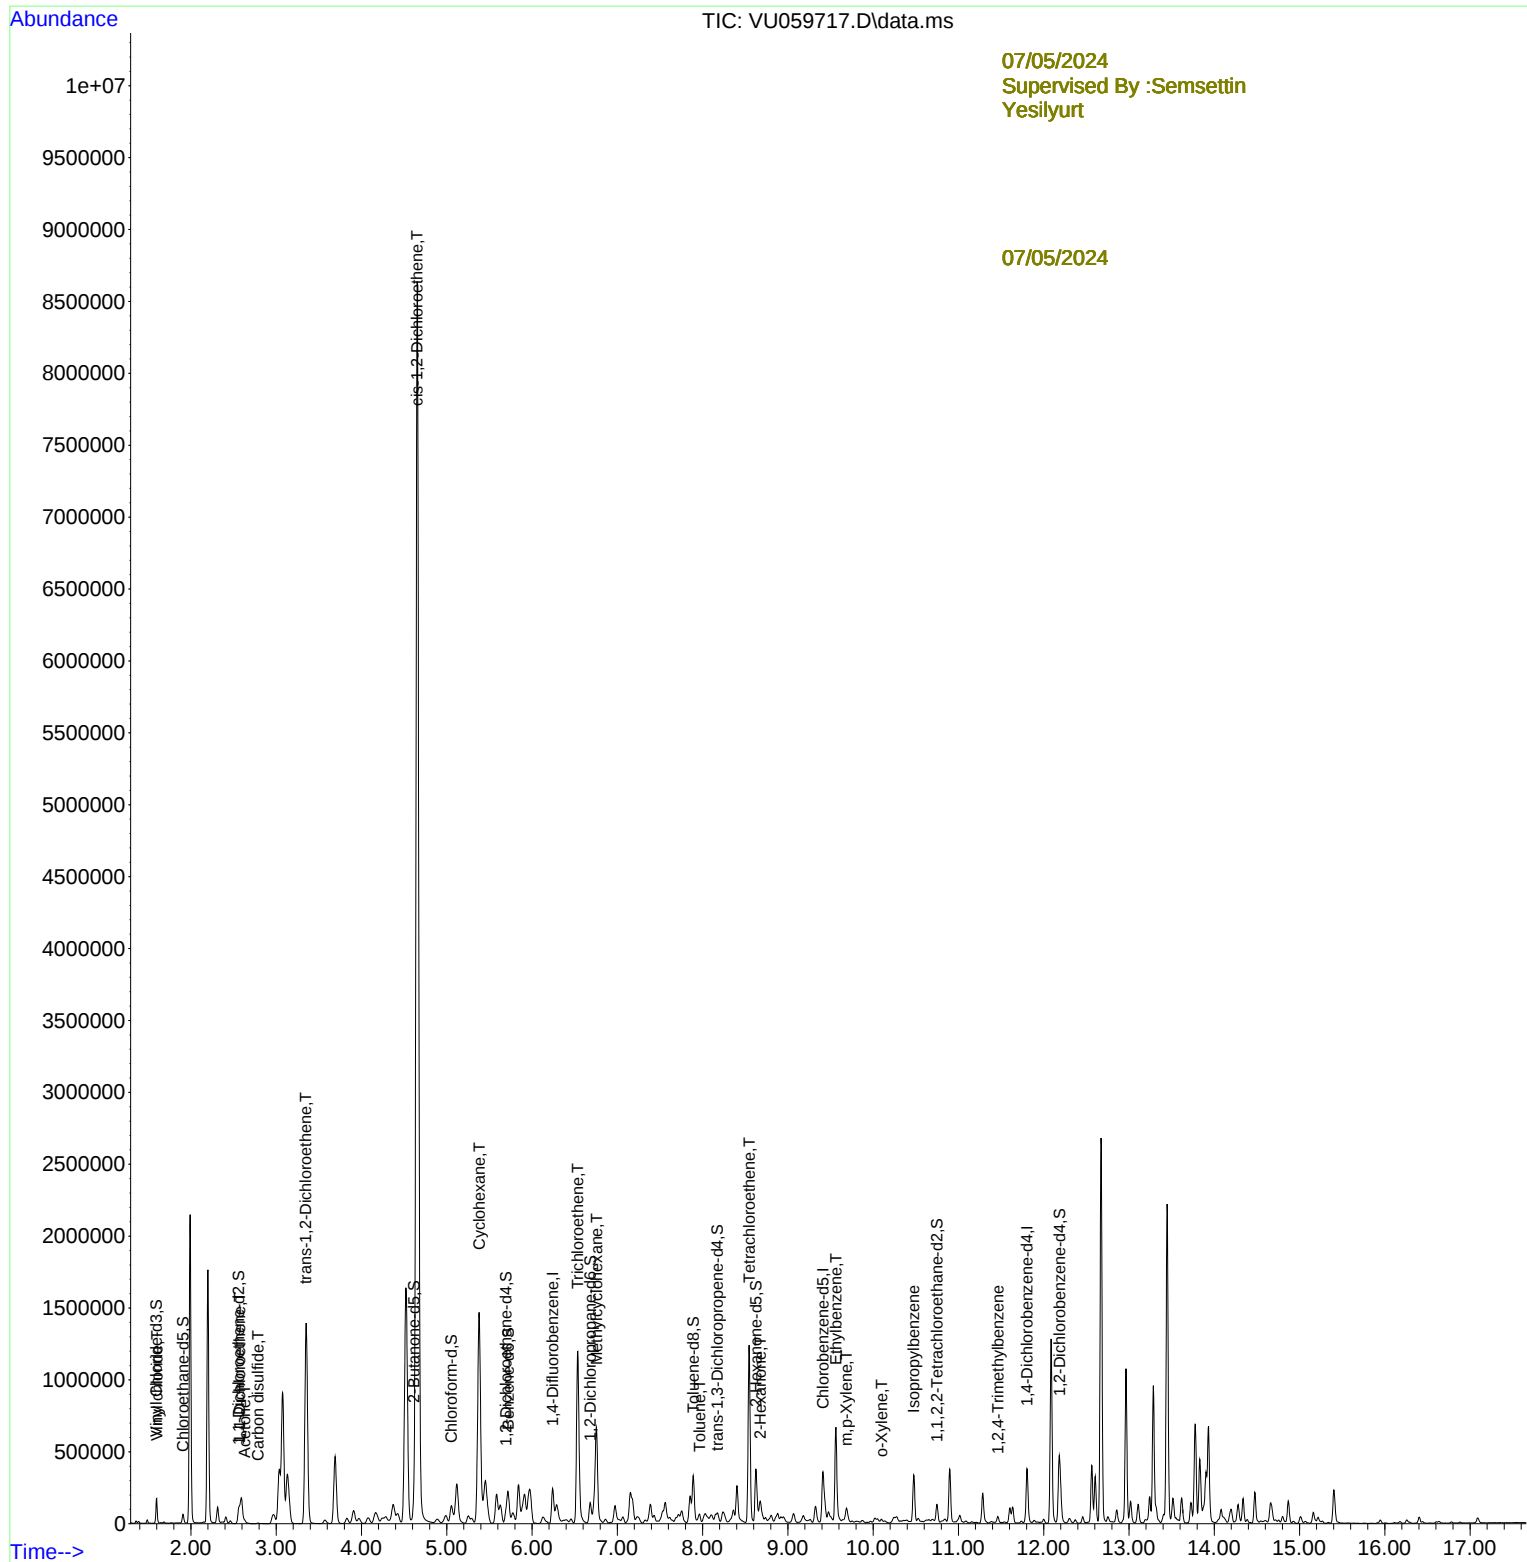




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059717.D
Acq On : 02 Jul 2024 04:28
Operator : MD/SY
Sample : P3121-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COBM6

Manual IntegrationsAPPROVED

Quant Time: Jul 02 07:22:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

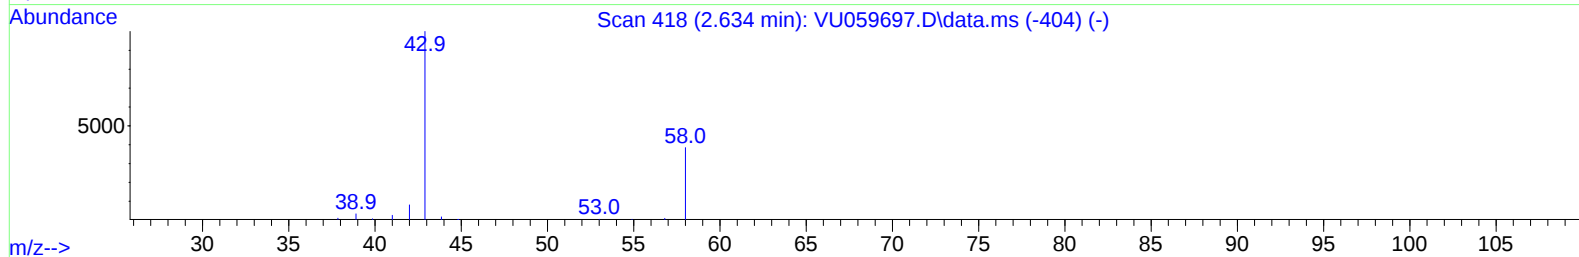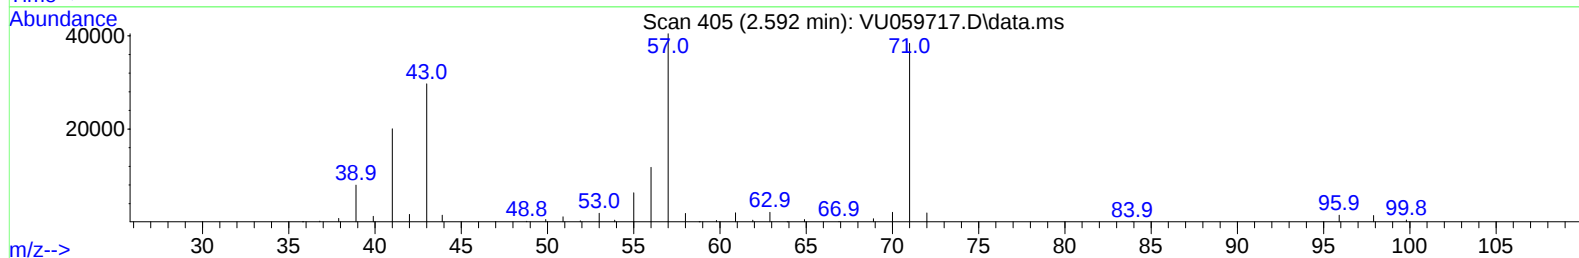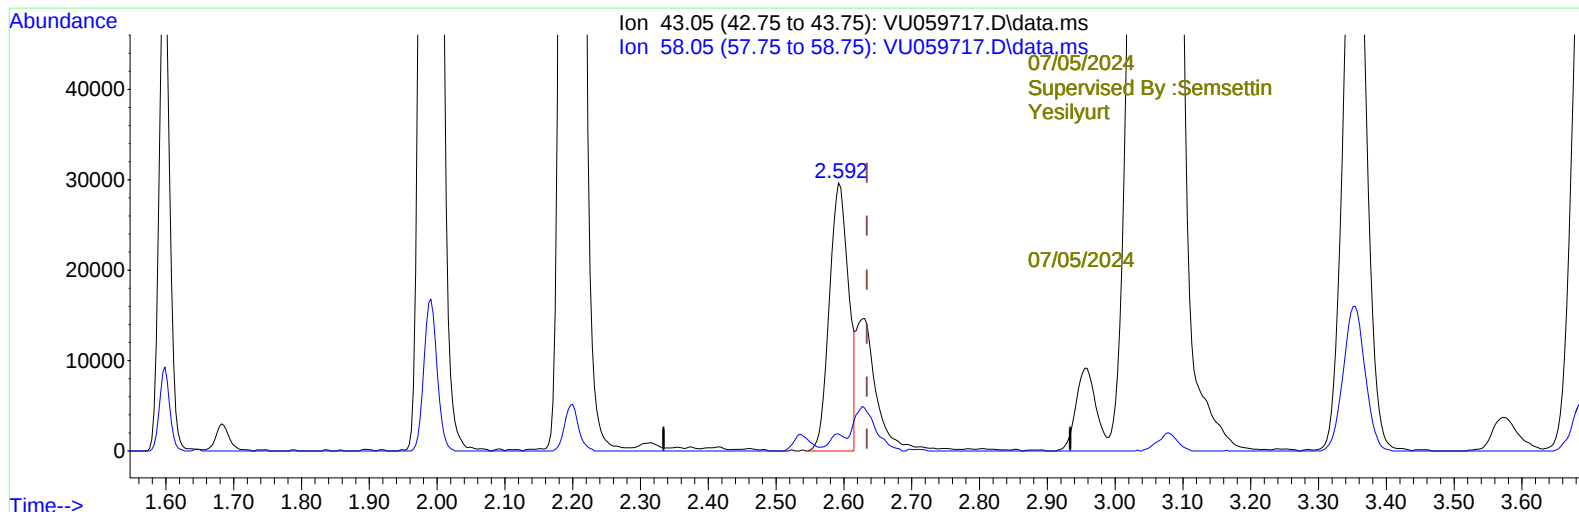

TIC: VU059717.D\data.ms

(13) Acetone (T)

2.592min (-0.042) 29.48 ug/L

response 58492

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	5.31
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059717.D
Acq On : 02 Jul 2024 04:28
Operator : MD/SY
Sample : P3121-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COBM6

Manual IntegrationsAPPROVED

Quant Time: Jul 02 07:22:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

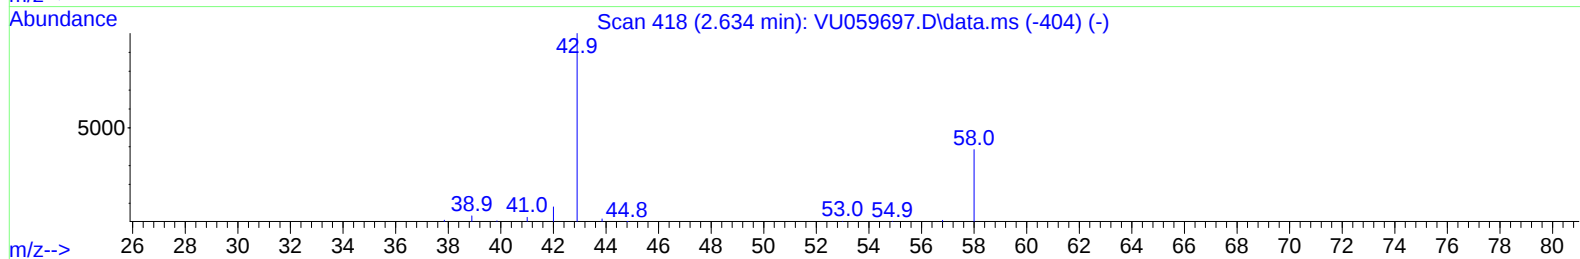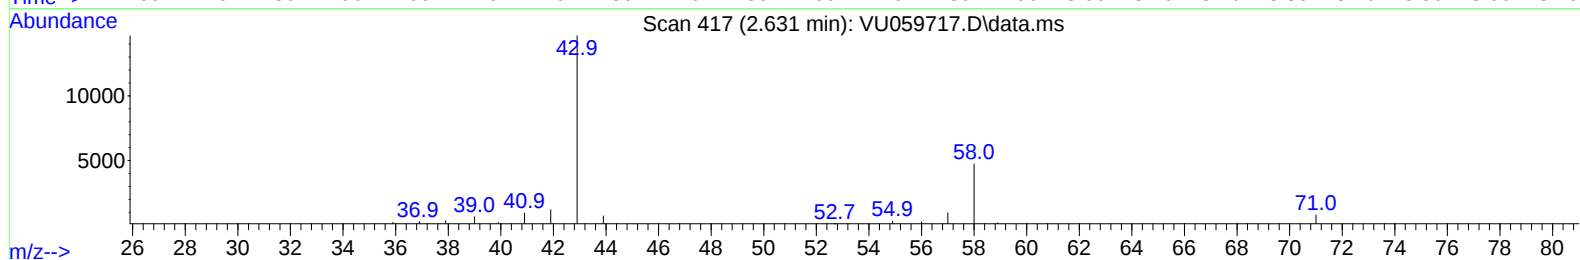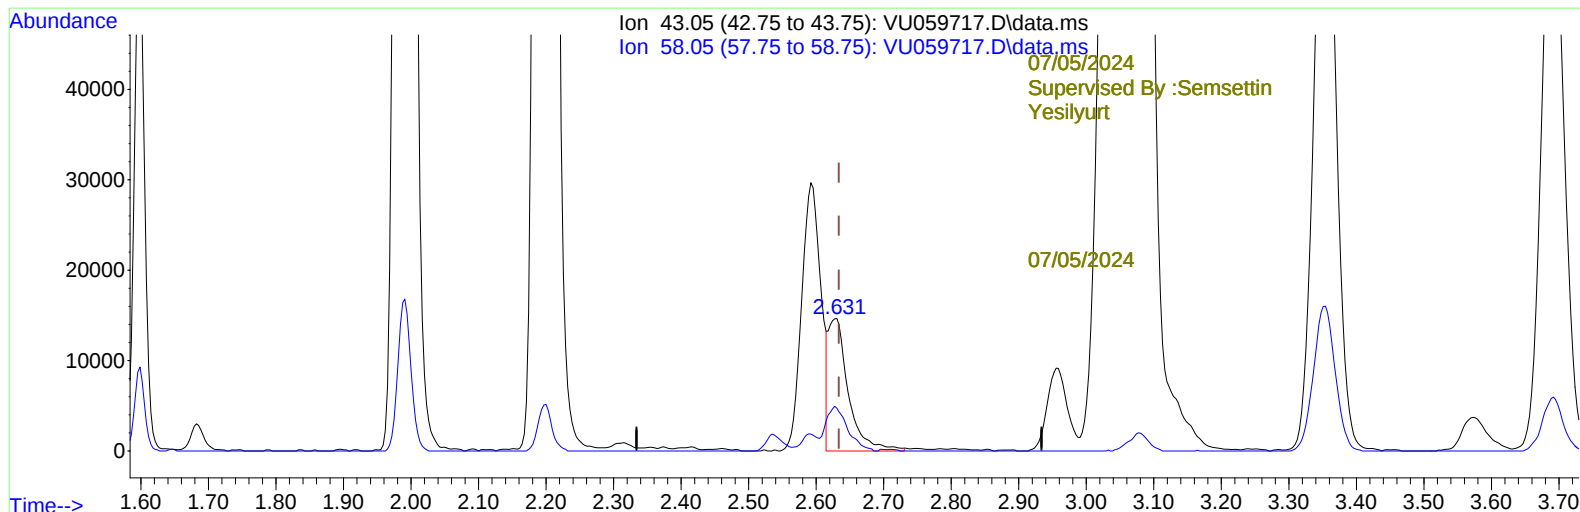

TIC: VU059717.D\data.ms

(13) Acetone (T)

2.631min (-0.003) 15.24 ug/L m

response 30228

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	10.28
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
 Data File : VU059717.D
 Acq On : 02 Jul 2024 04:28
 Operator : MD/SY
 Sample : P3121-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COBM6

Manual IntegrationsAPPROVED

Quant Time: Jul 02 07:22:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 29 01:51:23 2024
 Response via : Initial Calibration

Reviewed By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	213514	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	203351	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	107216	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	35486	2.390	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	47.800%	
7) Chloroethane-d5	1.907	69	42392	2.968	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	59.400%#	
11) 1,1-Dichloroethene-d2	2.560	65	18639	3.026	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	60.600%	
20) 2-Butanone-d5	4.618	46	166565	54.465	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	108.920%	
24) Chloroform-d	5.055	84	112994	3.708	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	74.200%	
26) 1,2-Dichloroethane-d4	5.695	65	55447	3.777	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	75.600%	
32) Benzene-d6	5.721	84	224136	4.005	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	80.000%	
36) 1,2-Dichloropropane-d6	6.682	67	71676	4.180	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	83.600%	
41) Toluene-d8	7.891	98	208402	4.006	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	80.200%	
43) trans-1,3-Dichloroprop...	8.174	79	22801	4.246	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	85.000%	
46) 2-Hexanone-d5	8.624	63	142501	63.866	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	127.740%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	62920	4.441	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	88.800%	
66) 1,2-Dichlorobenzene-d4	12.187	152	85094	4.459	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	89.200%	
Target Compounds						
5) Vinyl chloride	1.602	62	9004	0.419	ug/L	90
12) 1,1-Dichloroethene	2.573	96	8557	0.565	ug/L #	1
13) Acetone	2.631	43	30228m	15.237	ug/L	
14) Carbon disulfide	2.788	76	5056	0.100	ug/L	99
18) trans-1,2-Dichloroethene	3.345	96	124671	7.916	ug/L	91
22) cis-1,2-Dichloroethene	4.653	96	4751576	273.727	ug/L	96
30) Cyclohexane	5.380	56	771959	37.235	ug/L #	90
34) Trichloroethene	6.534	95	364365	21.787	ug/L	96
35) Methylcyclohexane	6.756	83	290623	12.213	ug/L	99
42) Toluene	7.965	91	38602	0.590	ug/L	98
47) Tetrachloroethene	8.547	164	287586	22.161	ug/L	96
48) 2-Hexanone	8.675	43	24412	4.619	ug/L #	40
52) Ethylbenzene	9.563	91	466127	6.950	ug/L	96
53) m,p-Xylene	9.685	106	22466	0.872	ug/L	91
54) o-Xylene	10.100	106	4972	0.203	ug/L	96
60) Isopropylbenzene	10.476	105	203792	3.077	ug/L	98
63) 1,2,4-Trimethylbenzene	11.463	105	23567	0.470	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059717.D
Acq On : 02 Jul 2024 04:28
Operator : MD/SY
Sample : P3121-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Jul 02 07:22:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
C0BM6

Manual IntegrationsAPPROVED

Reviewed By :Mahesh
Dadoda

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

(#)=qualifier out of range (m)=manual integration (+)=signals summed							

07/05/2024
Supervised By :Semsettin
Yesilyurt

07/05/2024