

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
 Data File : VU059699.D
 Acq On : 01 Jul 2024 21:17
 Operator : MD/SY
 Sample : P3121-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BF3

Quant Time: Jul 02 03:54:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 29 01:51:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	129352	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	138440	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	58841	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	30577	3.400	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	68.000%	
7) Chloroethane-d5	1.907	69	34852	4.027	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	80.600%	
11) 1,1-Dichloroethene-d2	2.560	65	13199	3.537	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	70.800%	
20) 2-Butanone-d5	4.624	46	111664	60.270	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	120.540%	
24) Chloroform-d	5.055	84	82359	4.461	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	89.200%	
26) 1,2-Dichloroethane-d4	5.695	65	41960	4.718	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.400%	
32) Benzene-d6	5.721	84	156091	4.097	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	82.000%	
36) 1,2-Dichloropropane-d6	6.685	67	53270	4.563	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	91.200%	
41) Toluene-d8	7.894	98	123691	3.492	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	69.800%#	
43) trans-1,3-Dichloroprop...	8.177	79	14381	3.934	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	78.600%	
46) 2-Hexanone-d5	8.627	63	81276	53.506	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	107.020%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	49924	5.175	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	103.600%	
66) 1,2-Dichlorobenzene-d4	12.190	152	51590	4.926	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.600%	
Target Compounds						Qvalue
16) Methylene chloride	3.042	84	1887	0.174	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059699.D
Acq On : 01 Jul 2024 21:17
Operator : MD/SY
Sample : P3121-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BF3


Quant Time: Jul 02 03:54:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

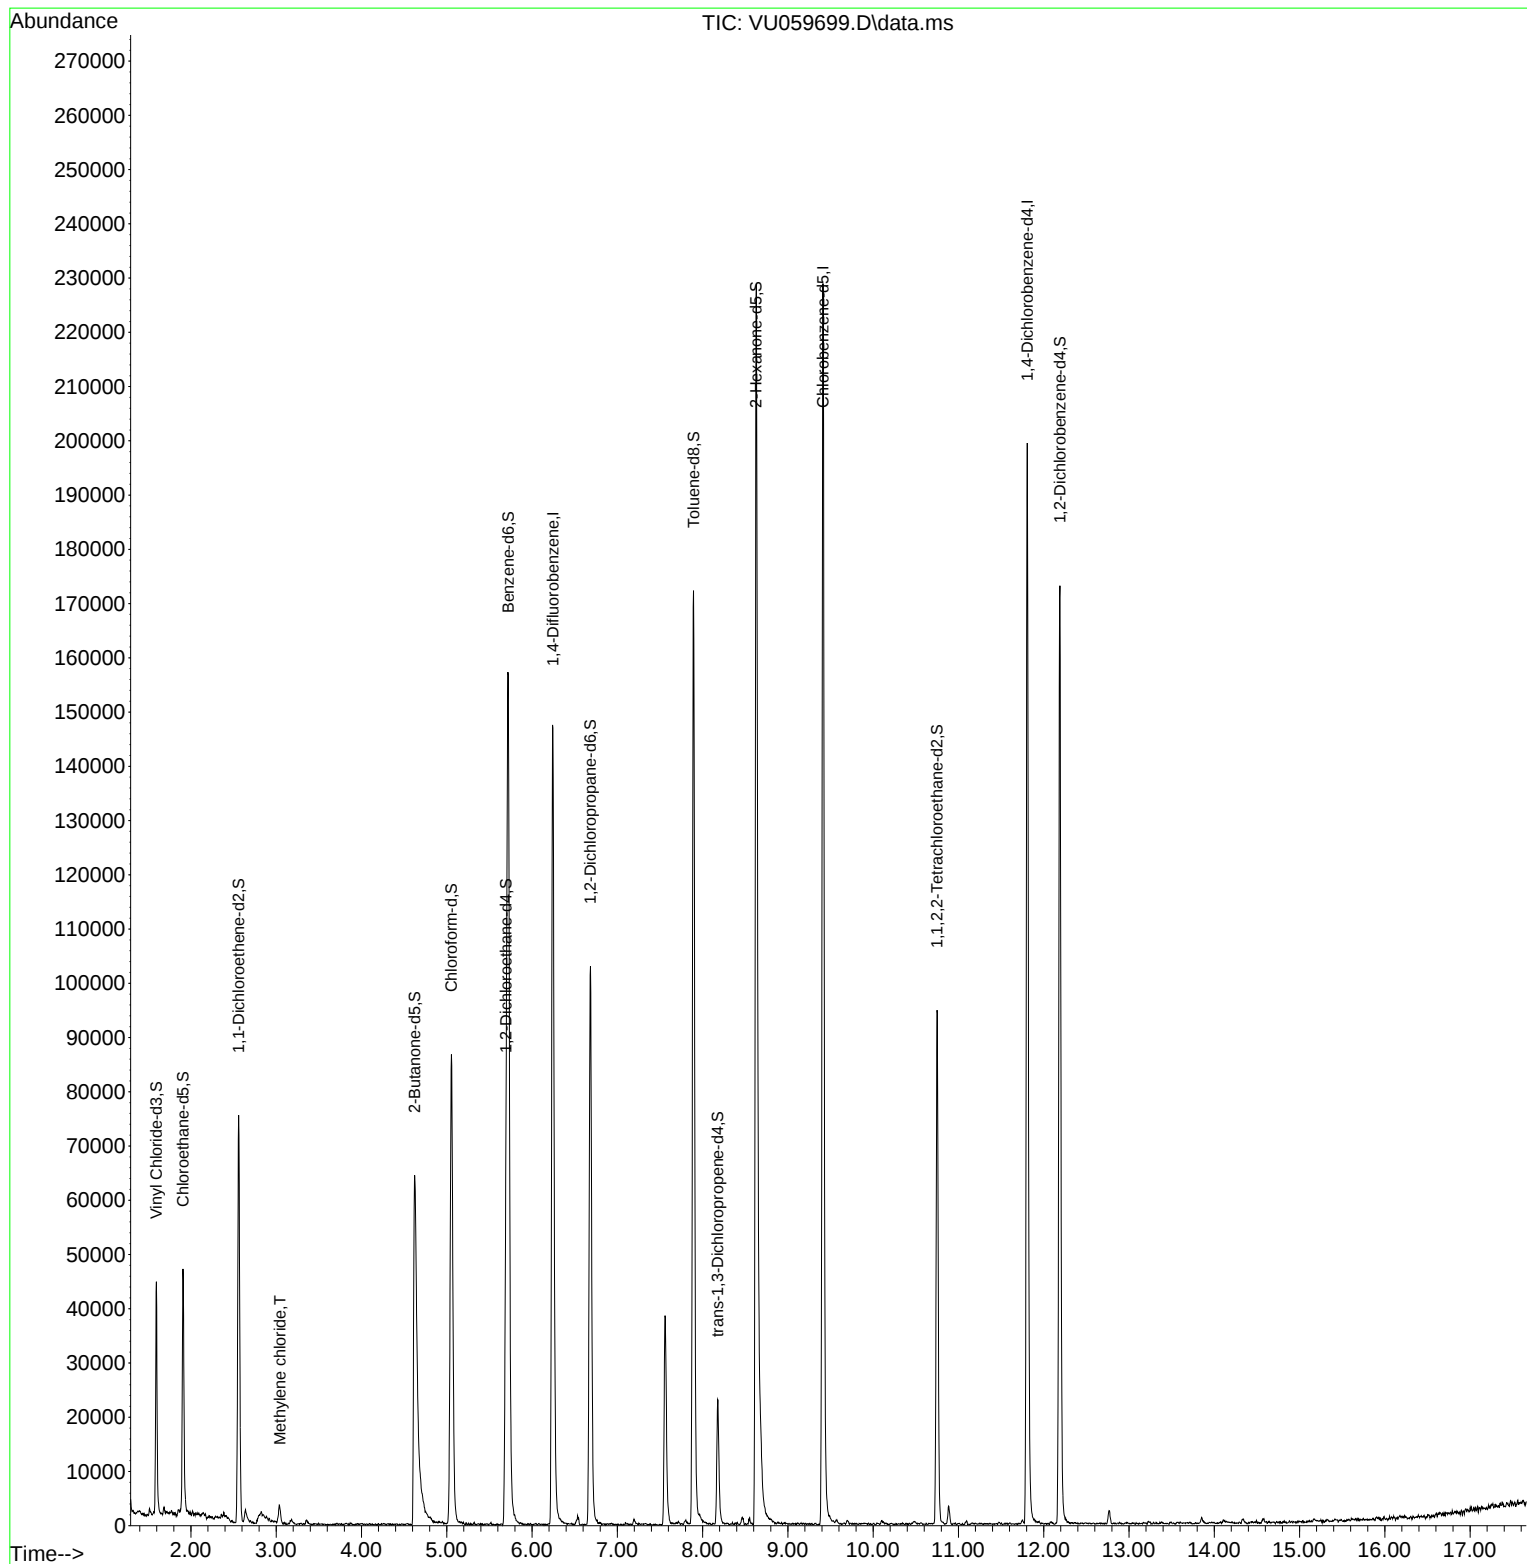

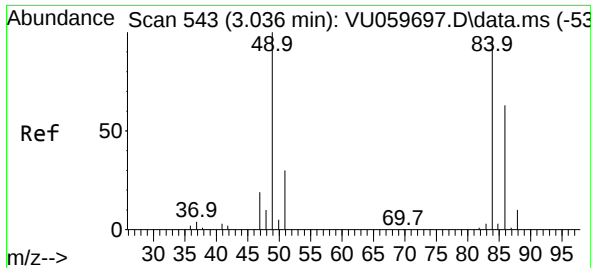

#16
Methylene chloride
Concen: 0.174 ug/L
RT: 3.042 min Scan# 54
Delta R.T. 0.003 min
Lab File: VU059699.D
Acq: 01 Jul 2024 21:17

Instrument :
MSVOA_U
ClientSampleId :
C0BF3

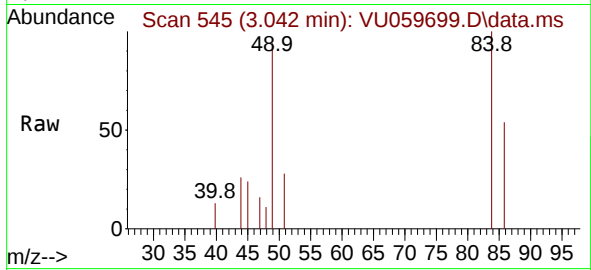

Tgt Ion: 84 Resp: 1887

Ion	Ratio	Lower	Upper
84	100		
86	53.8	42.1	78.1
49	93.6	80.6	149.8

