

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
 Data File : VU059706.D
 Acq On : 02 Jul 2024 00:05
 Operator : MD/SY
 Sample : P3121-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COBJO

Quant Time: Jul 02 03:55:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 29 01:51:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	210700	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	209797	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	104294	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	39302	2.683	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	53.600%	
7) Chloroethane-d5	1.907	69	45287	3.212	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	64.200%#	
11) 1,1-Dichloroethene-d2	2.560	65	19711	3.243	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	64.800%	
20) 2-Butanone-d5	4.621	46	173843	57.604	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	115.200%	
24) Chloroform-d	5.055	84	113864	3.786	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	75.800%	
26) 1,2-Dichloroethane-d4	5.695	65	60949	4.207	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.200%	
32) Benzene-d6	5.721	84	225521	3.906	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	78.200%	
36) 1,2-Dichloropropane-d6	6.682	67	73258	4.141	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	82.800%	
41) Toluene-d8	7.891	98	191845	3.574	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	71.400%	
43) trans-1,3-Dichloroprop...	8.177	79	22496	4.060	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	81.200%	
46) 2-Hexanone-d5	8.627	63	143753	62.448	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	124.900%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	69170	4.732	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.600%	
66) 1,2-Dichlorobenzene-d4	12.187	152	84403	4.547	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	91.000%	
Target Compounds						
					Qvalue	
14) Carbon disulfide	2.788	76	5307	0.106	ug/L #	86
22) cis-1,2-Dichloroethene	4.660	96	7699	0.449	ug/L	93
30) Cyclohexane	5.383	56	1529	0.071	ug/L #	85
34) Trichloroethene	6.541	95	6124	0.355	ug/L	95
47) Tetrachloroethene	8.547	164	344066	25.699	ug/L	95
52) Ethylbenzene	9.569	91	8961	0.130	ug/L	91
53) m,p-Xylene	9.685	106	13773	0.518	ug/L	95
54) o-Xylene	10.100	106	3674	0.146	ug/L	78
63) 1,2,4-Trimethylbenzene	11.466	105	10129	0.208	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059706.D
Acq On : 02 Jul 2024 00:05
Operator : MD/SY
Sample : P3121-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BJ0

Quant Time: Jul 02 03:55:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

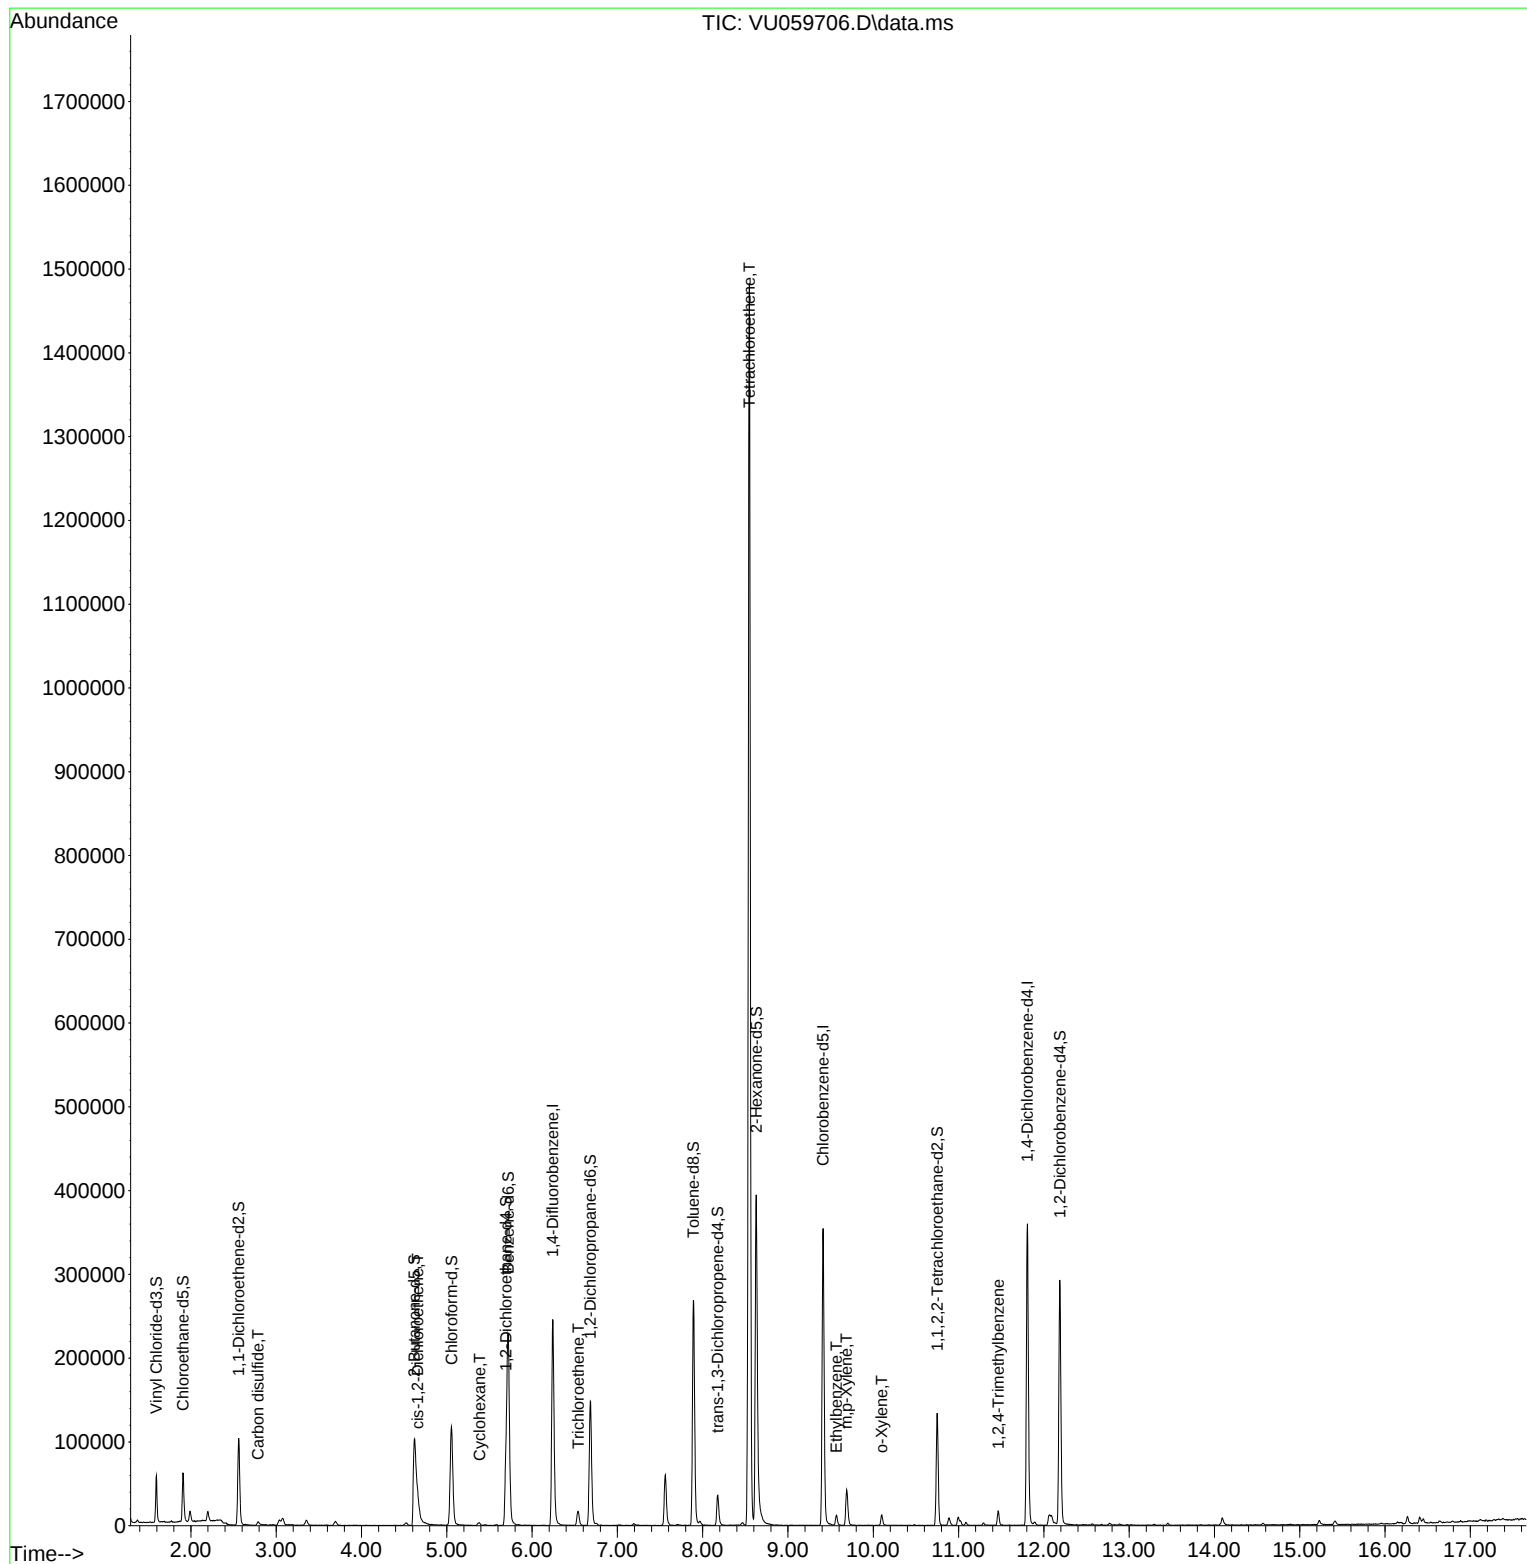

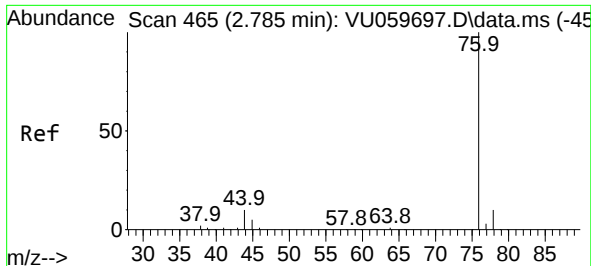

#14

Carbon disulfide

Concen: 0.106 ug/L

RT: 2.788 min Scan# 4

Delta R.T. 0.003 min

Lab File: VU059706.D

Acq: 02 Jul 2024 00:05

Instrument :

MSVOA_U

ClientSampleId :





C0BJ0

Tgt Ion: 76 Resp: 5307

Ion Ratio Lower Upper

76 100

78 14.1 7.3 10.9#

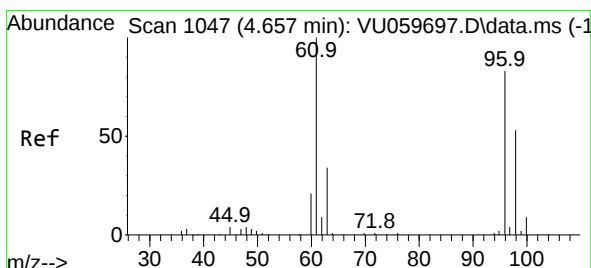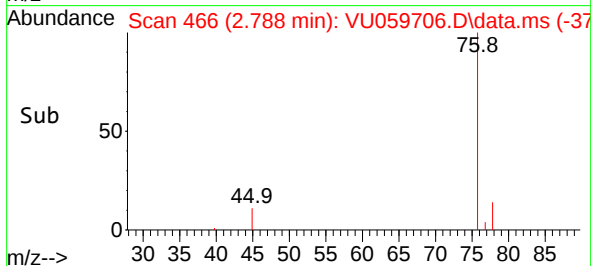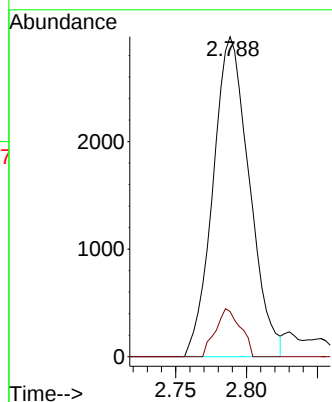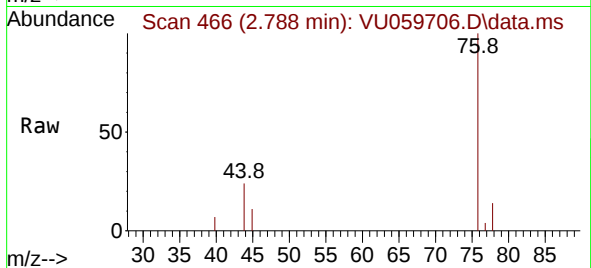

#22

cis-1,2-Dichloroethene

Concen: 0.449 ug/L

RT: 4.660 min Scan# 1048

Delta R.T. 0.000 min

Lab File: VU059706.D

Acq: 02 Jul 2024 00:05




Tgt Ion: 96 Resp: 7699


Ion Ratio Lower Upper

96 100

61 115.1 87.4 162.2

98 57.1 42.3 78.5

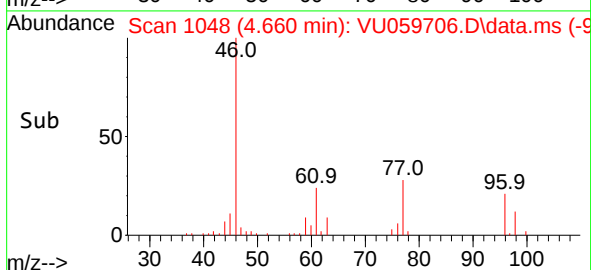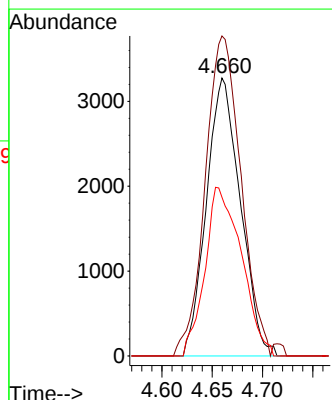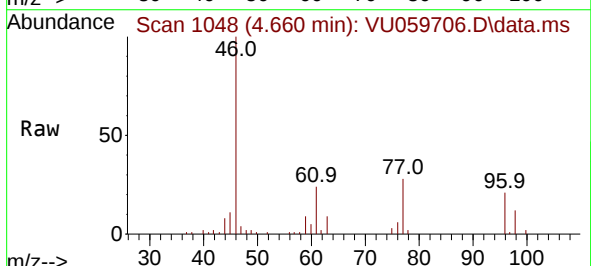

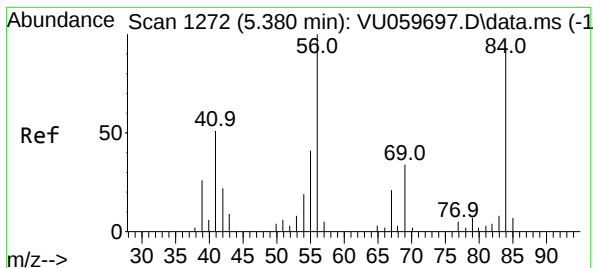

#30

Cyclohexane

Concen: 0.071 ug/L

RT: 5.383 min Scan# 11

Delta R.T. 0.003 min

Lab File: VU059706.D

Acq: 02 Jul 2024 00:05

Instrument :

MSVOA_U

ClientSampleId :

C0BJ0





Tgt Ion: 56 Resp: 1529

Ion Ratio Lower Upper

56 100

69 11.3 24.8 37.2#

84 93.9 69.8 104.8

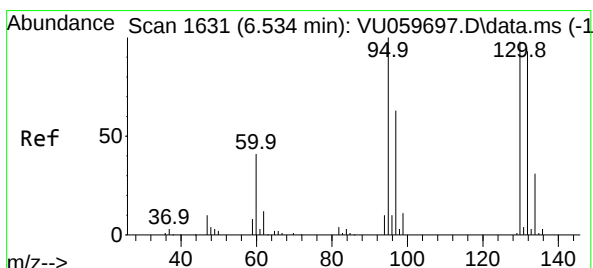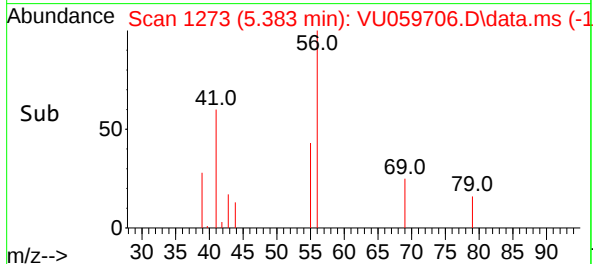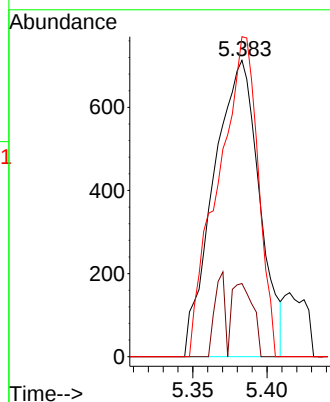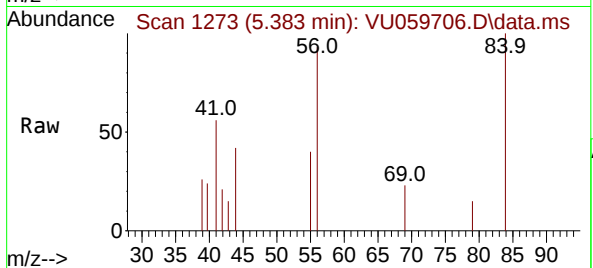

#34

Trichloroethene

Concen: 0.355 ug/L

RT: 6.541 min Scan# 1633

Delta R.T. 0.003 min

Lab File: VU059706.D

Acq: 02 Jul 2024 00:05

Tgt Ion: 95 Resp: 6124




Ion Ratio Lower Upper


95 100

97 67.8 45.3 84.1

132 98.2 64.0 119.0

130 101.8 69.1 128.3

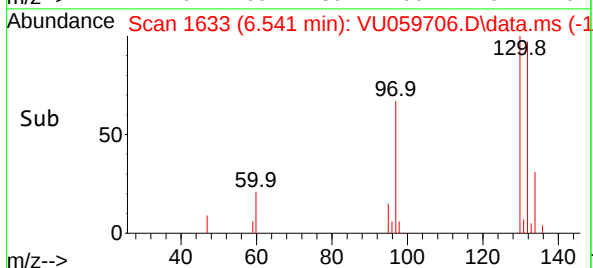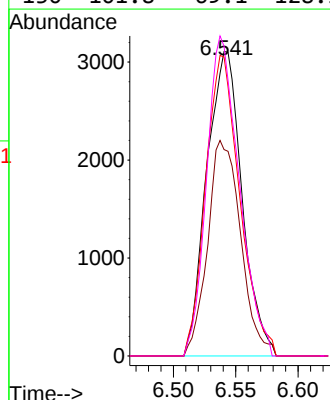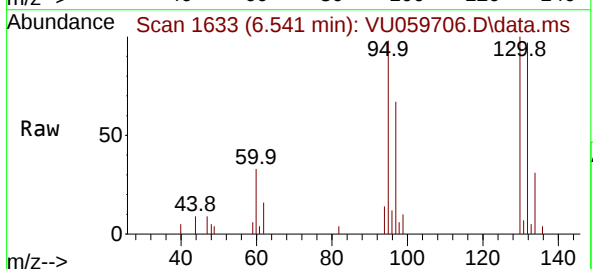

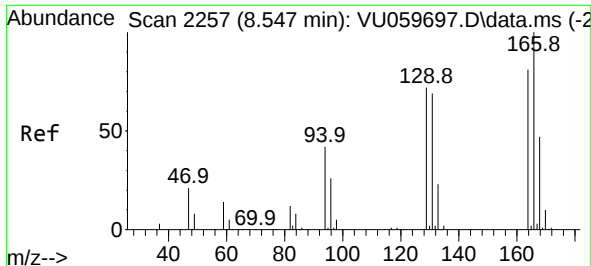

#47

Tetrachloroethene

Concen: 25.699 ug/L

RT: 8.547 min Scan# 21

Delta R.T. 0.000 min

Lab File: VU059706.D

Acq: 02 Jul 2024 00:05

Instrument :

MSVOA_U

ClientSampleId :

C0BJ0

Tgt Ion:164 Resp: 344066





Ion Ratio Lower Upper

164 100

129 91.8 70.8 131.4

131 88.1 64.8 120.3

166 127.2 91.1 169.1

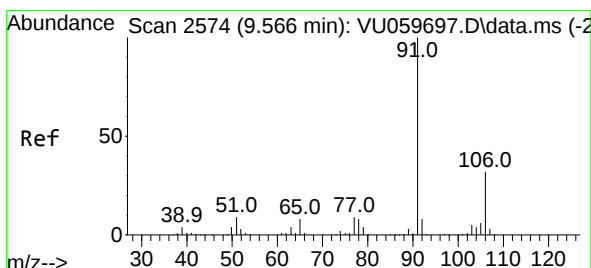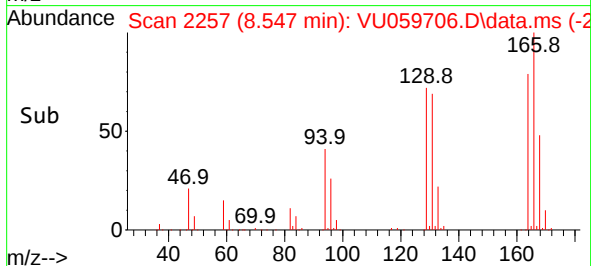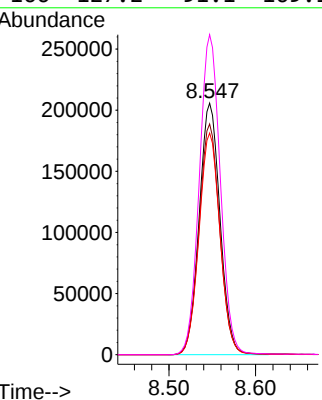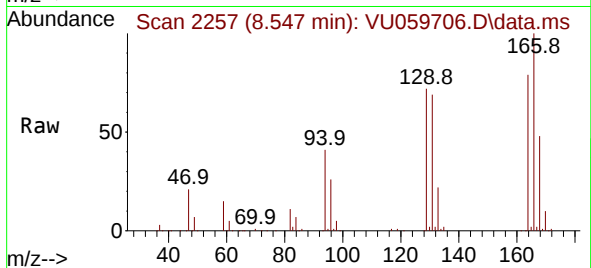

#52

Ethylbenzene

Concen: 0.130 ug/L

RT: 9.569 min Scan# 2575

Delta R.T. 0.007 min

Lab File: VU059706.D




Acq: 02 Jul 2024 00:05


Tgt Ion: 91 Resp: 8961

Ion Ratio Lower Upper

91 100

106 34.9 20.9 38.7


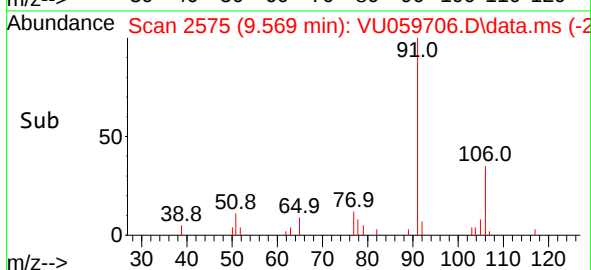
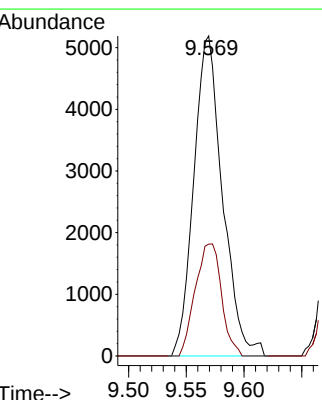
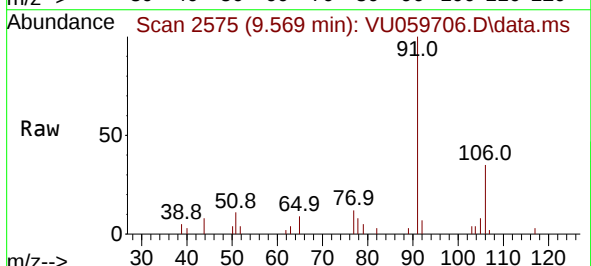


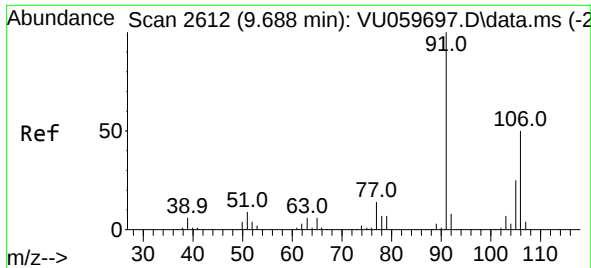

#53
m,p-Xylene
Concen: 0.518 ug/L
RT: 9.685 min Scan# 21
Delta R.T. -0.003 min
Lab File: VU059706.D
Acq: 02 Jul 2024 00:05




Instrument :
MSVOA_U
ClientSampleId :
C0BJ0


Tgt Ion:106 Resp: 13773
Ion Ratio Lower Upper
106 100
91 195.3 142.0 263.8

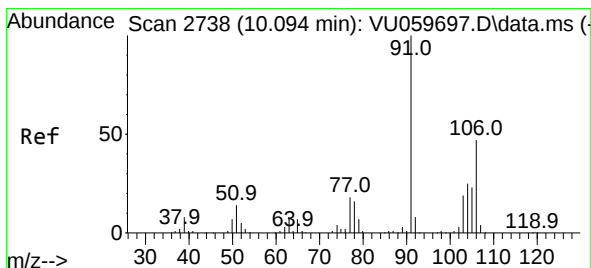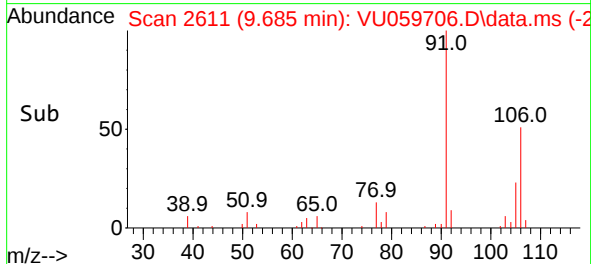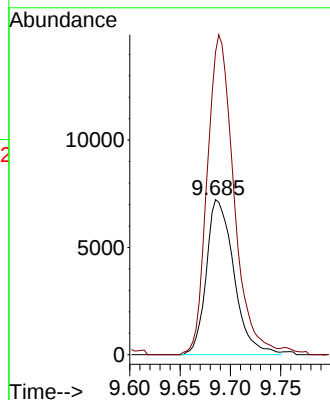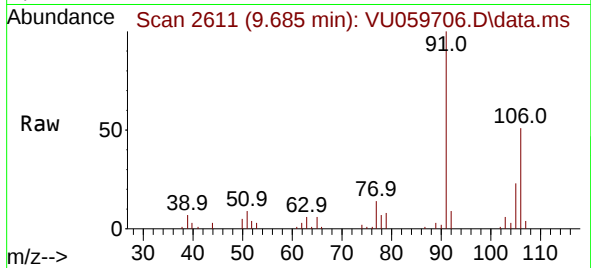

#54
o-Xylene
Concen: 0.146 ug/L
RT: 10.100 min Scan# 2740
Delta R.T. 0.006 min
Lab File: VU059706.D
Acq: 02 Jul 2024 00:05

Tgt Ion:106 Resp: 3674
Ion Ratio Lower Upper
106 100
91 182.0 151.6 281.6

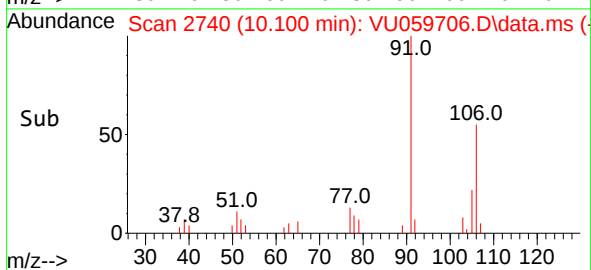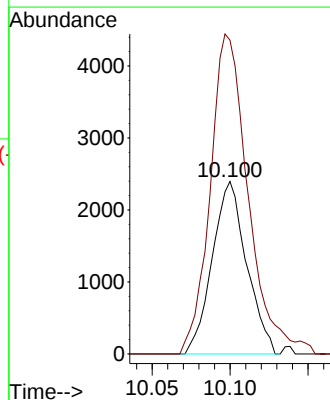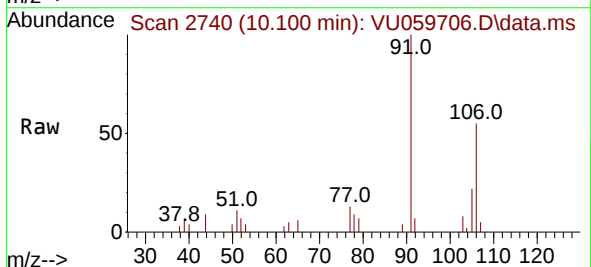

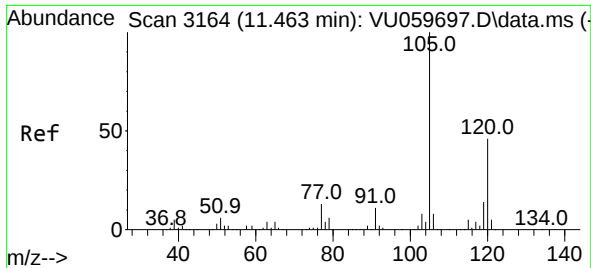

#63
1,2,4-Trimethylbenzene
Concen: 0.208 ug/L
RT: 11.466 min Scan# 3165
Delta R.T. 0.003 min
Lab File: VU059706.D
Acq: 02 Jul 2024 00:05

Instrument :
MSVOA_U
ClientSampleId :
C0BJ0

Tgt Ion:105 Resp: 10129
Ion Ratio Lower Upper
105 100
120 44.4 35.4 53.0

