

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
 Data File : VU059704.D
 Acq On : 01 Jul 2024 23:17
 Operator : MD/SY
 Sample : P3121-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COBH6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	107	rVB	56426	64495	8.40%	0.973%
2	1.907	184	192	211	rVB	60737	86073	11.21%	1.298%
3	2.560	383	395	409	rBV	109826	178446	23.24%	2.691%
4	2.641	412	420	437	rVB	5035	10039	1.31%	0.151%
5	2.792	452	467	475	rBV2	11656	28895	3.76%	0.436%
6	3.042	535	545	558	rVB5	3699	8033	1.05%	0.121%
7	4.624	1024	1037	1084	rBV2	107179	384034	50.02%	5.792%
8	5.055	1153	1171	1194	rBV	123129	271925	35.42%	4.101%
9	5.718	1357	1377	1397	rBV2	240562	618881	80.61%	9.334%
10	6.242	1526	1540	1568	rBV	243318	476424	62.06%	7.186%
11	6.682	1664	1677	1703	rBV2	151157	299109	38.96%	4.511%
12	7.560	1937	1950	1976	rBV	64280	117788	15.34%	1.777%
13	7.891	2040	2053	2069	rBV	279828	494252	64.38%	7.455%
14	7.962	2070	2075	2089	rVB2	6949	13632	1.78%	0.206%
15	8.177	2129	2142	2165	rBV2	38190	69369	9.04%	1.046%
16	8.467	2223	2232	2245	rVB3	4797	9178	1.20%	0.138%
17	8.627	2271	2282	2323	rBV	402281	767735	100.00%	11.579%
18	9.412	2513	2526	2553	rBV	355338	605195	78.83%	9.128%
19	9.566	2563	2574	2590	rVB	20432	32819	4.27%	0.495%
20	9.689	2601	2612	2629	rBV2	74806	133946	17.45%	2.020%
21	10.097	2729	2739	2753	rBV	19669	34746	4.53%	0.524%
22	10.750	2930	2942	2960	rBV	144573	228332	29.74%	3.444%
23	10.891	2974	2986	2999	rBV4	10185	21096	2.75%	0.318%
24	10.994	3008	3018	3036	rBV2	18453	46758	6.09%	0.705%
25	11.084	3036	3046	3058	rVB2	8012	13521	1.76%	0.204%
26	11.290	3098	3110	3123	rBV3	6510	12120	1.58%	0.183%
27	11.463	3154	3164	3180	rVB2	35621	58524	7.62%	0.883%
28	11.640	3211	3219	3227	rVB2	5456	8257	1.08%	0.125%
29	11.807	3259	3271	3290	rBV	375462	609567	79.40%	9.194%
30	11.888	3290	3296	3305	rVB3	7479	11969	1.56%	0.181%
31	12.090	3340	3359	3376	rBV5	14457	34727	4.52%	0.524%
32	12.187	3377	3389	3407	rVV	312317	510018	66.43%	7.692%
33	12.775	3562	3572	3580	rBV4	7970	14082	1.83%	0.212%
34	13.450	3771	3782	3792	rBV4	8301	12449	1.62%	0.188%
35	14.087	3968	3980	3993	rBV	23442	43407	5.65%	0.655%
36	14.878	4217	4226	4237	rVB10	5474	9438	1.23%	0.142%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059704.D
Acq On : 01 Jul 2024 23:17
Operator : MD/SY
Sample : P3121-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BH6

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0

37	15.222	4322	4333	4345	rBV2	20655	34984	4.56%	0.528%
38	15.409	4380	4391	4403	rBV2	18125	31600	4.12%	0.477%
39	16.142	4610	4619	4626	rBV2	11116	19388	2.53%	0.292%
40	16.257	4645	4655	4667	rBV3	31827	56499	7.36%	0.852%
41	16.405	4687	4701	4707	rBV2	32254	53176	6.93%	0.802%
42	16.444	4708	4713	4723	rVB3	20949	29228	3.81%	0.441%
43	16.634	4756	4772	4783	rBV4	11641	25579	3.33%	0.386%
44	16.785	4811	4819	4826	rBV7	5491	9471	1.23%	0.143%
45	17.109	4915	4920	4934	rBV8	6401	11080	1.44%	0.167%
46	17.328	4981	4988	4994	rVB6	5857	9068	1.18%	0.137%
47	17.376	4997	5003	5013	rVB9	6493	10824	1.41%	0.163%




Sum of corrected areas: 6630176

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059704.D
Acq On : 01 Jul 2024 23:17
Operator : MD/SY
Sample : P3121-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COBH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

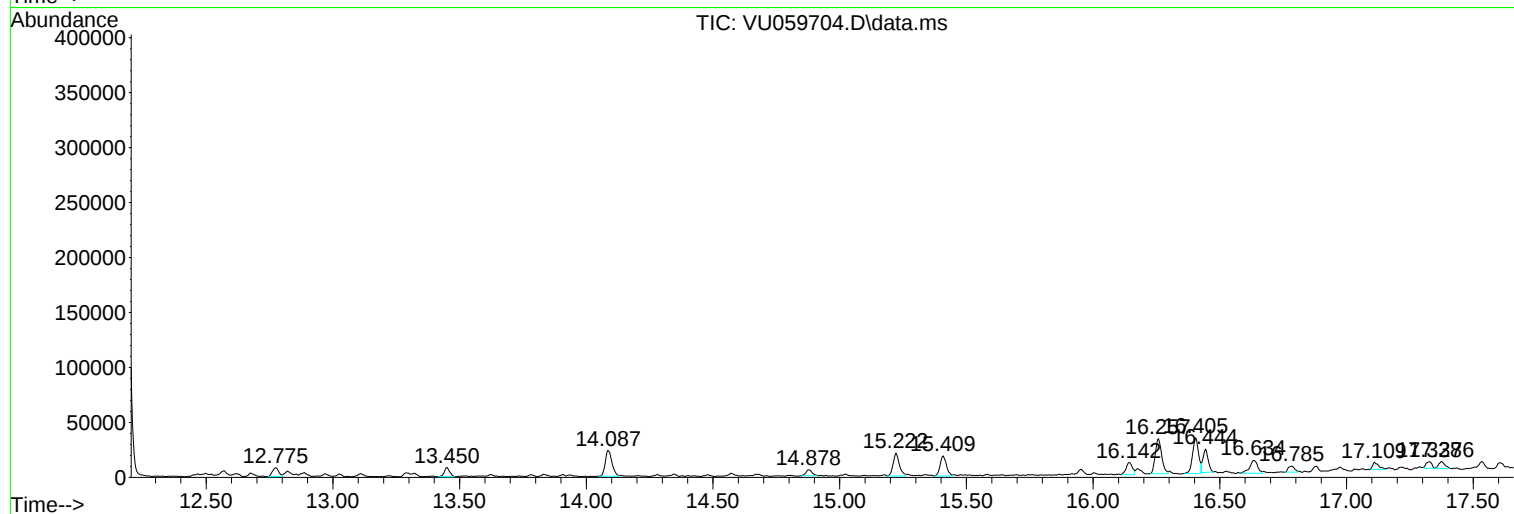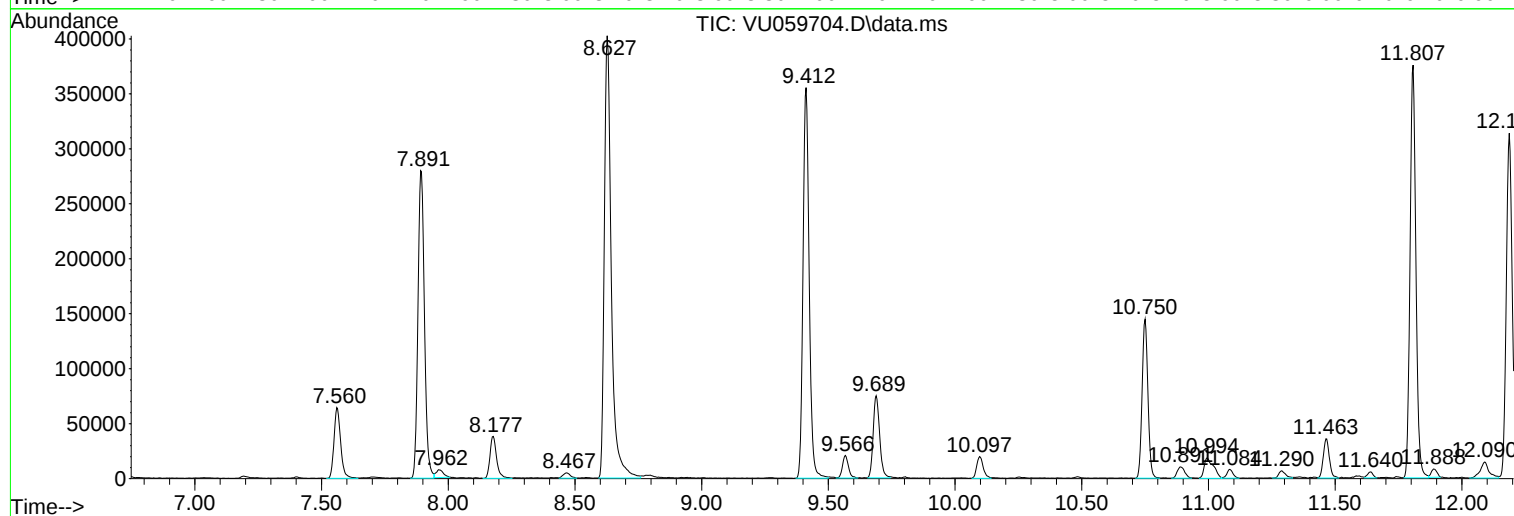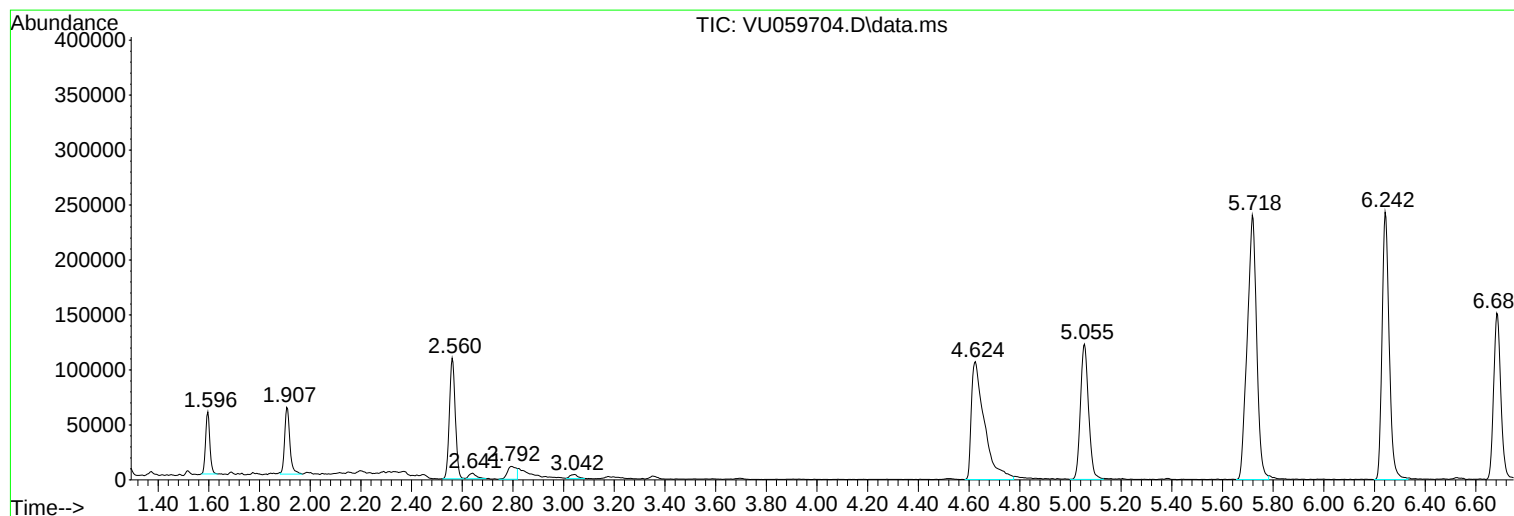

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059704.D
Acq On : 01 Jul 2024 23:17
Operator : MD/SY
Sample : P3121-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059704.D
Acq On : 01 Jul 2024 23:17
Operator : MD/SY
Sample : P3121-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------