

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
 Data File : VU059720.D
 Acq On : 02 Jul 2024 05:39
 Operator : MD/SY
 Sample : P3084-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G75

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU059720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.448	349	360	381	rVB	529944	845448	6.68%	4.647%
2	2.560	383	395	408	rBV	89448	148169	1.17%	0.814%
3	2.792	444	467	535	rBV	2875685	12648297	100.00%	69.523%
4	4.624	1025	1037	1039	rBV2	99510	160768	1.27%	0.884%
5	5.055	1156	1171	1193	rBV	112290	265921	2.10%	1.462%
6	5.717	1358	1377	1417	rBV2	210222	559751	4.43%	3.077%
7	6.242	1527	1540	1569	rBV	239496	458060	3.62%	2.518%
8	6.682	1664	1677	1696	rBV	136395	270624	2.14%	1.488%
9	7.891	2040	2053	2068	rBV	251340	439898	3.48%	2.418%
10	8.627	2270	2282	2314	rBV	338629	622782	4.92%	3.423%
11	9.412	2512	2526	2555	rBV	336192	575360	4.55%	3.163%
12	10.749	2930	2942	2959	rBV	120979	193080	1.53%	1.061%
13	11.804	3259	3270	3292	rBV	332238	559016	4.42%	3.073%
14	12.187	3377	3389	3413	rVB	266865	445801	3.52%	2.450%




Sum of corrected areas: 18192975

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059720.D
Acq On : 02 Jul 2024 05:39
Operator : MD/SY
Sample : P3084-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

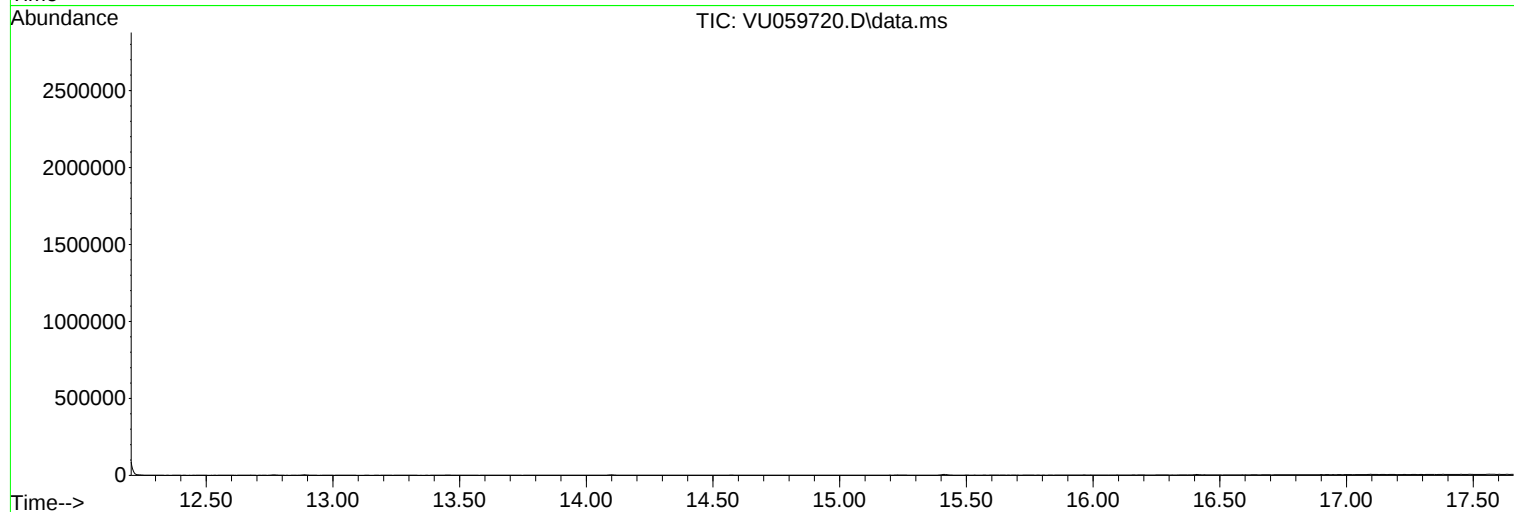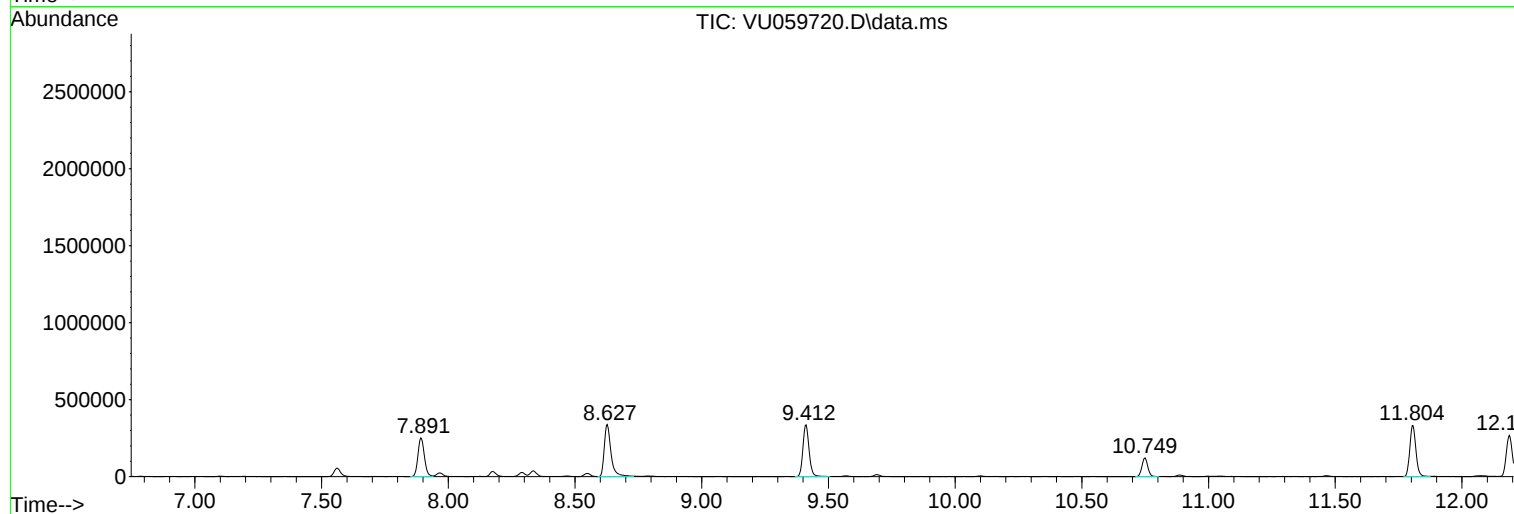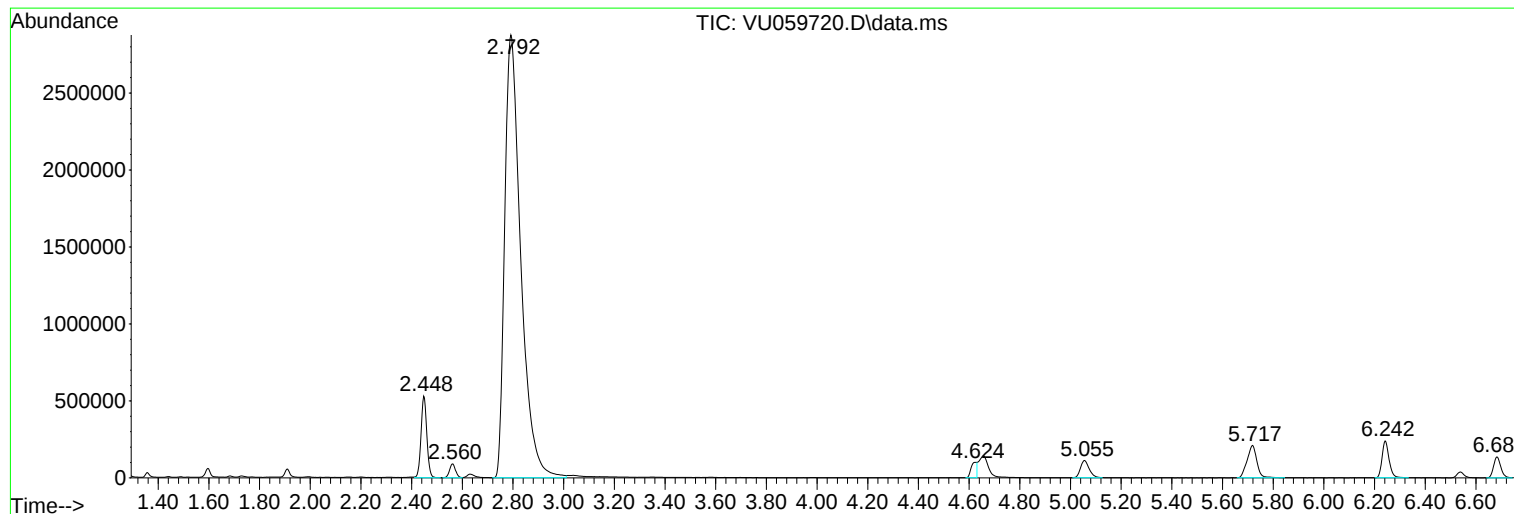

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059720.D
Acq On : 02 Jul 2024 05:39
Operator : MD/SY
Sample : P3084-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G75







Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.447	9.23 ug/L	845448	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	64
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	59
4	Propane, 2-nitro-			89	C3H7NO2	000079-46-9	9
5	Acetyl chloride			78	C2H3ClO	000075-36-5	9

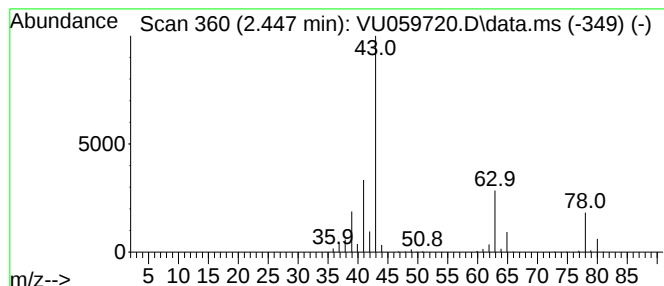

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059720.D
Acq On : 02 Jul 2024 05:39
Operator : MD/SY
Sample : P3084-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G75










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.792	138.06 ug/L	12648300	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	9

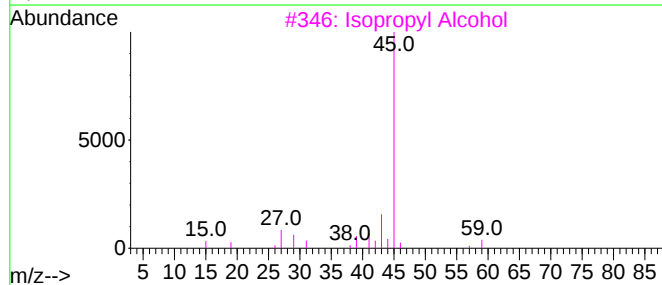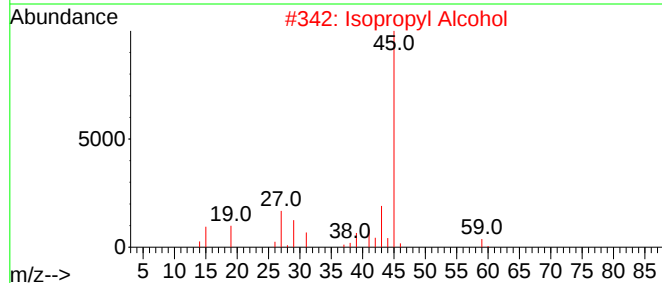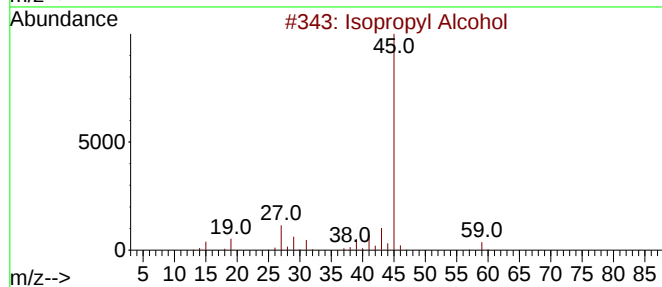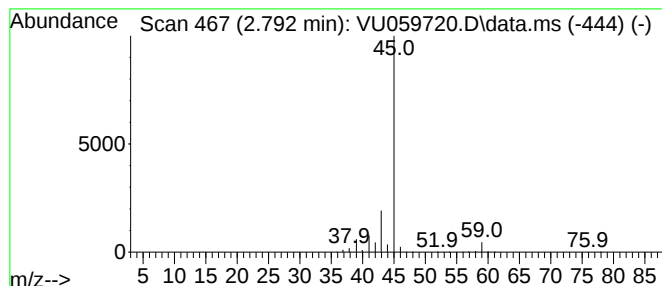

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059720.D
Acq On : 02 Jul 2024 05:39
Operator : MD/SY
Sample : P3084-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.447	9.2	ug/L	845448	1	6.242	458060	5.0
Isopropyl Alcohol	2.792	138.1	ug/L	12648300	1	6.242	458060	5.0