

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
 Data File : VU059721.D
 Acq On : 02 Jul 2024 06:03
 Operator : MD/SY
 Sample : P3084-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G89

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.448	342	360	382	rVB	642071	1043326	9.14%	5.842%
2	2.560	385	395	409	rBV2	86410	146545	1.28%	0.821%
3	2.792	445	467	525	rBV	2621401	11409370	100.00%	63.888%
4	4.657	1021	1047	1076	rBV3	227566	740320	6.49%	4.146%
5	5.055	1152	1171	1194	rBV	108863	247101	2.17%	1.384%
6	5.718	1355	1377	1395	rBV2	207957	550361	4.82%	3.082%
7	6.242	1528	1540	1560	rBV	232313	449870	3.94%	2.519%
8	6.538	1618	1632	1653	rBV	66354	128491	1.13%	0.720%
9	6.682	1663	1677	1696	rBV	134696	265094	2.32%	1.484%
10	7.891	2042	2053	2068	rBV	252709	431026	3.78%	2.414%
11	8.628	2271	2282	2310	rBV	324939	613255	5.38%	3.434%
12	9.412	2514	2526	2549	rBV	334654	569288	4.99%	3.188%
13	10.750	2932	2942	2954	rBV	121477	195646	1.71%	1.096%
14	11.804	3257	3270	3285	rBV	345691	571851	5.01%	3.202%
15	12.187	3377	3389	3412	rVB	289691	496717	4.35%	2.781%




Sum of corrected areas: 17858261

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059721.D
Acq On : 02 Jul 2024 06:03
Operator : MD/SY
Sample : P3084-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

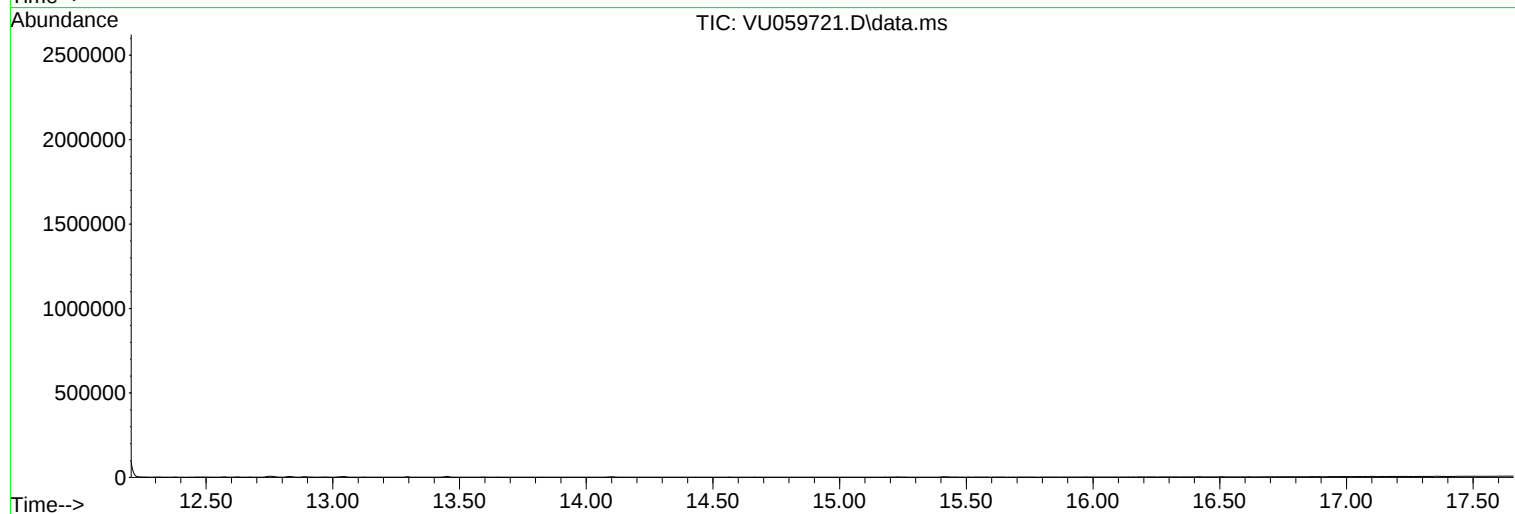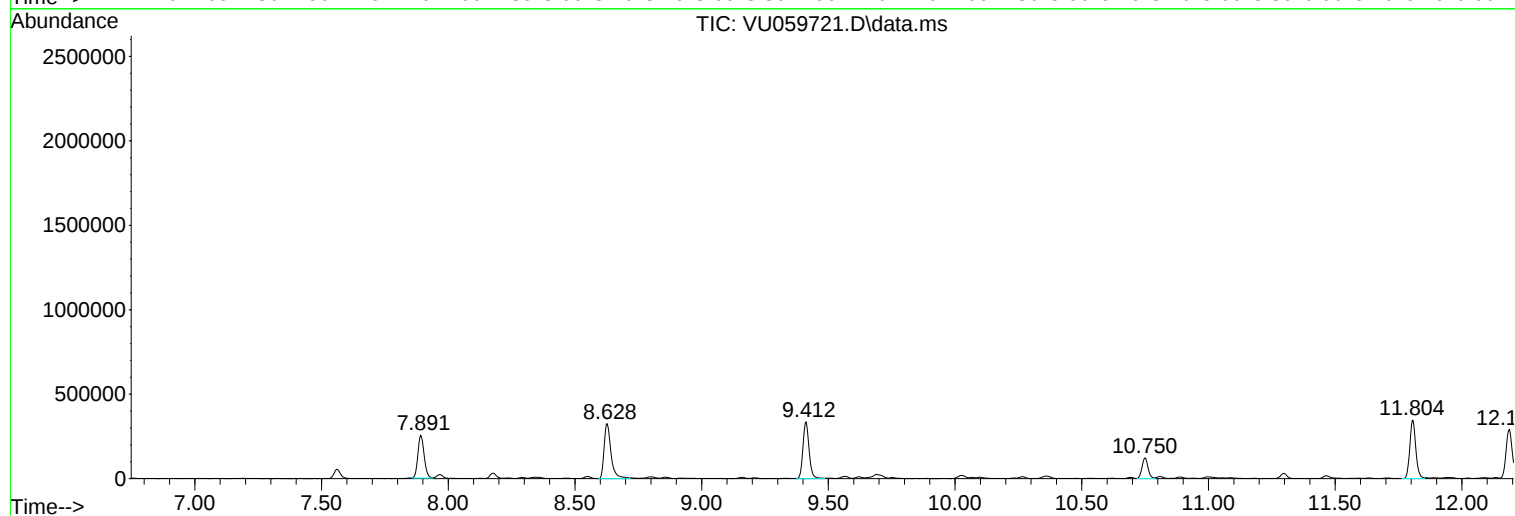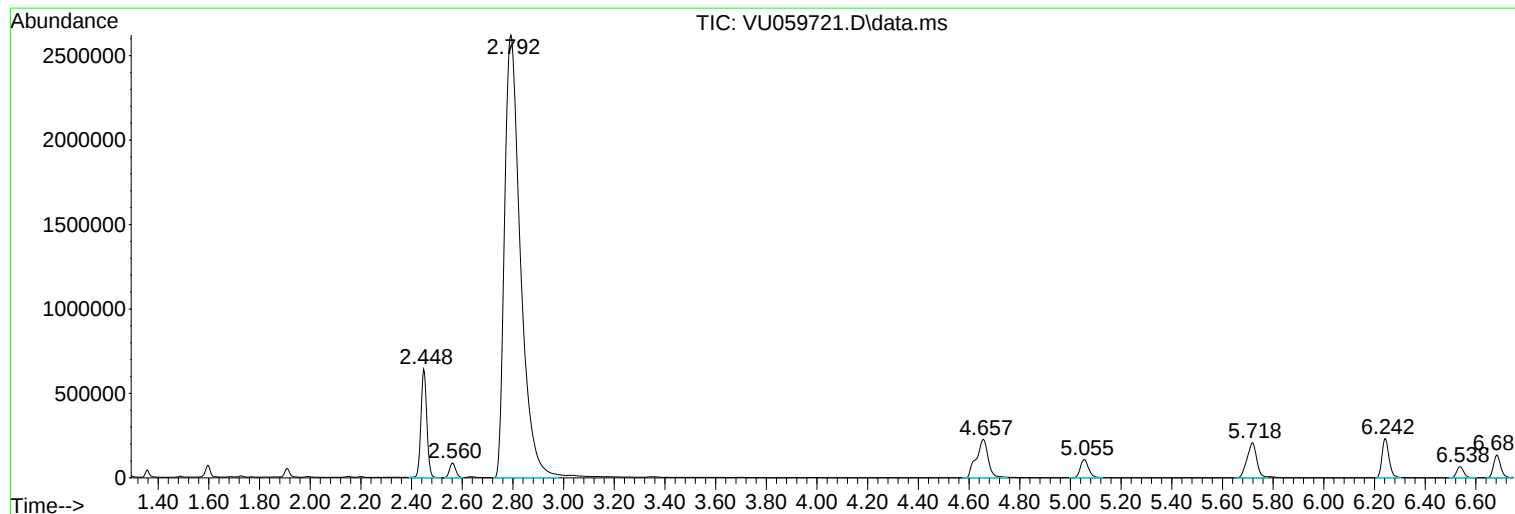

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059721.D
Acq On : 02 Jul 2024 06:03
Operator : MD/SY
Sample : P3084-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G89







Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.448	11.60 ug/L	1043330	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	58
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	45
4	Propane, 2-nitro-			89	C3H7NO2	000079-46-9	9
5	Acetyl chloride			78	C2H3ClO	000075-36-5	9

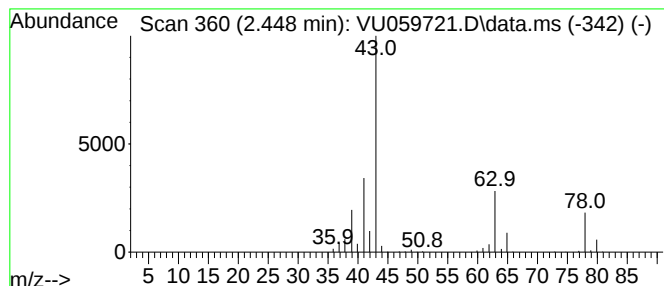

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059721.D
Acq On : 02 Jul 2024 06:03
Operator : MD/SY
Sample : P3084-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G89










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.792	126.81 ug/L	11409400	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

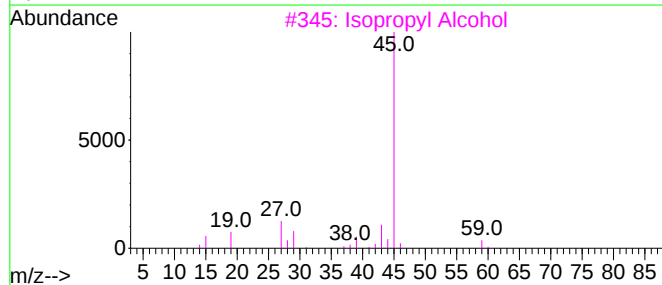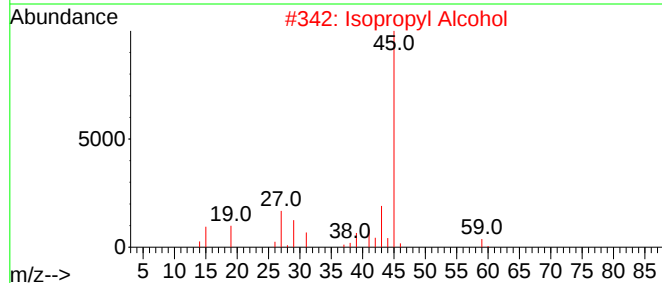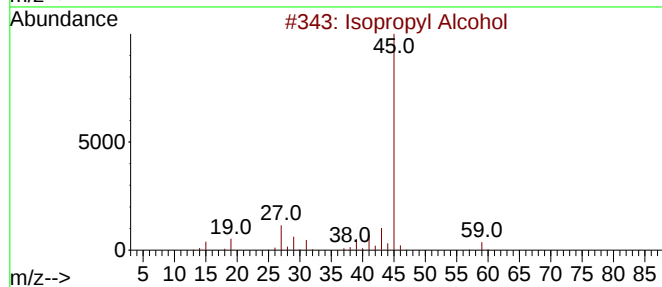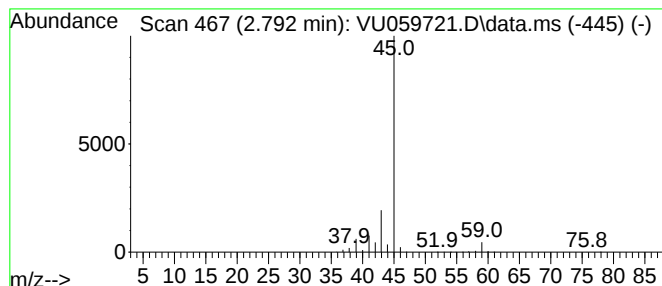

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059721.D
Acq On : 02 Jul 2024 06:03
Operator : MD/SY
Sample : P3084-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.448	11.6	ug/L	1043330	1	6.242	449870	5.0
Isopropyl Alcohol	2.792	126.8	ug/L	11409400	1	6.242	449870	5.0