


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070124\
Data File : VU059670.D
Acq On : 01 Jul 2024 08:54
Operator : MD/SY
Sample : BFB168
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB168

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jul 04 04:26:48 2024

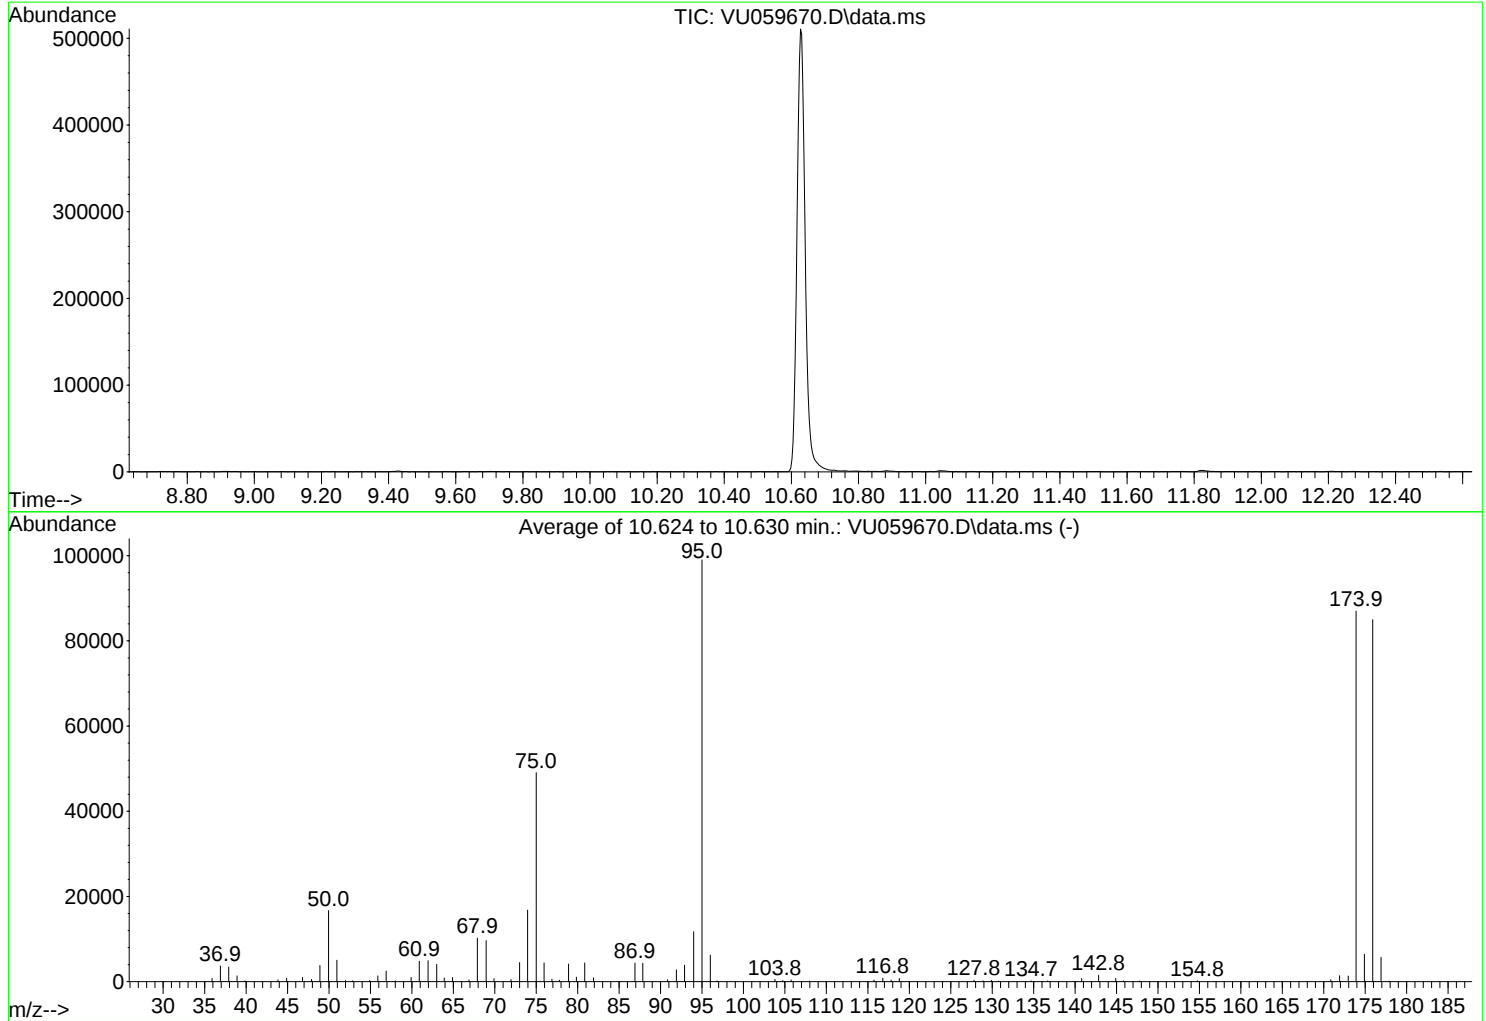

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.9	16690	PASS
75	95	30	80	49.5	49053	PASS
95	95	100	100	100.0	99019	PASS
96	95	5	9	6.3	6239	PASS
173	174	0.00	2	1.5	1310	PASS
174	95	50	120	87.8	86979	PASS
175	174	5	9	7.4	6419	PASS
176	174	95	101	97.7	84960	PASS
177	176	5	9	6.7	5725	PASS

m/z	Abundance
43.80	256.0

Instrument :
MSVOA_U
ClientSampleId :
BFB168

m/z	Abundance
35.90	704.0
36.90	3461.0
37.90	3318.0
38.90	1254.0
39.90	176.0
43.90	596.0
44.90	744.0
46.80	1056.0
47.90	553.0
48.90	3642.0
50.00	15919.0
51.00	5077.0
52.00	317.0
52.80	178.0
55.00	308.0
55.90	1283.0
56.90	2370.0
58.00	226.0
59.90	961.0
60.90	4605.0
61.90	4812.0
63.00	3853.0
63.90	893.0
64.90	975.0
65.90	102.0
66.90	422.0
67.90	9895.0
68.90	9713.0
69.90	658.0
72.00	472.0
73.00	4222.0
73.90	16225.0
75.00	47056.0
76.00	4401.0
76.90	533.0
77.80	372.0
78.90	3961.0
79.90	1036.0
80.80	4254.0
81.90	935.0
86.90	3902.0
87.80	4287.0
90.80	383.0
91.90	2735.0
92.90	3721.0
94.00	11430.0
95.00	94824.0
96.00	5999.0
96.80	207.0
103.80	479.0
104.80	249.0
105.70	391.0
107.90	139.0
114.70	123.0
115.70	359.0
116.80	773.0
117.80	342.0
118.80	752.0
127.80	318.0
128.90	172.0
129.90	320.0
130.70	153.0
134.70	168.0
136.60	157.0
140.80	733.0
142.80	1421.0
144.90	765.0
145.90	201.0
147.80	168.0
154.70	224.0
170.80	440.0
171.90	1279.0
172.90	1379.0
173.90	81584.0
174.90	5939.0
175.90	79160.0
176.90	5487.0
177.80	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB168

m/z	Abundance
35.90	813.0
36.90	3814.0
37.90	3524.0
38.90	1363.0
39.80	192.0
43.90	678.0
44.90	836.0
46.80	1022.0
47.90	561.0
48.90	3877.0
50.00	17184.0
51.00	5126.0
52.00	291.0
52.90	201.0
54.90	243.0
55.90	1409.0
56.90	2561.0
58.00	206.0
59.90	1033.0
60.90	4952.0
61.90	5116.0
63.00	4273.0
63.90	876.0
64.90	1038.0
66.90	433.0
67.90	10714.0
68.90	9853.0
69.90	717.0
71.90	495.0
73.00	4646.0
73.90	17312.0
75.00	50496.0
76.00	4559.0
76.90	619.0
77.80	348.0
78.90	4265.0
79.80	1068.0
80.90	4575.0
81.90	927.0
86.90	4515.0
87.90	4472.0
90.90	444.0
91.90	2848.0
92.90	3903.0
94.00	12029.0
95.00	101936.0
96.00	6361.0
96.80	187.0
103.80	545.0
104.80	296.0
105.70	410.0
107.90	145.0
115.70	361.0
116.80	852.0
117.80	387.0
118.80	765.0
127.80	352.0
128.90	178.0
129.90	311.0
130.80	161.0
134.70	191.0
136.70	205.0
140.80	794.0
142.90	1548.0
144.90	809.0
145.90	217.0
147.80	156.0
154.80	251.0
170.80	456.0
171.90	1425.0
172.90	1339.0
173.90	89512.0
174.90	6609.0
175.90	87536.0
176.90	5895.0
177.90	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB168

m/z	Abundance
35.90	747.0
36.90	3833.0
37.90	3453.0
38.90	1413.0
39.80	201.0
43.90	700.0
44.90	803.0
46.80	824.0
47.90	525.0
48.90	3845.0
49.90	16968.0
50.90	4856.0
52.00	226.0
52.90	194.0
54.80	210.0
55.90	1374.0
56.90	2555.0
57.90	144.0
59.90	1024.0
60.90	4899.0
62.00	4889.0
63.00	4071.0
63.90	788.0
64.90	913.0
66.90	371.0
67.90	10067.0
69.00	9280.0
69.90	728.0
71.90	516.0
73.00	4554.0
74.00	16896.0
75.00	49608.0
75.90	4264.0
76.90	622.0
77.80	330.0
78.90	4180.0
79.80	1042.0
80.90	4335.0
81.90	817.0
86.90	4716.0
87.90	4245.0
90.90	484.0
91.90	2747.0
92.90	3937.0
94.00	11723.0
95.00	100296.0
96.00	6356.0
96.90	128.0
103.80	511.0
104.70	242.0
105.80	409.0
108.00	124.0
115.80	367.0
116.80	820.0
117.80	397.0
118.80	691.0
127.80	352.0
128.90	176.0
129.90	299.0
130.80	176.0
134.70	172.0
136.80	207.0
140.80	765.0
141.90	132.0
142.90	1575.0
144.90	695.0
145.80	187.0
147.80	169.0
154.80	255.0
156.70	117.0
170.90	417.0
171.90	1495.0
173.00	1212.0
173.90	89840.0
174.90	6709.0
175.90	88184.0
176.90	5792.0
177.90	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB168