


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU070218\  
 Data File : VU025132.D  
 Acq On : 02 Jul 2018 09:36  
 Operator : MD/SY  
 Sample : BFB  
 Misc : 5.0mL/MSVOA U/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\82U061318W.M  
 Title : SW846 8260  
 Last Update : Wed Jun 13 13:55:26 2018

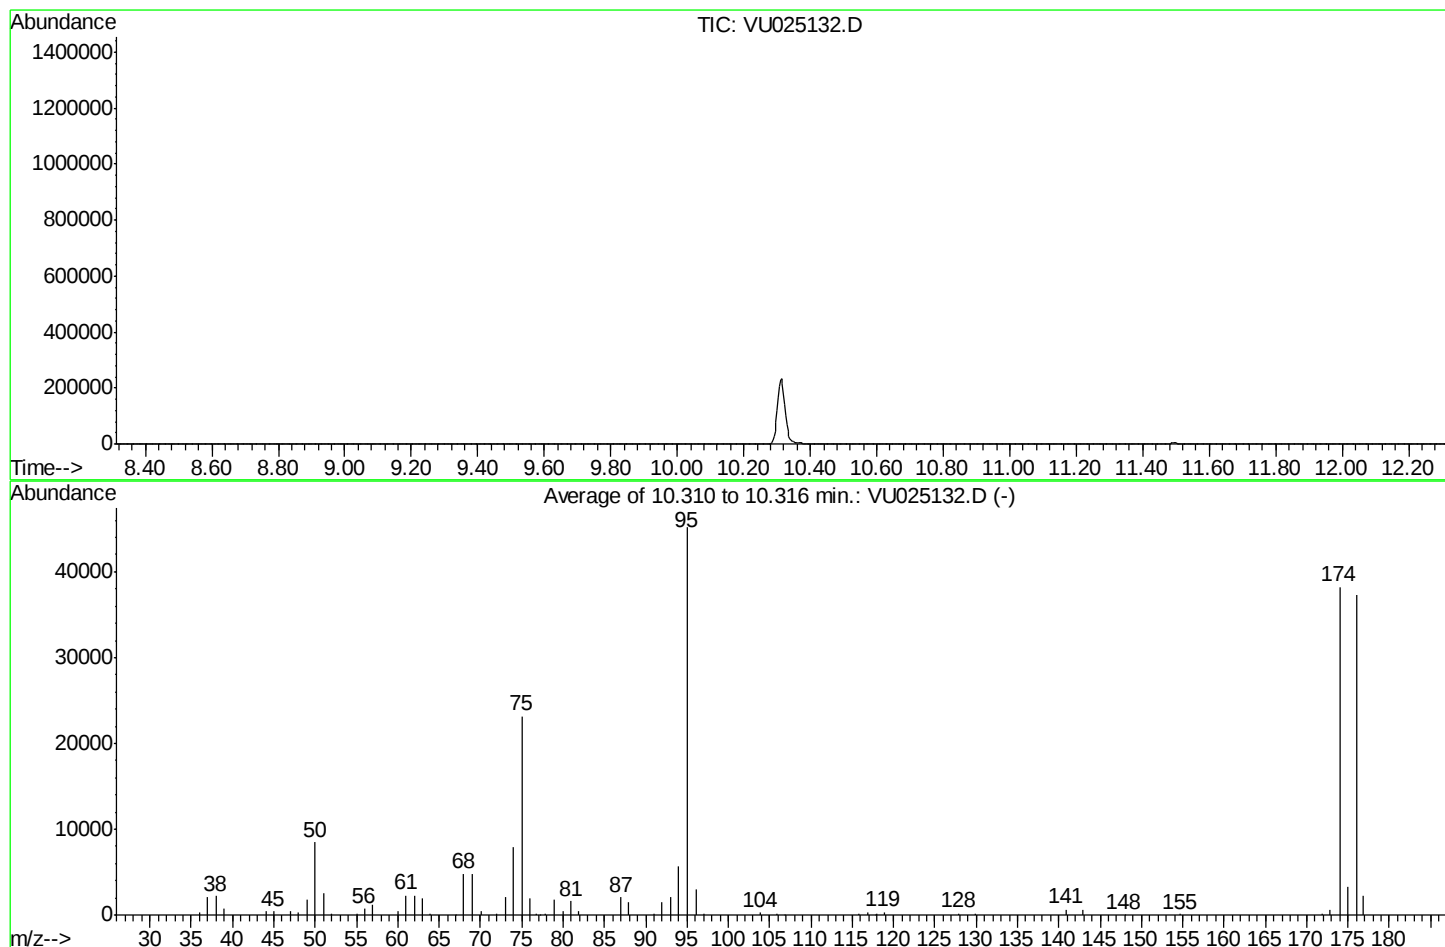

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3010

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.8      | 8483    | PASS             |
| 75          | 95           | 30           | 60           | 51.3      | 23160   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 45176   | PASS             |
| 96          | 95           | 5            | 9            | 6.5       | 2959    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.5       | 576     | PASS             |
| 174         | 95           | 50           | 100          | 84.5      | 38189   | PASS             |
| 175         | 174          | 5            | 9            | 8.5       | 3230    | PASS             |
| 176         | 174          | 95           | 101          | 97.6      | 37266   | PASS             |
| 177         | 176          | 5            | 9            | 6.2       | 2293    | PASS             |