

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU070219\
Quantitation Report (QT Reviewed)


Data File : VU033149.D
Acq On : 02 Jul 2019 18:35
Operator : JC/SP
Sample : K3597-09DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAM66DL

Manual Integrations
APPROVED

MMDadoda
7/3/2019 11:34:56 AM

Quant Time: Jul 03 03:55:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 03 02:14:33 2019
Response via : Initial Calibration

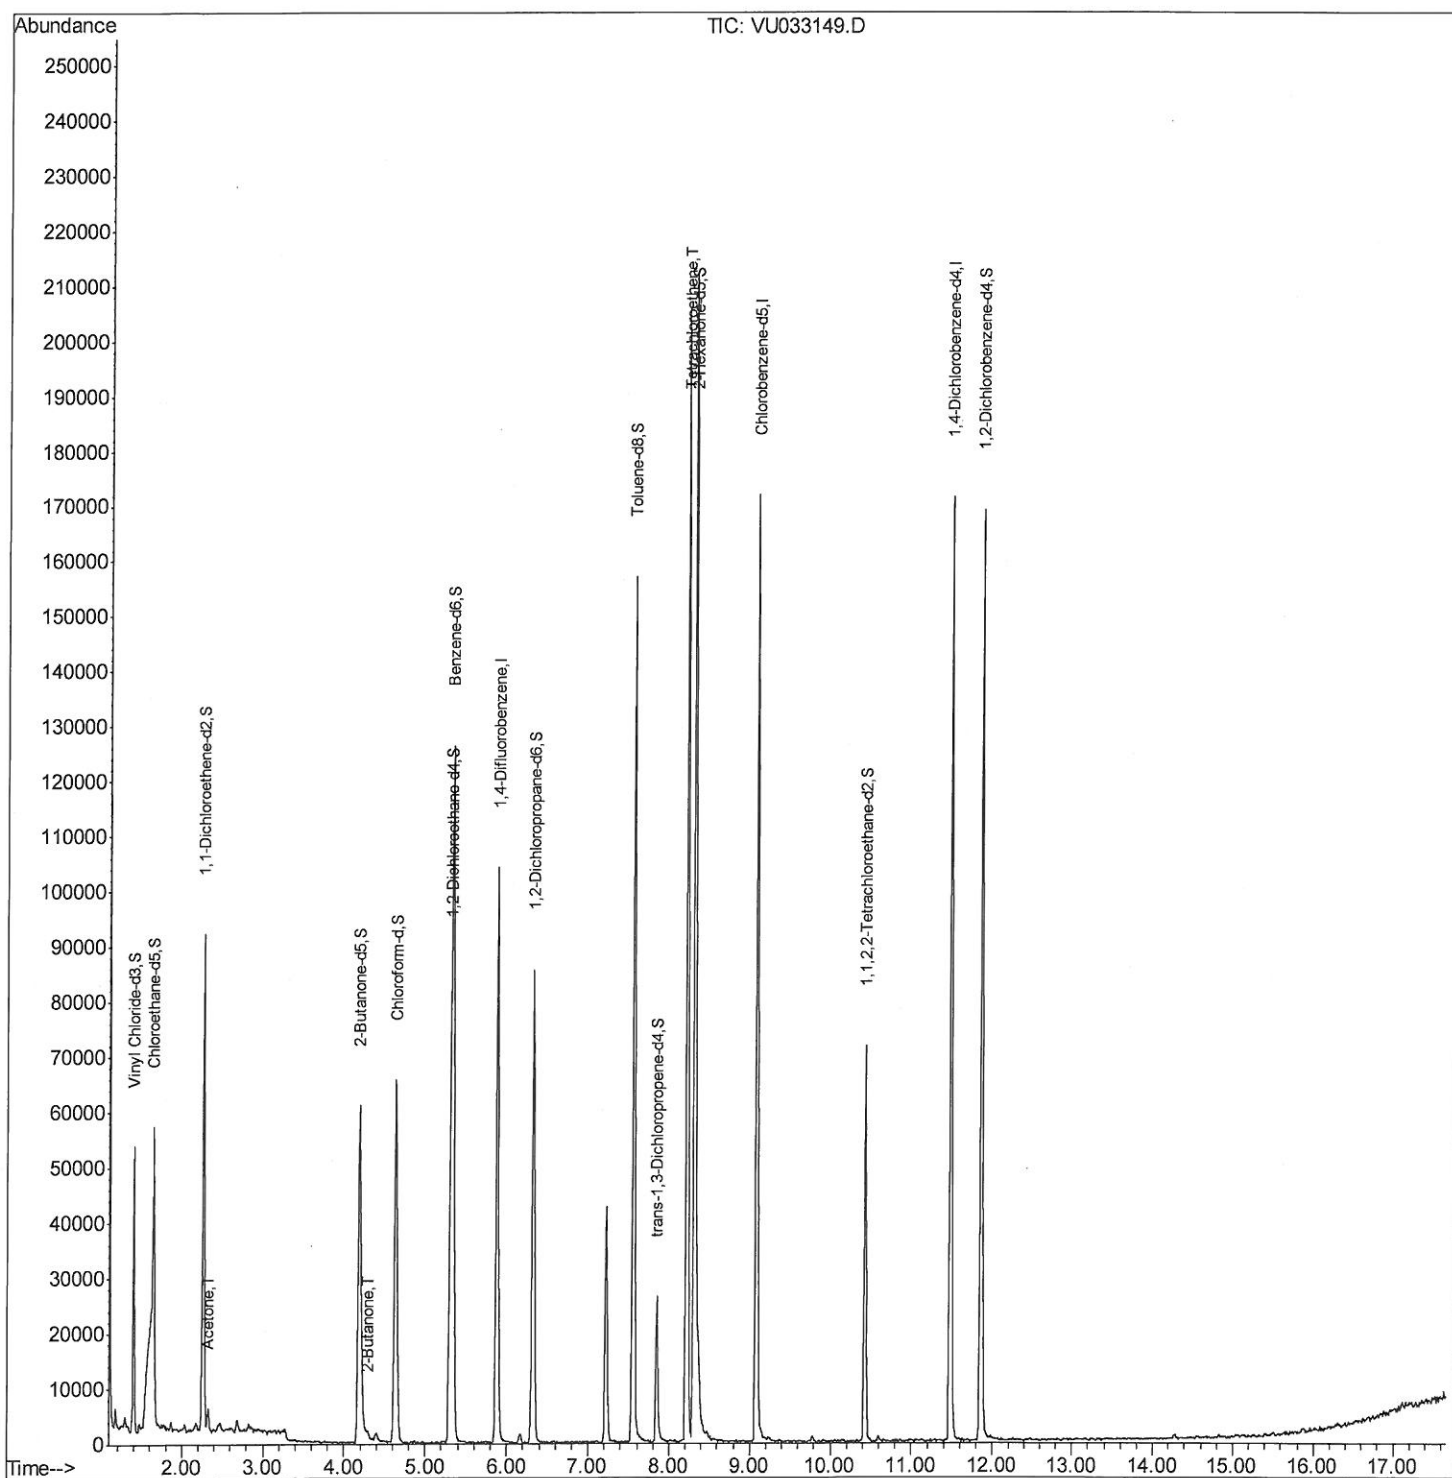

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU070219\
Quantitation Report (Qedit)




Data File : VU033149.D
Acq On : 02 Jul 2019 18:35
Operator : JC/SP
Sample : K3597-09DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAM66DL

Manual Integrations
APPROVED

MMDadoda
7/3/2019 11:34:56 AM

Quant Time: Jul 03 02:19:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 03 02:14:33 2019
Response via : Initial Calibration

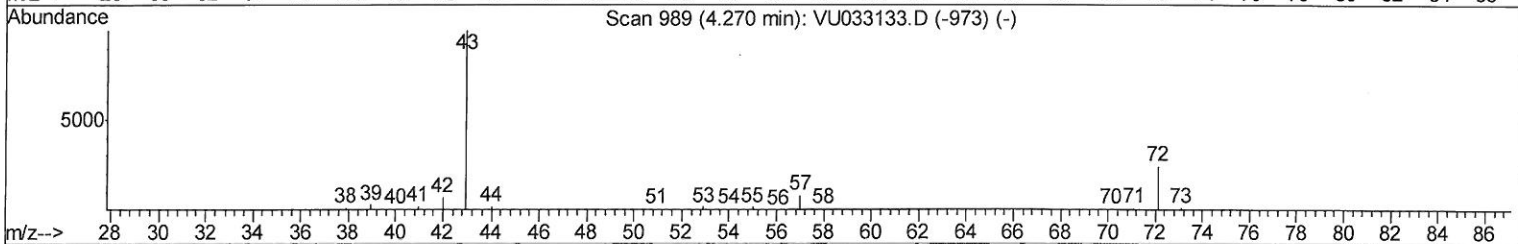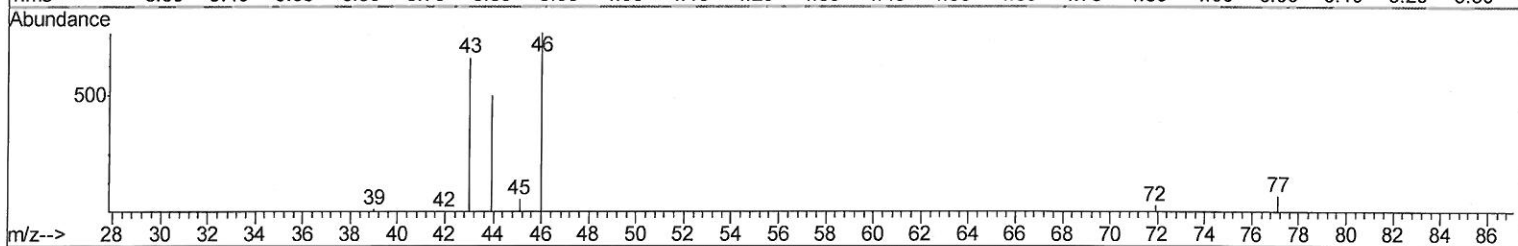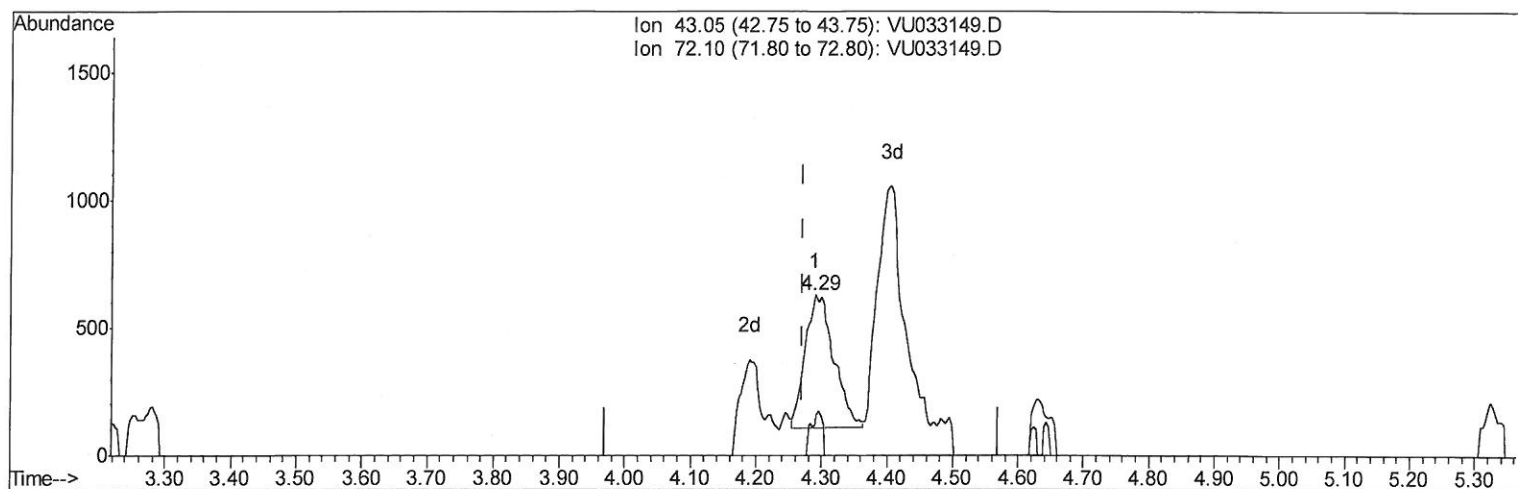

TIC: VU033149.D

(21) 2-Butanone (T)

4.289min (+0.019) 0.79ug/L

response 1604

Ion	Exp%	Act%
43.05	100	100
72.10	24.20	12.91
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU070219\
Quantitation Report (Qedit)




Data File : VU033149.D
Acq On : 02 Jul 2019 18:35
Operator : JC/SP
Sample : K3597-09DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
GAM66DL

Manual Integrations
APPROVED

MMDadoda
7/3/2019 11:34:56 AM

Quant Time: Jul 03 02:19:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 03 02:14:33 2019
Response via : Initial Calibration

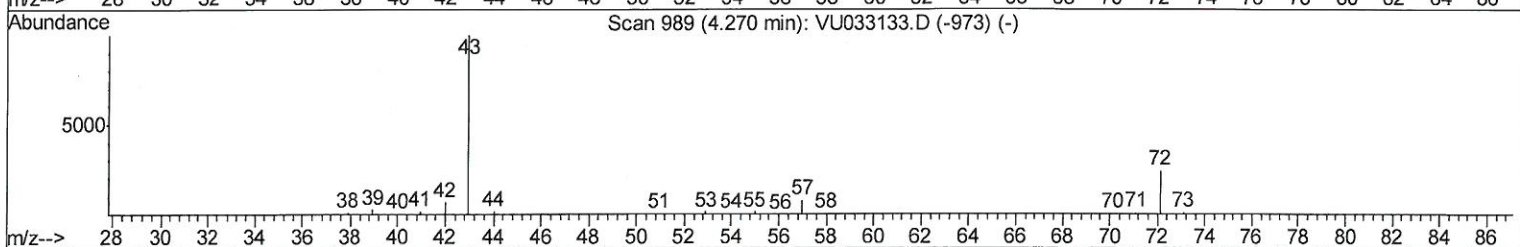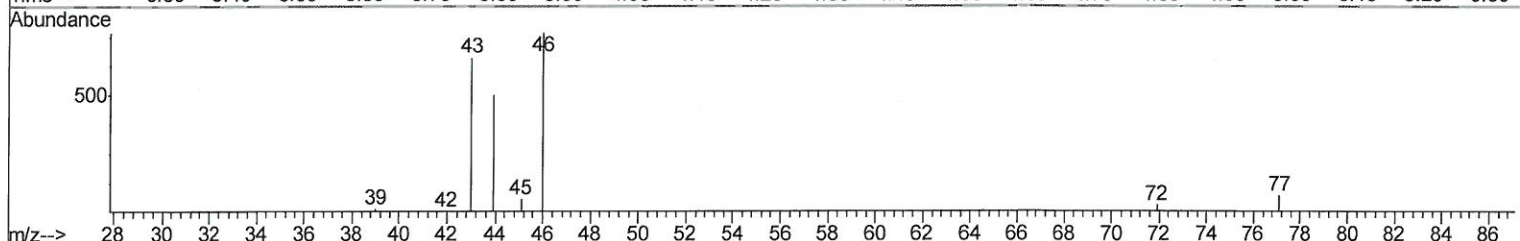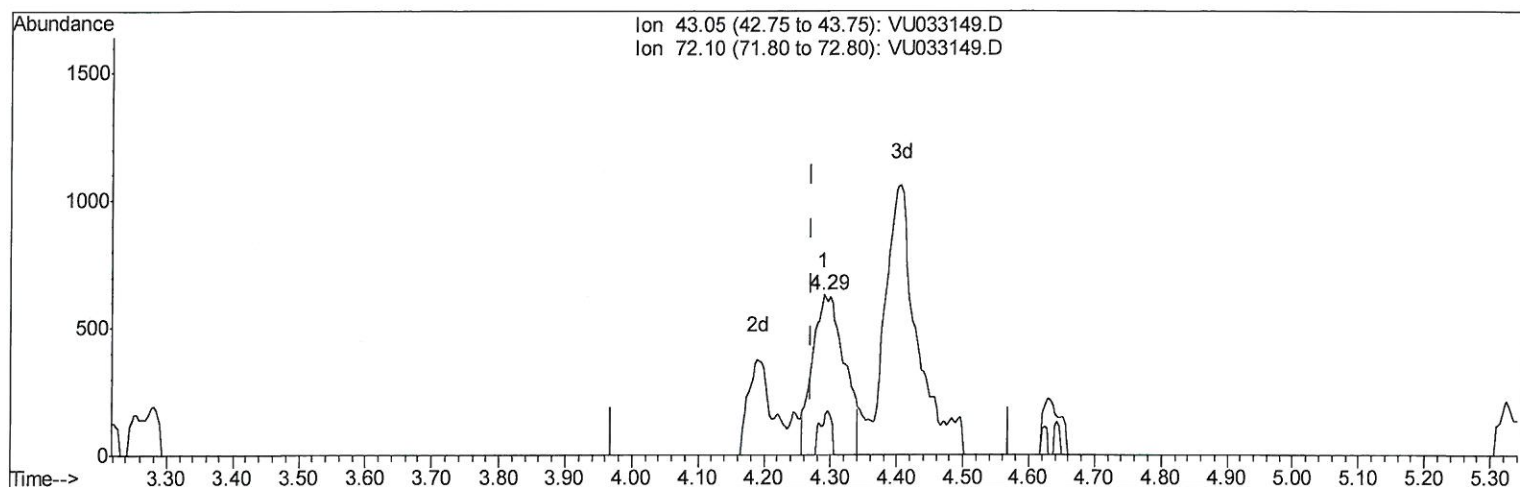

TIC: VU033149.D

(21) 2-Butanone (T)

4.289min (+0.019) 1.02ug/L m

response 2080

Ion Exp% Act%

43.05 100 100

72.10 24.20 9.95#

0.00 0.00 0.00

0.00 0.00 0.00

> 110
713119

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU070219\
Quantitation Report (QT Reviewed)

Data File : VU033149.D
Acq On : 02 Jul 2019 18:35
Operator : JC/SP
Sample : K3597-09DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAM66DL

Manual Integrations
APPROVED

MMDadoda
7/3/2019 11:34:56 AM

Quant Time: Jul 03 03:55:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 03 02:14:33 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	83141	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	88434	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	44183	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	33021	6.86	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	137.20%#
7) Chloroethane-d5	1.64	69	30113	6.84	ug/L	-0.03
Spiked Amount	5.000	Range	65 - 130	Recovery	=	136.80%#
11) 1,1-Dichloroethene-d2	2.26	63	51370	4.53	ug/L	-0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.60%
20) 2-Butanone-d5	4.19	46	99934	57.04	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.08%
24) Chloroform-d	4.64	84	62984	5.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.60%
26) 1,2-Dichloroethane-d4	5.30	65	36605	5.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.20%
32) Benzene-d6	5.33	84	117976	5.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.20%
36) 1,2-Dichloropropane-d6	6.32	67	38515	5.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.20%
41) Toluene-d8	7.56	98	103483	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.40%
43) trans-1,3-Dichloropropene-	7.85	79	14726	4.85	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.00%
46) 2-Hexanone-d5	8.31	63	67160	53.65	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.30%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	33852	5.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	45229	5.69	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.80%

Target Compounds

					Qvalue
13) Acetone	2.32	43	3787	2.689	ug/L 85
21) 2-Butanone	4.29	43	2080m	1.021	ug/L
47) Tetrachloroethene	8.22	164	43738	7.406	ug/L 95

7 MQ
7/3/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed