

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070219\
 Data File : VU033137.D
 Acq On : 02 Jul 2019 13:45
 Operator : JC/SP
 Sample : K3608-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAML2

Quant Time: Jul 03 02:35:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 03 02:14:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	90335	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	92514	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	44884	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	35750	6.84	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	136.80%#
7) Chloroethane-d5	1.68	69	29084	6.08	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	121.60%
11) 1,1-Dichloroethene-d2	2.27	63	54282	4.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.20%
20) 2-Butanone-d5	4.19	46	92783	48.74	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.48%
24) Chloroform-d	4.64	84	64659	5.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.40%
26) 1,2-Dichloroethane-d4	5.31	65	37369	5.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.40%
32) Benzene-d6	5.33	84	123091	5.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.80%
36) 1,2-Dichloropropane-d6	6.32	67	39713	5.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.60%
41) Toluene-d8	7.56	98	109800	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.80%
43) trans-1,3-Dichloropropene-	7.85	79	15601	4.91	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.20%
46) 2-Hexanone-d5	8.31	63	59023	45.07	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.14%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	31252	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	43308	5.36	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	5279	3.449 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070219\
Data File : VU033137.D
Acq On : 02 Jul 2019 13:45
Operator : JC/SP
Sample : K3608-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAML2

Quant Time: Jul 03 02:35:17 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 03 02:14:33 2019
Response via : Initial Calibration

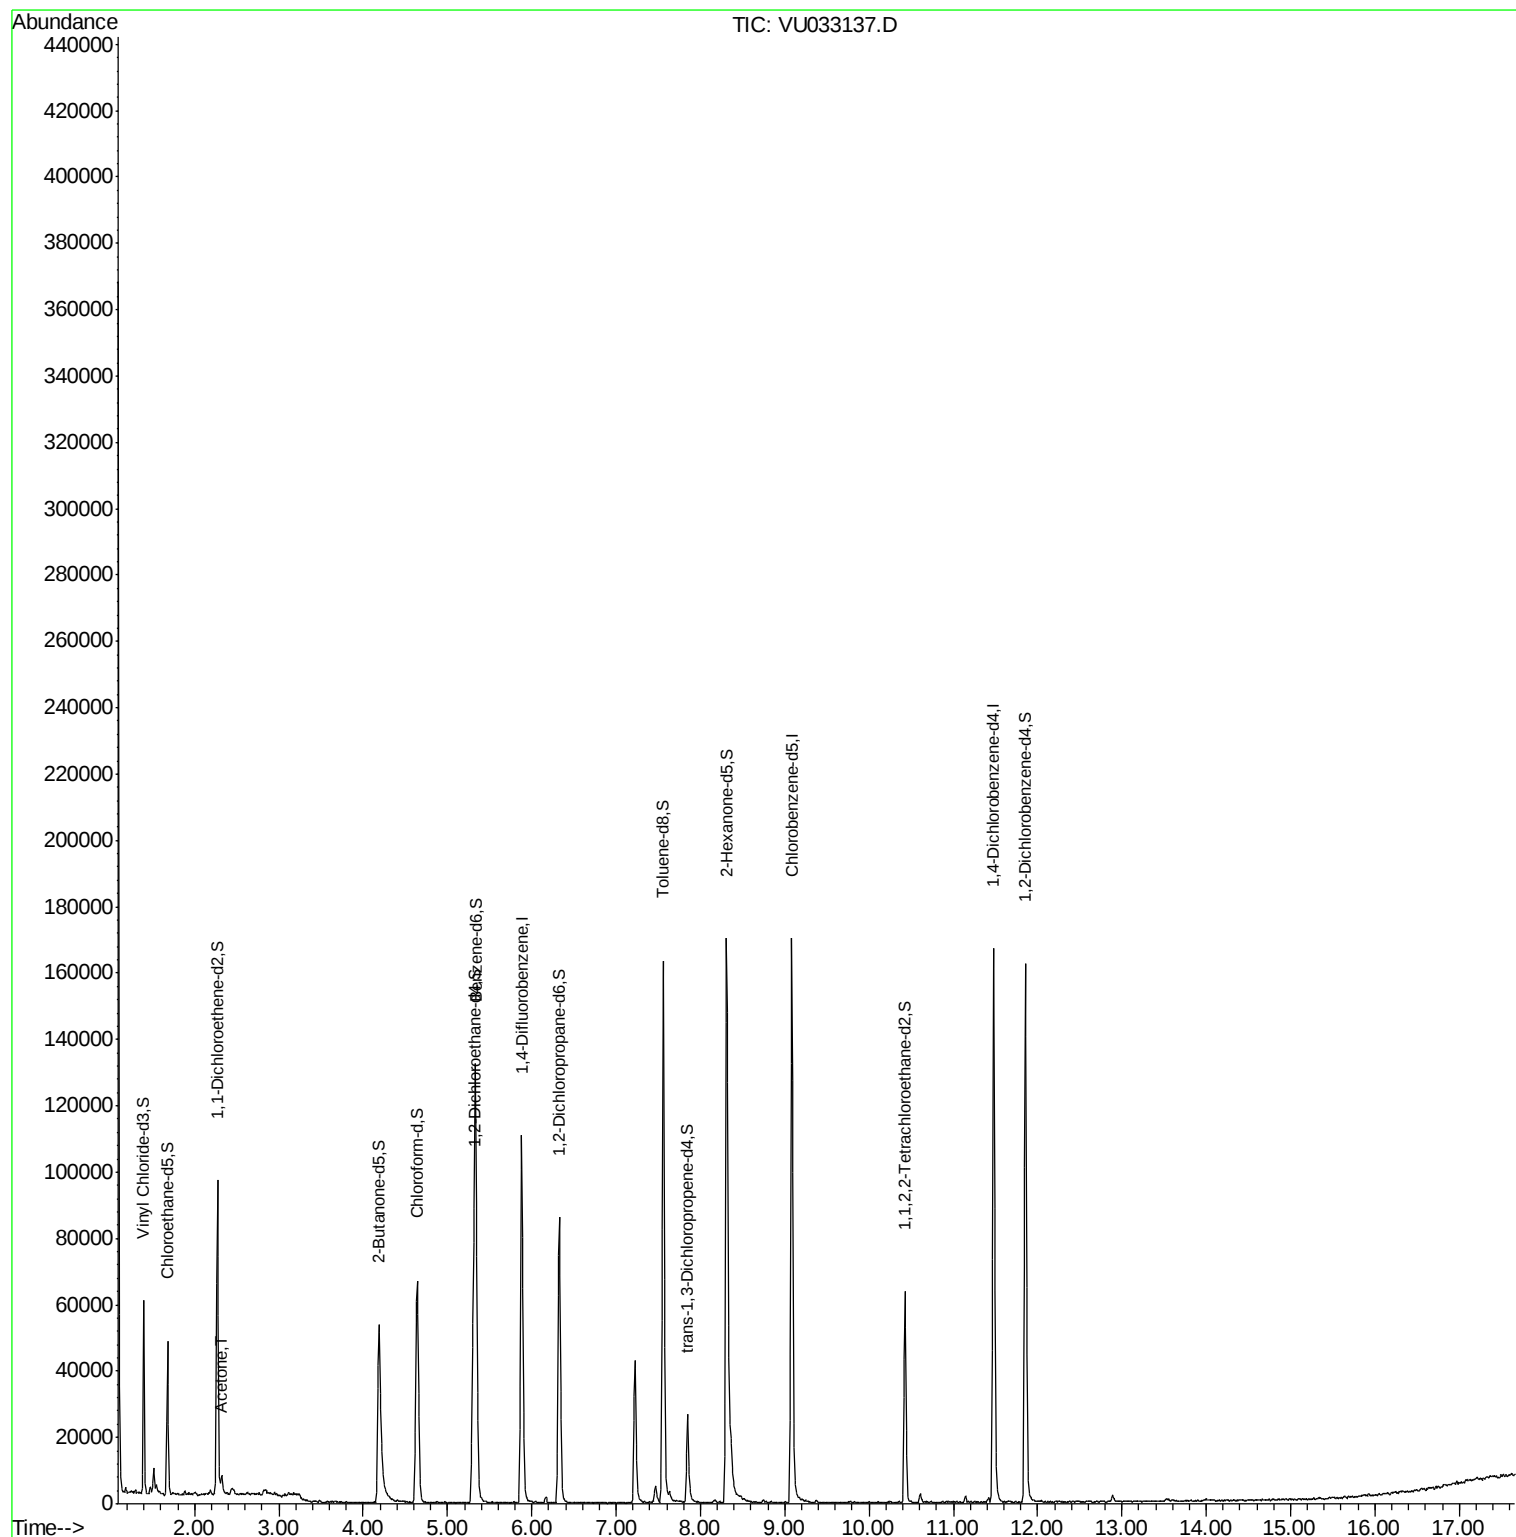

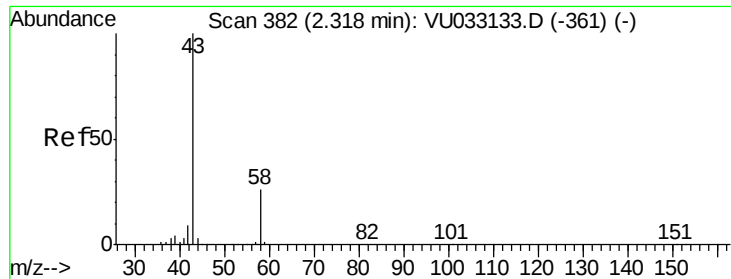

#13

Acetone

Concen: 3.449 ug/L

RT: 2.32 min Scan# 382

Delta R.T. -0.00 min

Lab File: VU033137.D

Acq: 02 Jul 2019 13:45

Instrument :

MSVOA_U

ClientSampleId :

GAML2

Tot Ion: 43 Resp: 5279

Ion Ratio Lower Upper

43 100

58 26.9 0.0 55.4

