

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070219\
 Data File : VU033141.D
 Acq On : 02 Jul 2019 15:22
 Operator : JC/SP
 Sample : K3608-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAML3

Quant Time: Jul 03 02:54:41 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 03 02:14:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	87063	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	89674	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	43001	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	37009	7.34	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	146.80%#
7) Chloroethane-d5	1.68	69	28942	6.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	125.60%
11) 1,1-Dichloroethene-d2	2.27	63	56683	4.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	95.40%
20) 2-Butanone-d5	4.19	46	97415	53.10	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.20%
24) Chloroform-d	4.64	84	66925	5.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.20%
26) 1,2-Dichloroethane-d4	5.31	65	37632	5.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.20%
32) Benzene-d6	5.33	84	126752	5.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	117.80%
36) 1,2-Dichloropropane-d6	6.32	67	40834	5.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	114.00%
41) Toluene-d8	7.56	98	112252	5.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.40%
43) trans-1,3-Dichloropropene-	7.85	79	16203	5.26	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	105.20%
46) 2-Hexanone-d5	8.31	63	63594	50.10	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.20%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	33062	5.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.20%
64) 1,2-Dichlorobenzene-d4	11.85	152	45147	5.83	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.60%


Target Compounds				Ovalue
13) Acetone	2.32	43	3645	2.471 ug/L 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070219\
Data File : VU033141.D
Acq On : 02 Jul 2019 15:22
Operator : JC/SP
Sample : K3608-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAML3

Quant Time: Jul 03 02:54:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 03 02:14:33 2019
Response via : Initial Calibration

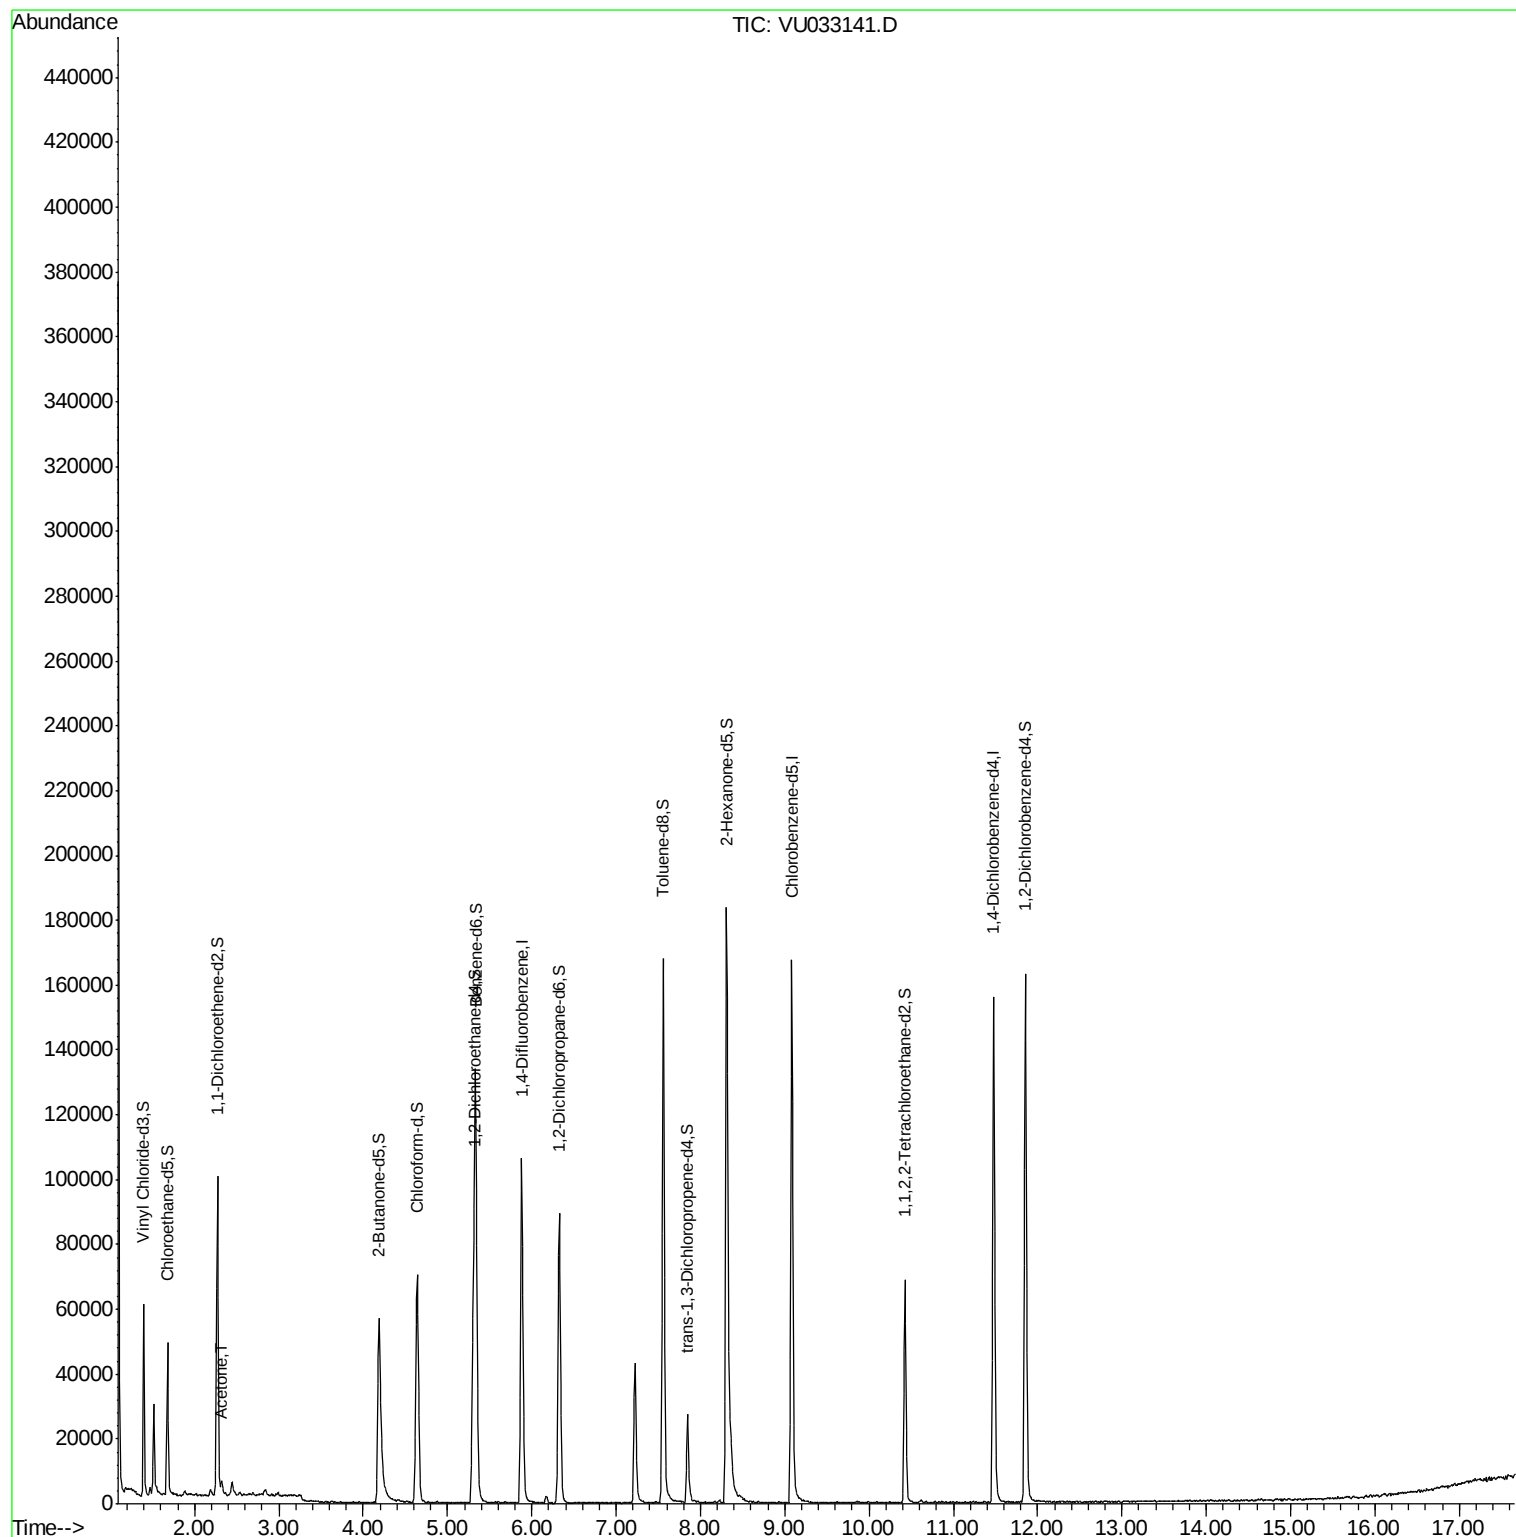

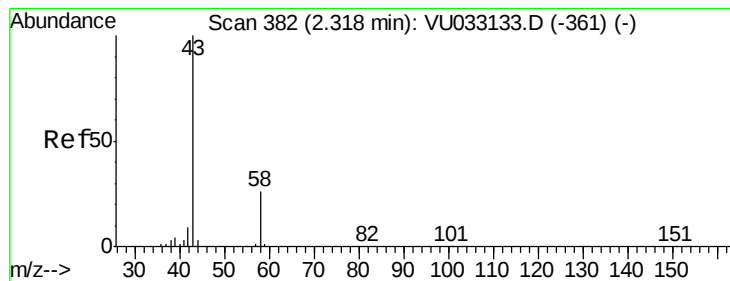

#13
Acetone
Concen: 2.471 ug/L
RT: 2.32 min Scan# 382
Delta R.T. -0.00 min
Lab File: VU033141.D
Acq: 02 Jul 2019 15:22

Instrument :
MSVOA_U
ClientSampleId :
GAML3

Tot Ion: 43 Resp: 3645
Ion Ratio Lower Upper
43 100
58 24.0 0.0 55.4

