


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU070219\
Data File : VU033126.D
Acq On : 02 Jul 2019 08:24
Operator : JC/SP
Sample : BFB23
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB23

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Jul 03 02:14:33 2019

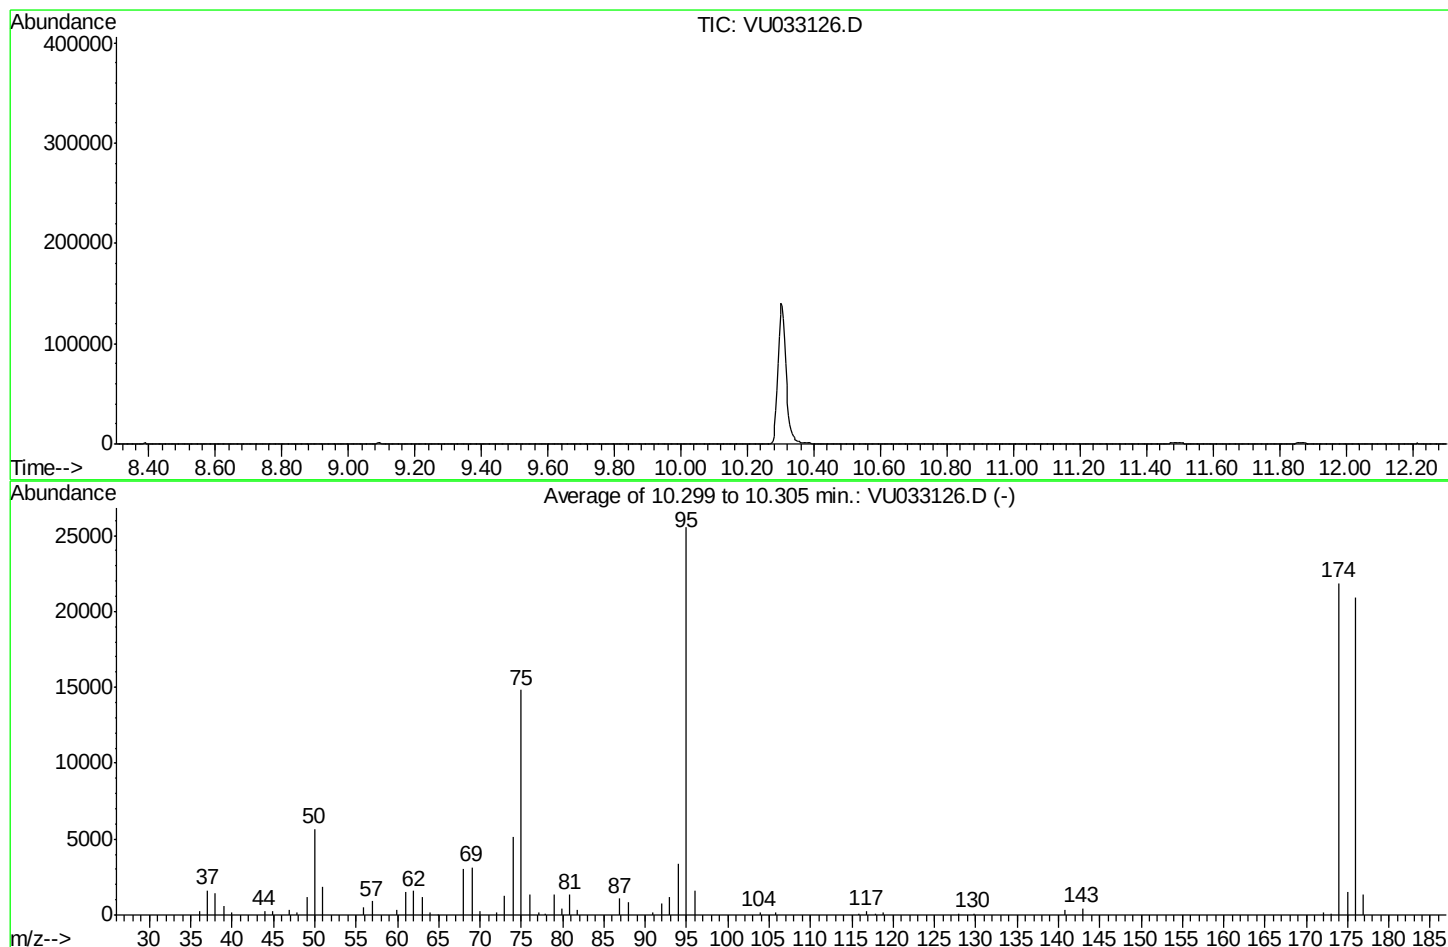

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	5686	PASS
75	95	30	80	58.0	14815	PASS
95	95	100	100	100.0	25536	PASS
96	95	5	9	6.2	1579	PASS
173	174	0.00	2	0.6	124	PASS
174	95	50	120	85.7	21877	PASS
175	174	5	9	7.1	1549	PASS
176	174	95	101	95.8	20952	PASS
177	176	5	9	6.4	1336	PASS

m/z	Abundance
43.90	239.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.00	246.0
37.00	1570.0
38.00	1433.0
39.00	608.0
40.00	143.0
43.90	529.0
45.00	224.0
47.10	288.0
47.80	163.0
49.00	1160.0
50.00	5411.0
51.00	1766.0
56.00	476.0
57.00	877.0
60.00	312.0
61.00	1404.0
62.00	1427.0
63.00	1113.0
64.00	178.0
64.90	103.0
68.00	2988.0
69.00	2993.0
70.00	204.0
72.00	159.0
73.00	1177.0
74.00	4957.0
75.00	14188.0
76.00	1288.0
77.10	122.0
77.90	116.0
78.90	1357.0
79.90	366.0
80.90	1191.0
81.80	314.0
87.00	1141.0
88.00	798.0
91.00	156.0
92.00	791.0
93.00	1126.0
94.10	3209.0
95.00	24512.0
96.00	1492.0
103.90	169.0
105.80	120.0
115.90	122.0
116.80	254.0
118.90	178.0
127.90	101.0
129.70	125.0
140.80	375.0
142.90	389.0
172.10	179.0
174.00	20496.0
175.00	1398.0
176.00	19544.0
177.00	1265.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.00	241.0
37.00	1695.0
38.00	1446.0
39.00	616.0
39.90	134.0
43.90	511.0
45.00	233.0
46.90	345.0
47.90	179.0
49.00	1185.0
50.00	5805.0
51.00	1959.0
55.90	525.0
57.00	929.0
60.00	331.0
61.00	1511.0
62.00	1630.0
63.00	1247.0
63.90	174.0
68.00	3185.0
69.00	3233.0
70.10	231.0
71.90	186.0
73.00	1292.0
74.00	5343.0
75.00	15414.0
76.00	1414.0
77.10	126.0
77.90	121.0
78.90	1383.0
79.90	436.0
80.90	1409.0
81.80	313.0
87.00	1121.0
88.00	898.0
91.00	184.0
92.00	843.0
93.00	1200.0
94.10	3412.0
95.00	26368.0
96.10	1644.0
103.90	221.0
105.90	148.0
115.90	130.0
116.80	272.0
117.80	102.0
118.80	170.0
127.90	110.0
129.80	133.0
140.80	393.0
142.90	445.0
172.00	194.0
174.00	22496.0
175.00	1615.0
176.00	21536.0
176.90	1376.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.00	227.0
37.00	1675.0
38.00	1373.0
39.00	572.0
39.90	126.0
43.90	463.0
44.90	233.0
46.90	356.0
47.90	188.0
49.00	1124.0
50.00	5843.0
51.00	1898.0
55.90	539.0
56.90	921.0
59.90	322.0
61.00	1529.0
62.00	1655.0
63.00	1249.0
63.90	172.0
68.00	3067.0
69.00	3147.0
70.10	223.0
71.90	182.0
73.00	1322.0
74.00	5135.0
75.00	14844.0
76.00	1352.0
77.00	148.0
77.90	107.0
78.90	1337.0
79.90	416.0
80.90	1411.0
81.80	282.0
86.90	946.0
88.00	924.0
90.90	167.0
92.00	776.0
92.90	1231.0
94.00	3468.0
95.00	25728.0
96.10	1603.0
103.90	243.0
105.90	164.0
115.80	126.0
116.80	242.0
117.90	133.0
118.80	174.0
127.90	113.0
129.80	123.0
140.90	329.0
142.90	445.0
171.90	218.0
173.00	372.0
174.00	22640.0
175.00	1635.0
176.00	21776.0
176.90	1368.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23