
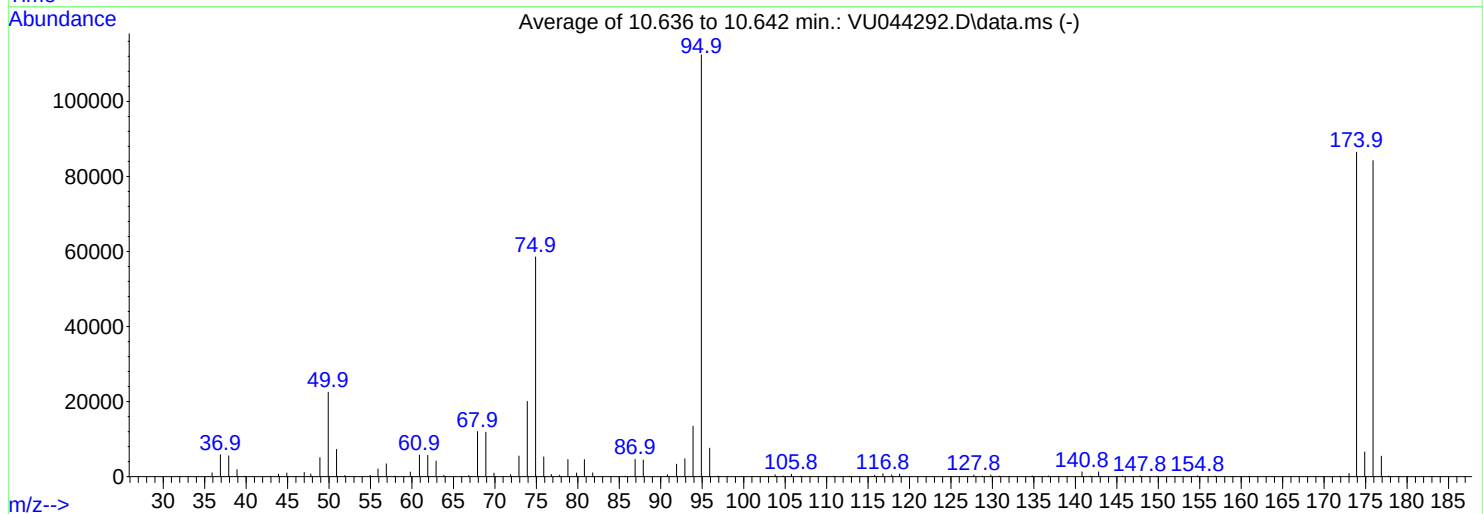


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070221\
 Data File : VU044292.D
 Acq On : 02 Jul 2021 09:10
 Operator : SY/MD
 Sample : BFB49
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB003

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR062121WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Jul 03 04:56:00 2021

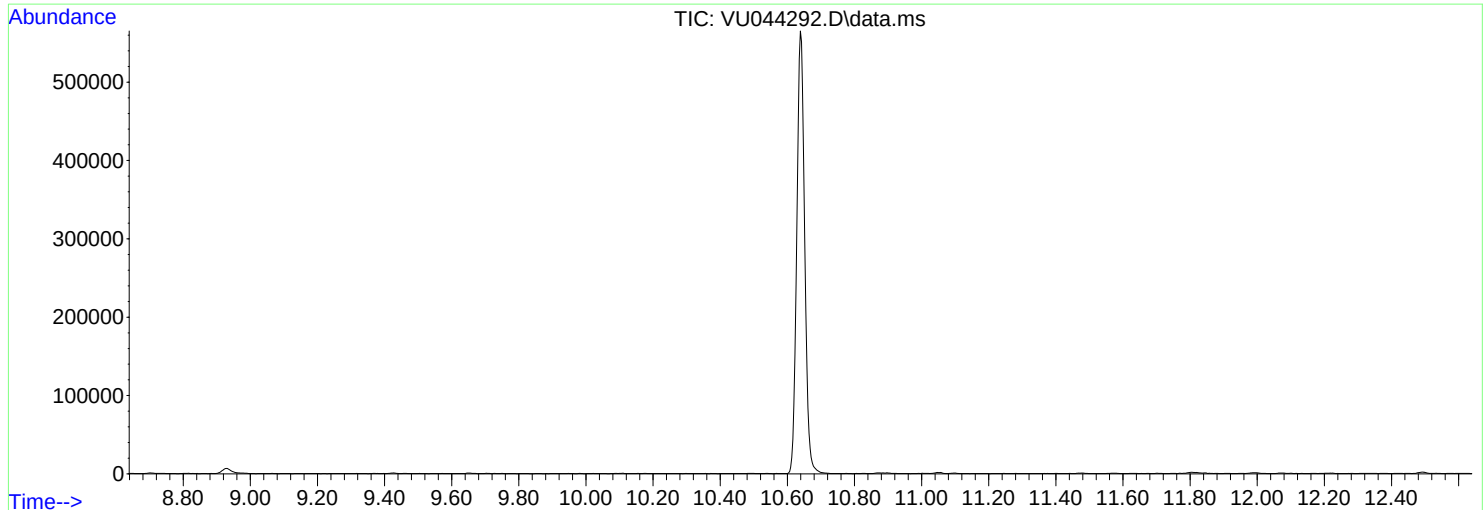

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	22515	PASS
75	95	30	80	52.1	58565	PASS
95	95	100	100	100.0	112405	PASS
96	95	5	9	6.8	7601	PASS
173	174	0.00	2	1.0	856	PASS
174	95	50	120	76.9	86464	PASS
175	174	5	9	7.6	6582	PASS
176	174	95	101	97.4	84224	PASS
177	176	5	9	6.5	5479	PASS

m/z	Abundance
35.90	1034.0
36.90	5719.0
37.90	5431.0
38.90	1799.0
39.90	144.0
42.90	125.0
43.90	1042.0
44.90	969.0
47.00	1127.0
47.80	772.0
48.90	4947.0
49.90	22048.0
50.90	7125.0
51.90	282.0
55.00	335.0
55.90	2034.0
56.90	3420.0
58.00	160.0
59.80	1234.0
60.90	5689.0
61.90	5619.0
62.90	4113.0
63.90	365.0
66.80	338.0
67.90	11967.0
68.90	11857.0
69.90	917.0
71.90	529.0
72.90	5293.0
73.90	19840.0
74.90	58152.0
75.90	5072.0
76.80	565.0
77.90	373.0
78.80	4389.0
79.80	1013.0
80.80	4515.0
81.80	1029.0
83.00	138.0
85.70	122.0
86.90	4645.0
87.90	4259.0
90.80	557.0
91.90	3164.0
92.90	4822.0
93.90	13573.0
94.90	111856.0
95.90	7454.0
96.90	217.0
103.80	531.0
104.80	170.0
105.80	631.0
106.90	127.0
110.80	147.0
111.70	103.0
112.80	142.0
115.80	332.0
116.80	823.0
117.90	493.0
118.80	697.0
127.80	415.0
128.80	168.0
129.80	427.0
130.80	170.0
134.80	196.0
136.80	183.0
140.80	1211.0
141.80	161.0
142.80	1295.0
144.80	123.0
145.70	143.0
147.80	286.0
149.80	105.0
154.70	267.0
156.80	215.0
160.90	115.0
171.90	159.0
173.00	901.0
173.90	89368.0
174.90	6649.0
175.90	86664.0
176.90	5549.0
177.80	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
43.90	371.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
35.90	978.0
36.90	5796.0
37.90	5470.0
38.90	1936.0
39.80	157.0
42.90	108.0
43.90	1060.0
44.90	959.0
47.00	1123.0
47.80	693.0
48.90	5044.0
49.90	22280.0
50.90	7113.0
51.90	311.0
54.90	310.0
55.90	1963.0
56.90	3336.0
57.90	175.0
59.80	1172.0
60.90	5627.0
61.90	5557.0
62.90	4112.0
63.80	353.0
66.90	297.0
67.90	11584.0
68.90	11562.0
69.90	965.0
71.90	569.0
72.90	5578.0
73.90	19688.0
74.90	57296.0
75.90	5210.0
76.80	636.0
77.80	382.0
78.80	4571.0
79.90	962.0
80.80	4464.0
81.80	971.0
82.90	145.0
85.70	100.0
86.90	4452.0
87.90	4389.0
90.80	462.0
91.90	3399.0
92.90	4657.0
93.90	12898.0
94.90	109544.0
95.90	7472.0
96.90	165.0
103.80	498.0
104.70	160.0
105.70	598.0
106.80	116.0
110.90	119.0
112.70	137.0
115.80	356.0
116.80	687.0
117.80	435.0
118.80	646.0
127.70	447.0
128.80	162.0
129.80	425.0
130.80	159.0
134.80	221.0
136.70	204.0
140.80	1278.0
141.80	142.0
142.80	1200.0
145.70	159.0
147.80	228.0
149.70	114.0
154.80	199.0
156.90	161.0
158.90	112.0
171.80	126.0
173.00	792.0
173.90	81088.0
174.90	6265.0
175.90	79328.0
176.90	5247.0
177.80	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
35.90	1087.0
36.90	6030.0
37.90	5705.0
38.90	1940.0
39.80	146.0
42.90	114.0
43.90	1092.0
44.90	1010.0
47.00	1166.0
47.80	747.0
48.90	5267.0
49.90	23216.0
50.90	7482.0
51.90	321.0
55.00	336.0
55.90	2110.0
56.90	3505.0
58.00	173.0
59.80	1272.0
60.90	5952.0
61.90	5800.0
62.90	4233.0
63.90	373.0
66.80	335.0
67.90	12493.0
68.90	12149.0
69.90	967.0
71.90	599.0
72.90	5692.0
73.90	20640.0
74.90	60248.0
75.90	5406.0
76.80	623.0
77.70	391.0
78.80	4718.0
79.90	1015.0
80.80	4681.0
81.80	1025.0
83.00	134.0
85.70	124.0
86.90	4755.0
87.90	4623.0
90.80	513.0
91.90	3438.0
92.90	4852.0
93.90	13895.0
94.90	115816.0
95.90	7877.0
96.90	200.0
103.80	548.0
104.70	167.0
105.70	647.0
106.80	128.0
110.80	130.0
112.80	157.0
115.80	353.0
116.80	799.0
117.80	492.0
118.80	707.0
127.80	461.0
128.80	155.0
129.80	444.0
130.80	175.0
134.80	229.0
136.70	216.0
140.80	1322.0
141.80	159.0
142.80	1285.0
145.70	162.0
147.80	273.0
149.70	106.0
154.70	259.0
156.80	185.0
160.90	112.0
171.80	148.0
173.00	874.0
173.90	88936.0
174.90	6833.0
175.90	86680.0
176.90	5642.0
177.80	172.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003