


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU070319\
Data File : VU033159.D
Acq On : 03 Jul 2019 09:20
Operator : JC/SP
Sample : BFB33
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB33

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Title : VOC Analysis
Last Update : Wed Jul 03 22:32:40 2019

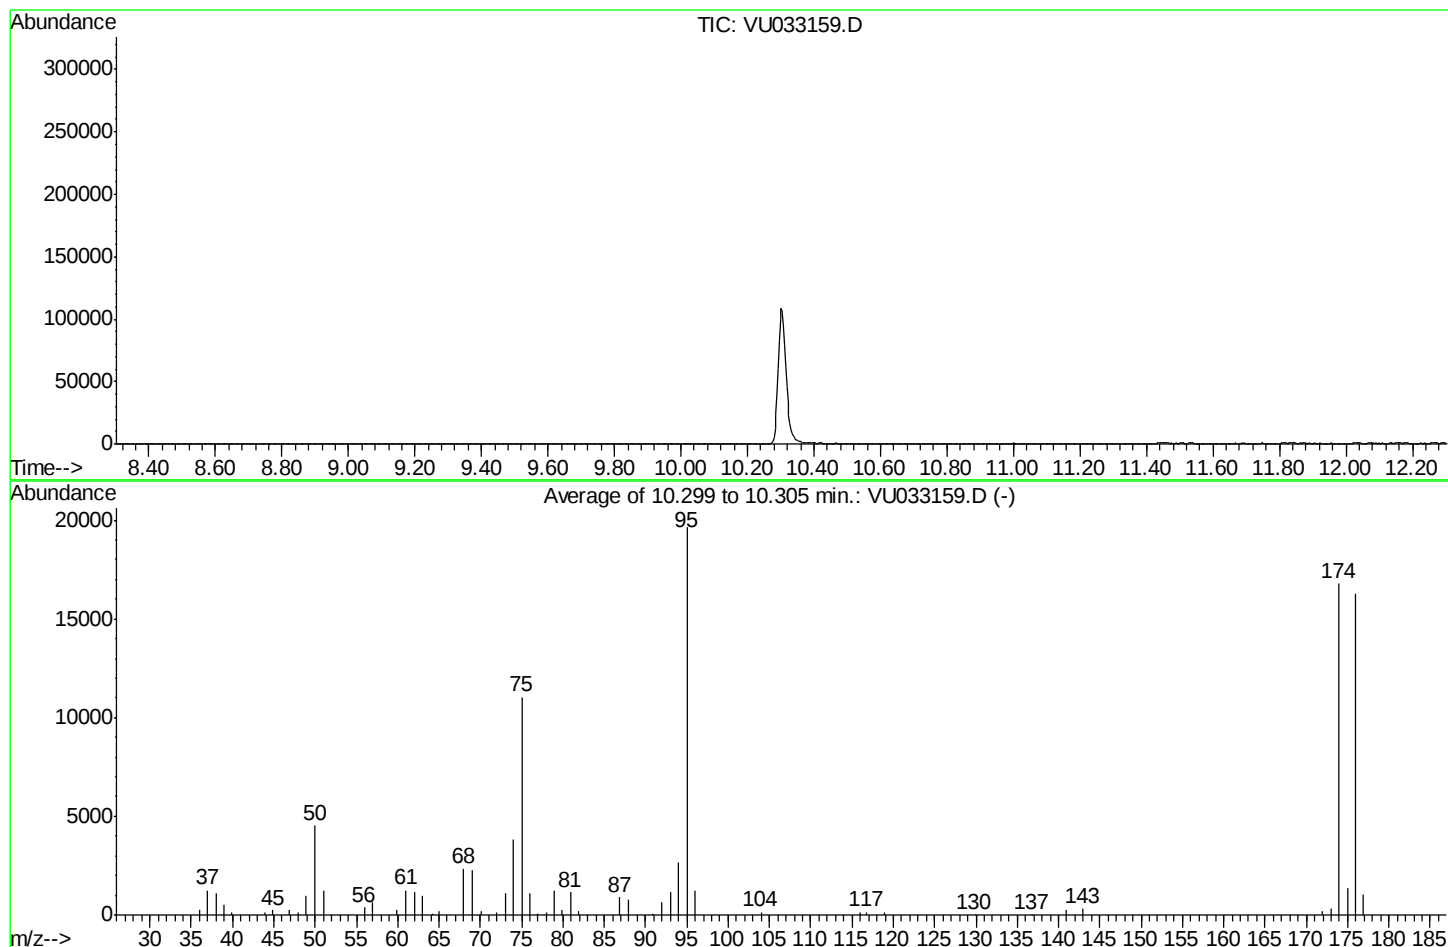

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	4529	PASS
75	95	30	80	56.2	11042	PASS
95	95	100	100	100.0	19637	PASS
96	95	5	9	6.4	1256	PASS
173	174	0.00	2	1.8	301	PASS
174	95	50	120	85.4	16773	PASS
175	174	5	9	8.0	1334	PASS
176	174	95	101	97.1	16287	PASS
177	176	5	9	6.3	1021	PASS

m/z	Abundance
43.90	262.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
36.00	267.0
37.00	1200.0
38.00	1067.0
39.00	526.0
40.00	125.0
43.90	376.0
44.90	195.0
46.90	286.0
47.80	150.0
48.90	1023.0
50.00	4468.0
51.00	1130.0
55.90	370.0
57.00	626.0
60.00	249.0
61.00	1209.0
62.00	1210.0
63.00	996.0
64.20	111.0
65.00	151.0
68.00	2251.0
69.00	2161.0
70.00	170.0
72.00	149.0
73.00	979.0
74.00	3816.0
75.00	10661.0
76.00	1020.0
78.00	124.0
78.90	1151.0
79.90	271.0
80.90	1074.0
81.90	217.0
86.90	844.0
88.00	758.0
92.00	667.0
93.00	1139.0
94.00	2446.0
95.00	18792.0
96.00	1176.0
104.00	169.0
116.00	115.0
116.80	135.0
118.90	124.0
140.80	255.0
143.00	306.0
172.00	175.0
173.00	317.0
174.00	15393.0
175.00	1275.0
176.00	15573.0
176.90	1007.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
35.90	300.0
37.00	1277.0
38.00	1129.0
39.00	519.0
40.00	127.0
44.00	359.0
44.90	234.0
46.90	292.0
47.90	145.0
48.90	960.0
50.00	4702.0
51.00	1308.0
55.90	375.0
57.00	687.0
60.00	280.0
61.00	1292.0
62.00	1222.0
63.00	1020.0
64.20	136.0
65.00	170.0
68.00	2400.0
69.00	2335.0
70.10	216.0
72.00	160.0
73.00	1164.0
74.00	3993.0
75.00	11388.0
76.00	1120.0
77.00	109.0
77.90	144.0
78.90	1255.0
79.90	270.0
80.90	1204.0
81.90	218.0
86.90	910.0
87.90	824.0
90.80	102.0
92.00	729.0
93.00	1252.0
94.00	2740.0
95.00	20384.0
96.00	1272.0
104.00	168.0
115.90	114.0
116.80	162.0
118.90	158.0
129.90	100.0
136.80	103.0
140.80	288.0
143.00	330.0
171.80	183.0
173.00	307.0
174.00	17312.0
175.00	1382.0
176.00	16736.0
176.90	1038.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
35.00	269.0
37.00	1254.0
38.00	1094.0
39.00	483.0
39.00	113.0
44.00	374.0
44.00	259.0
46.00	238.0
48.00	140.0
48.00	864.0
50.00	4417.0
51.00	1297.0
56.00	370.0
57.00	670.0
59.00	285.0
61.00	1274.0
62.00	1143.0
63.00	959.0
64.00	182.0
68.00	2354.0
69.00	2295.0
70.10	217.0
72.00	134.0
73.00	1255.0
74.00	3593.0
75.00	11077.0
76.00	1120.0
77.00	131.0
78.00	1222.0
79.00	258.0
80.00	1192.0
81.00	198.0
86.00	884.0
87.00	765.0
90.00	101.0
92.00	644.0
93.00	1192.0
94.00	2714.0
95.00	19736.0
96.00	1320.0
104.00	133.0
115.00	116.0
116.00	179.0
118.00	194.0
140.00	308.0
142.00	319.0
171.00	197.0
173.00	279.0
174.00	17616.0
175.00	1346.0
176.00	16552.0
177.00	1019.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33