

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
 Data File : VU054752.D
 Acq On : 03 Jul 2023 16:29
 Operator : MD/SY
 Sample : 03505-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A46R9

Quant Time: Jul 05 04:43:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 05 04:39:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.248	114	248609	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	243881	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	114770	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	66246	4.187	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.800%
7) Chloroethane-d5	1.907	69	63401	4.280	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.600%
11) 1,1-Dichloroethene-d2	2.560	65	28005	3.963	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.200%
20) 2-Butanone-d5	4.624	46	255655	57.471	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.940%
24) Chloroform-d	5.058	84	142942	4.322	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.400%
26) 1,2-Dichloroethane-d4	5.698	65	74314	4.610	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.200%
32) Benzene-d6	5.724	84	259747	3.831	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.600%
36) 1,2-Dichloropropane-d6	6.689	67	94392	4.169	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.400%
41) Toluene-d8	7.894	98	219476	3.648	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.000%
43) trans-1,3-Dichloroprop...	8.177	79	34288	4.355	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.200%
46) 2-Hexanone-d5	8.631	63	172679	52.278	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.560%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	81294	4.815	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.400%
66) 1,2-Dichlorobenzene-d4	12.190	152	87640	4.527	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.600%
Target Compounds						
					Qvalue	
13) Acetone	2.631	43	96049	22.900	ug/L	99
16) Methylene chloride	3.042	84	27594	1.088	ug/L	96
21) 2-Butanone	4.721	43	17422	3.201	ug/L	98
33) Benzene	5.776	78	16465	0.188	ug/L	100
42) Toluene	7.968	91	267058	2.959	ug/L	99
47) Tetrachloroethene	8.554	164	4837	0.273	ug/L	96
48) 2-Hexanone	8.685	43	11977	1.271	ug/L #	74
49) Dibromochloromethane	8.554	129	4862	0.307	ug/L #	11
53) m,p-Xylene	9.689	106	10206	0.282	ug/L	93
54) o-Xylene	10.103	106	5635	0.161	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
Data File : VU054752.D
Acq On : 03 Jul 2023 16:29
Operator : MD/SY
Sample : 03505-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A46R9

Quant Time: Jul 05 04:43:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 05 04:39:25 2023
Response via : Initial Calibration

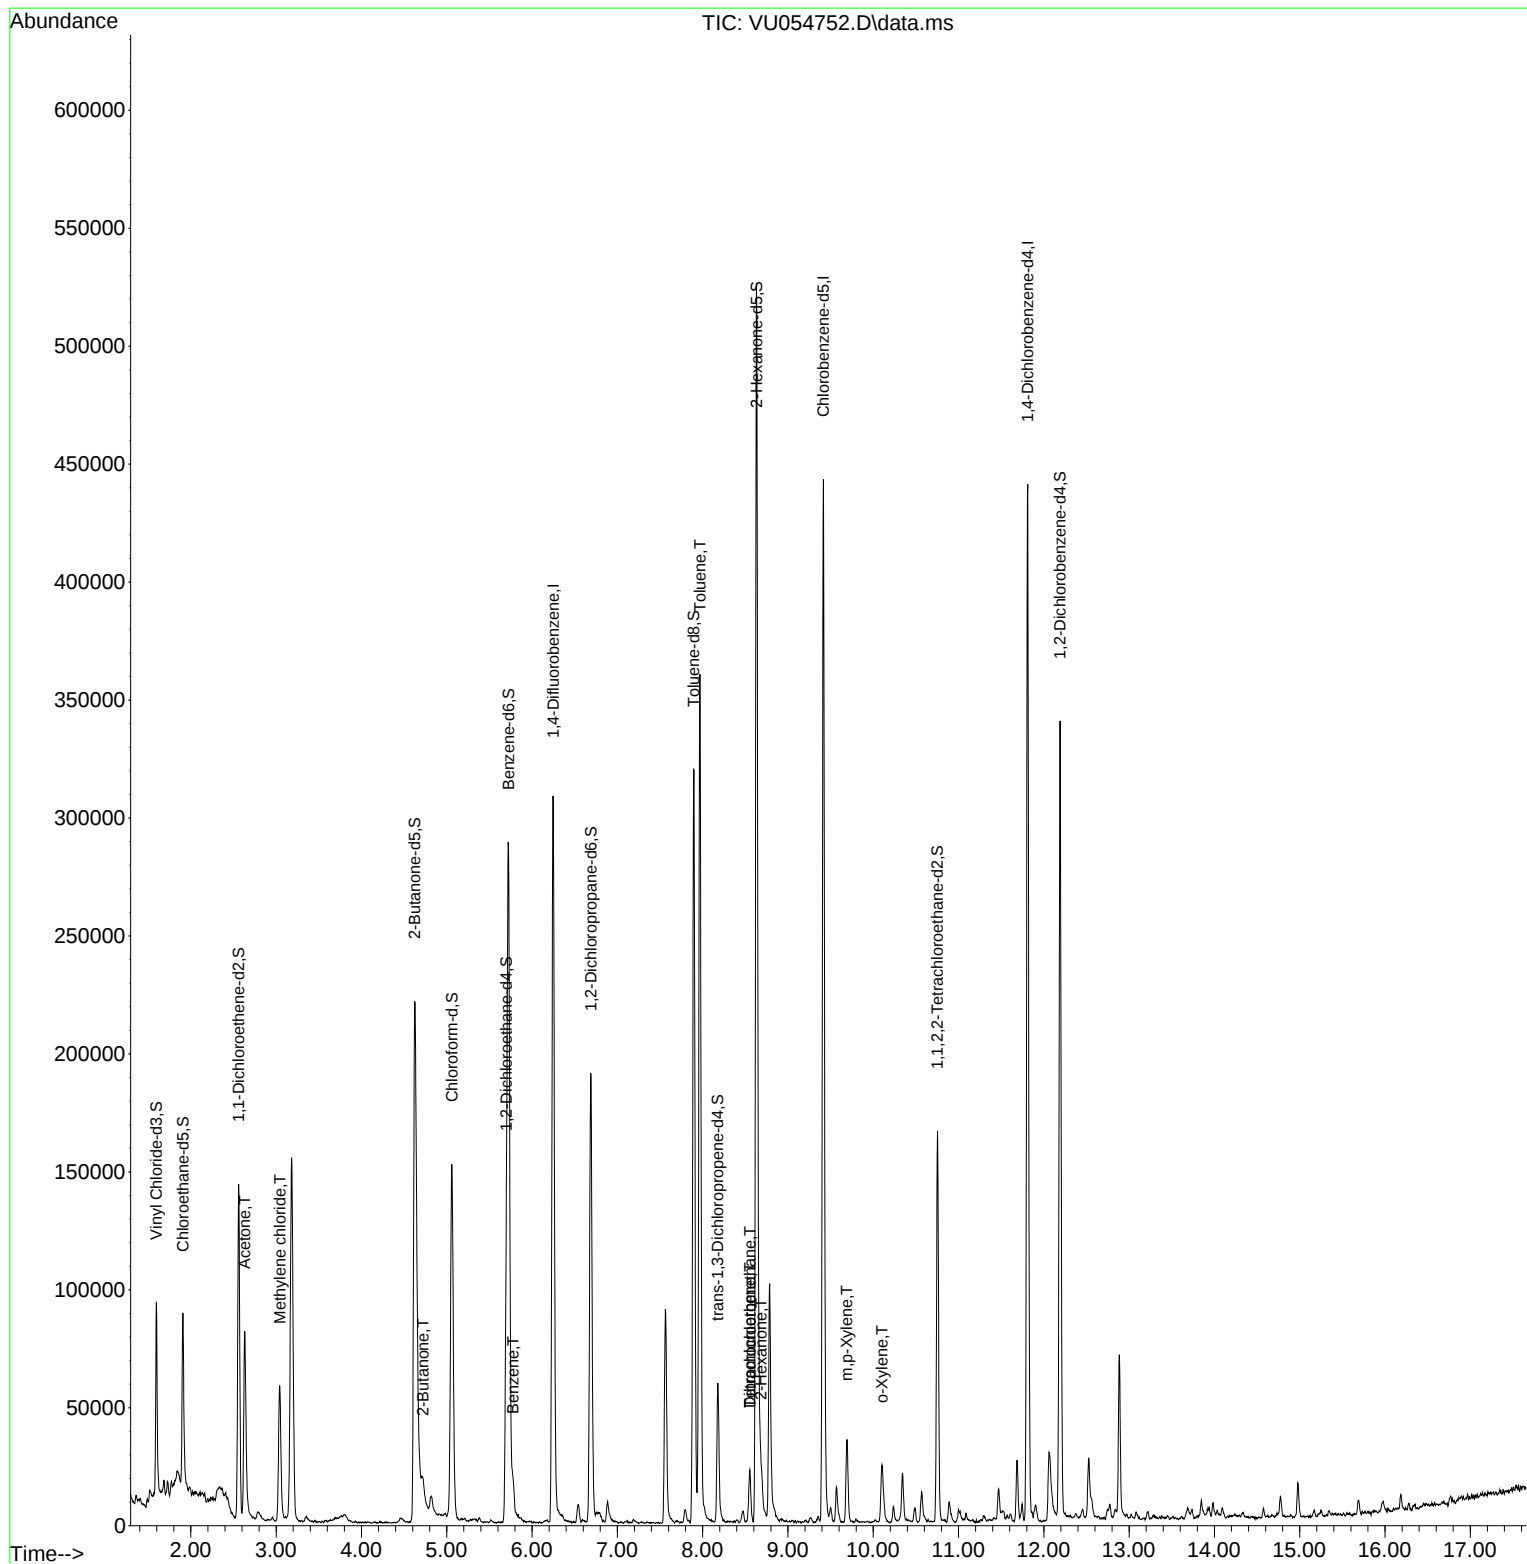

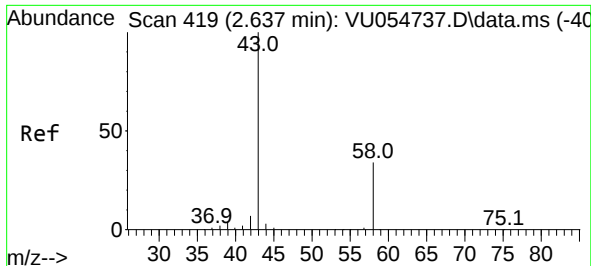

#13

Acetone

Concen: 22.900 ug/L

RT: 2.631 min Scan# 41

Delta R.T. -0.006 min

Lab File: VU054752.D

Acq: 03 Jul 2023 16:29

Instrument :

MSVOA_U

ClientSampleId :





A46R9

Tgt Ion: 43 Resp: 96049

Ion Ratio Lower Upper

43 100

58 33.2 0.0 67.2

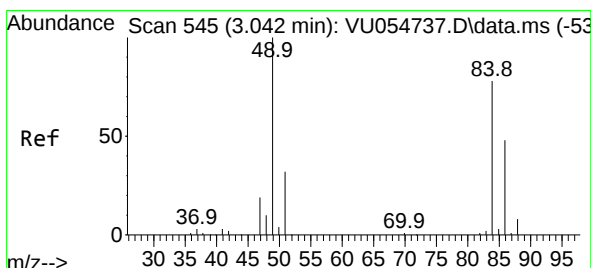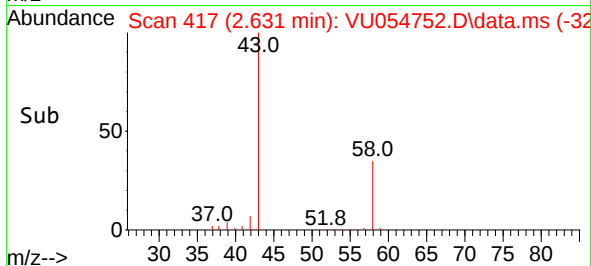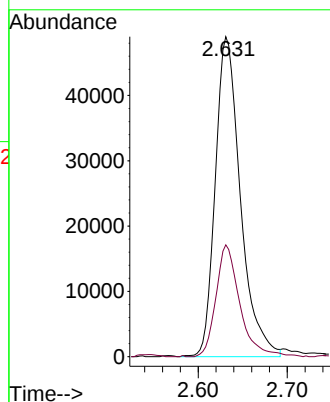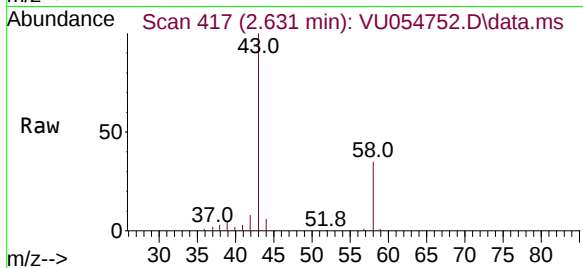

#16

Methylene chloride

Concen: 1.088 ug/L

RT: 3.042 min Scan# 545

Delta R.T. 0.000 min

Lab File: VU054752.D

Acq: 03 Jul 2023 16:29




Tgt Ion: 84 Resp: 27594


Ion Ratio Lower Upper

84 100

86 66.3 43.9 81.5

49 127.9 86.1 159.9

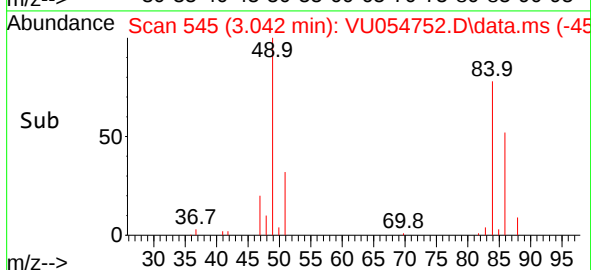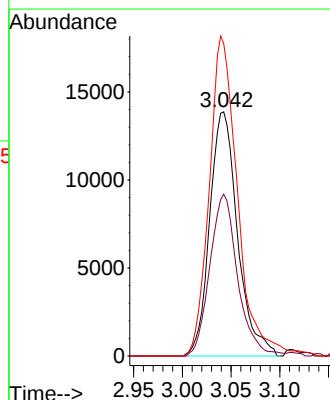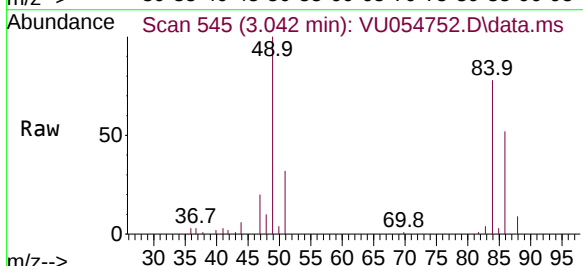

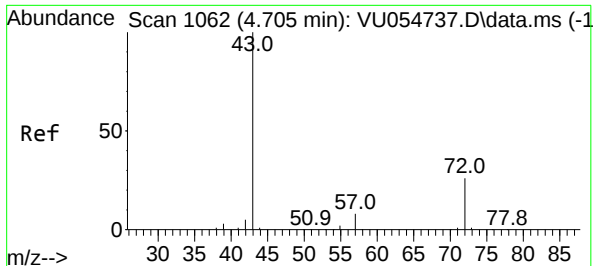

#21

2-Butanone

Concen: 3.201 ug/L

RT: 4.721 min Scan# 1067

Delta R.T. 0.016 min

Lab File: VU054752.D

Acq: 03 Jul 2023 16:29

Instrument :

MSVOA_U

ClientSampleId :





A46R9

Tgt Ion: 43 Resp: 17422

Ion Ratio Lower Upper

43 100

72 25.5 13.4 40.1

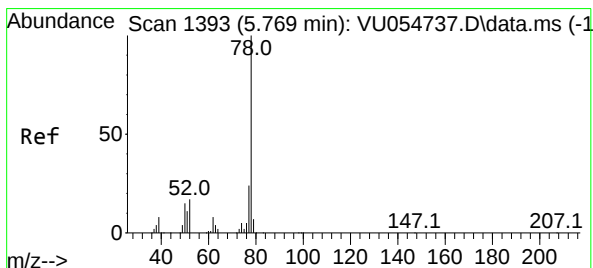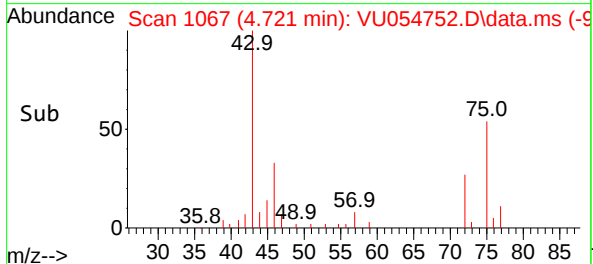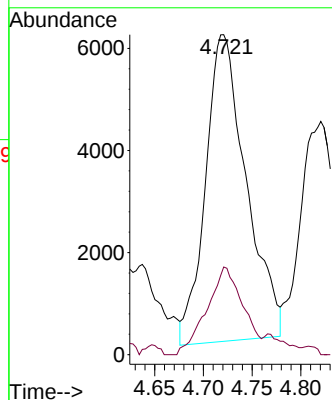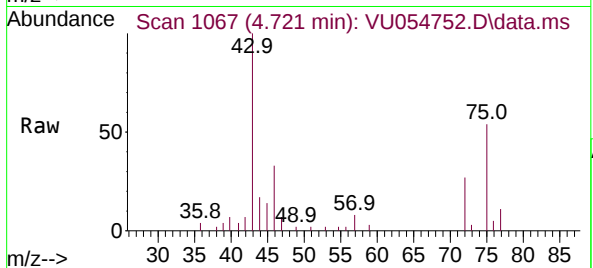

#33

Benzene

Concen: 0.188 ug/L




RT: 5.776 min Scan# 1395


Delta R.T. 0.007 min

Lab File: VU054752.D

Acq: 03 Jul 2023 16:29

Tgt Ion: 78 Resp: 16465


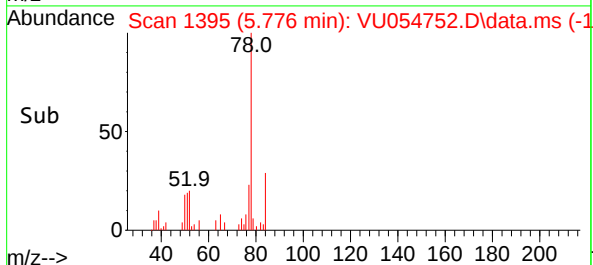
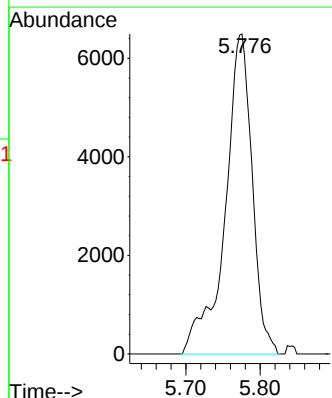
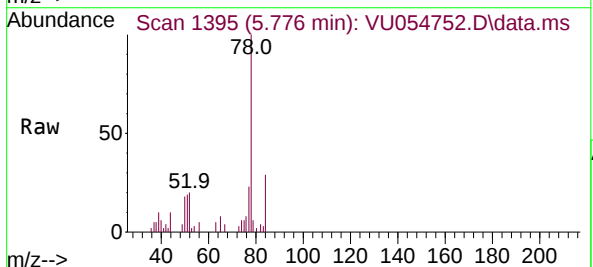


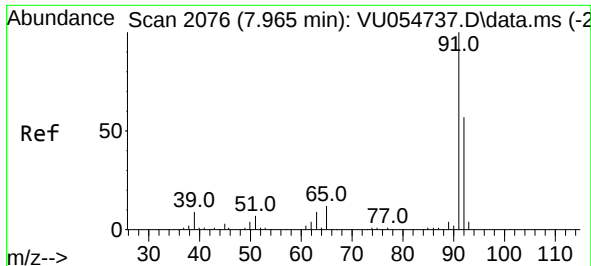

#42
Toluene
Concen: 2.959 ug/L
RT: 7.968 min Scan# 2076
Delta R.T. 0.003 min
Lab File: VU054752.D
Acq: 03 Jul 2023 16:29




Instrument :
MSVOA_U
ClientSampleId :
A46R9


Tgt Ion: 91 Resp: 267058
Ion Ratio Lower Upper
91 100
92 57.4 39.5 73.4

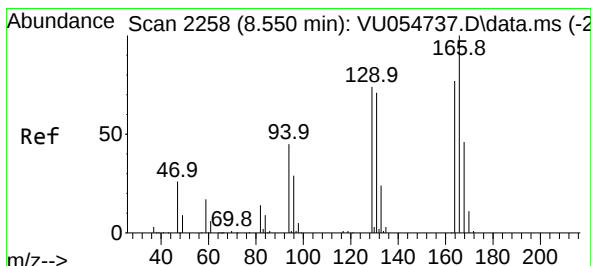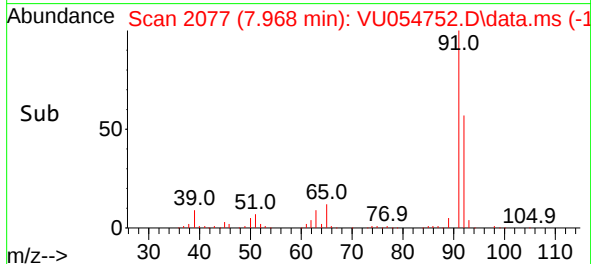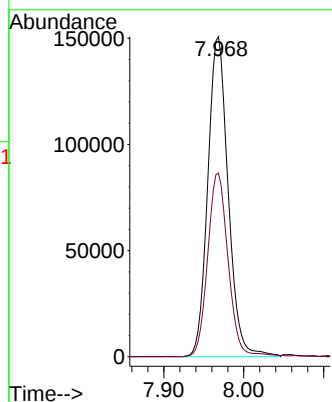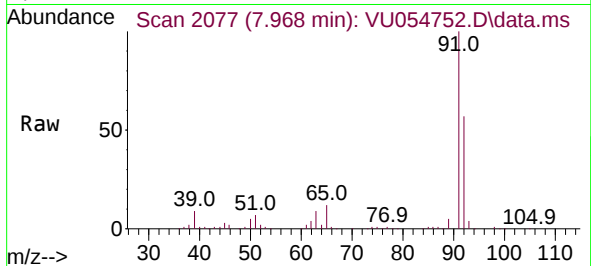

#47
Tetrachloroethene
Concen: 0.273 ug/L
RT: 8.554 min Scan# 2259
Delta R.T. 0.003 min
Lab File: VU054752.D
Acq: 03 Jul 2023 16:29

Tgt Ion: 164 Resp: 4837
Ion Ratio Lower Upper
164 100
129 102.8 67.7 125.7
131 94.1 64.6 120.0
166 122.0 88.1 163.7


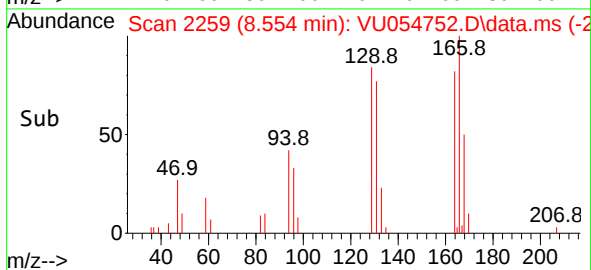
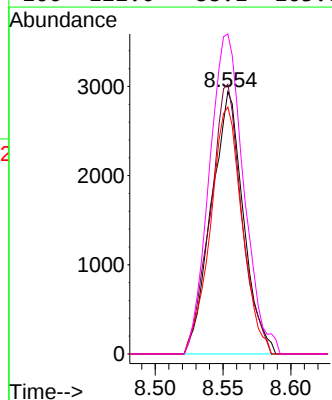
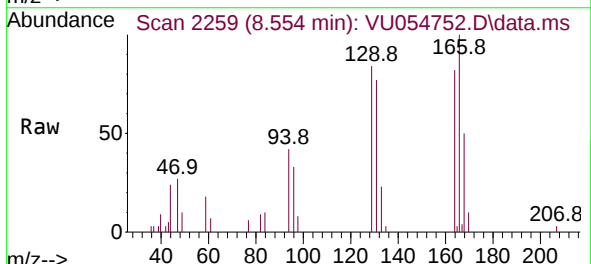


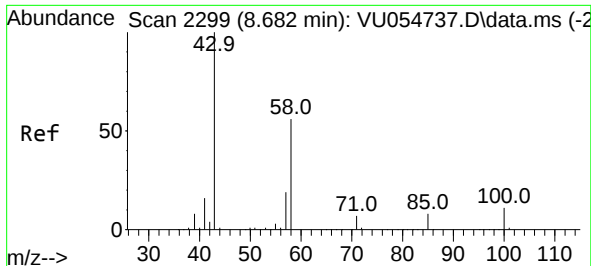

#48
2-Hexanone
Concen: 1.271 ug/L
RT: 8.685 min Scan# 2197
Delta R.T. 0.003 min
Lab File: VU054752.D
Acq: 03 Jul 2023 16:29




Instrument :
MSVOA_U
ClientSampleId :
A46R9


Tgt Ion: 43 Resp: 11977
Ion Ratio Lower Upper
43 100
58 33.0 45.2 67.8#
57 12.8 15.8 23.6#
100 5.6 8.7 13.1#

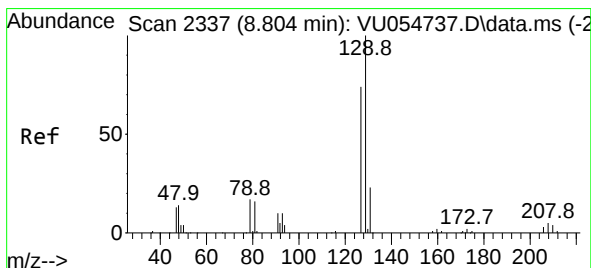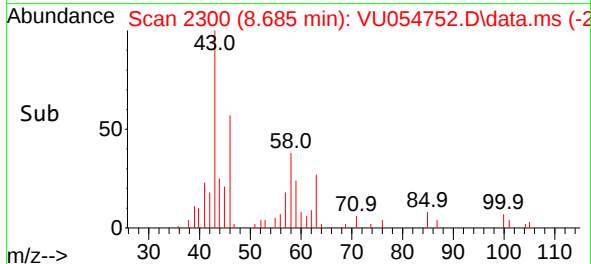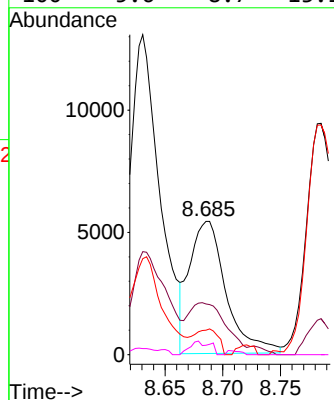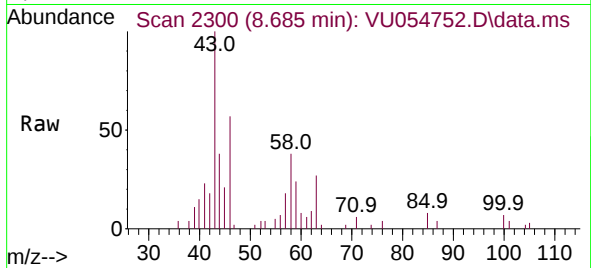

#49
Dibromochloromethane
Concen: 0.307 ug/L
RT: 8.554 min Scan# 2259
Delta R.T. -0.251 min
Lab File: VU054752.D
Acq: 03 Jul 2023 16:29

Tgt Ion: 129 Resp: 4862
Ion Ratio Lower Upper
129 100
127 0.0 53.2 98.8#


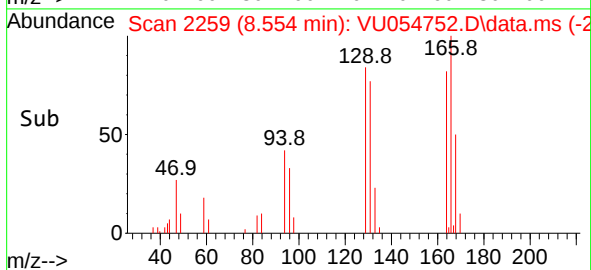
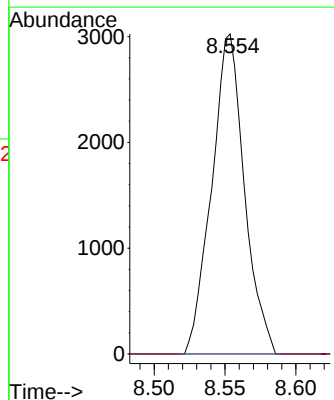
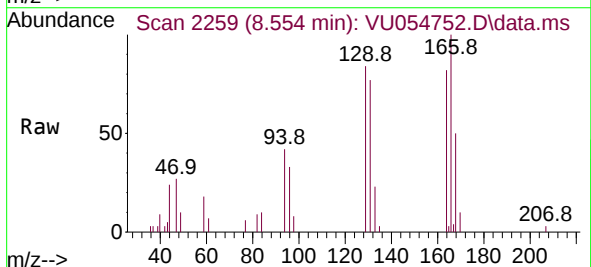


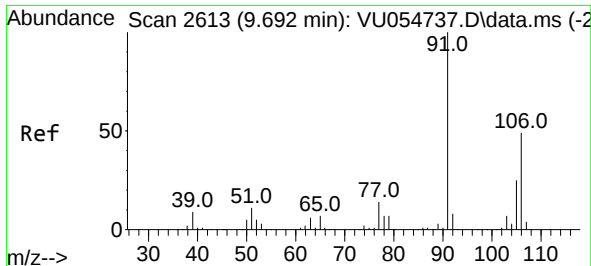

#53
m,p-Xylene
Concen: 0.282 ug/L
RT: 9.689 min Scan# 2741
Delta R.T. -0.003 min
Lab File: VU054752.D
Acq: 03 Jul 2023 16:29

Instrument :
MSVOA_U
ClientSampleId :
A46R9

Tgt Ion:106 Resp: 10206
Ion Ratio Lower Upper
106 100
91 199.3 147.0 273.0

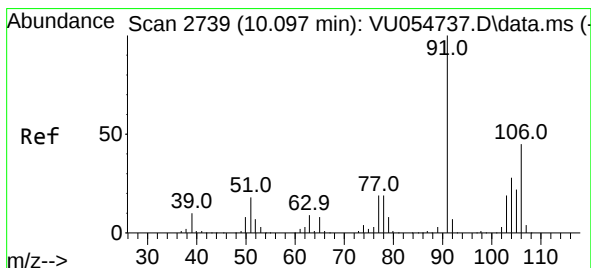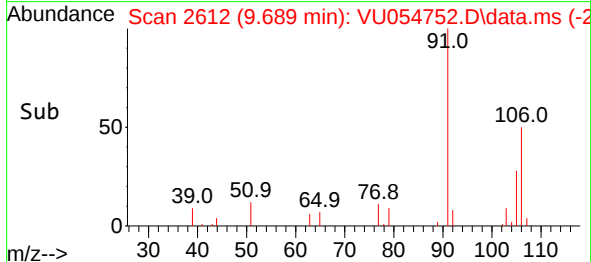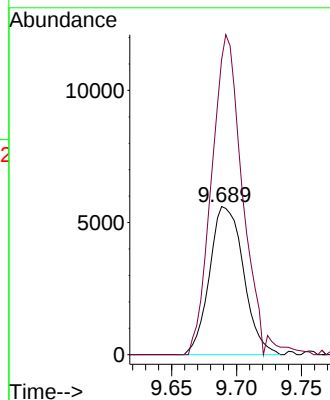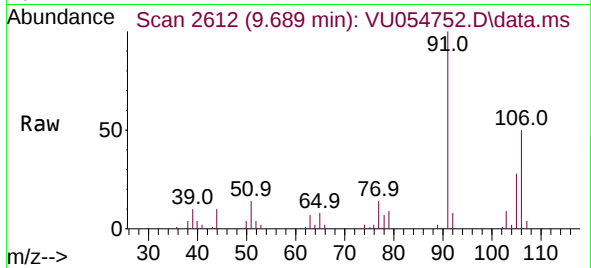

#54
o-Xylene
Concen: 0.161 ug/L
RT: 10.103 min Scan# 2741
Delta R.T. 0.007 min
Lab File: VU054752.D
Acq: 03 Jul 2023 16:29

Tgt Ion:106 Resp: 5635
Ion Ratio Lower Upper
106 100
91 214.7 154.5 286.9

