

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
 Data File : VU054741.D
 Acq On : 03 Jul 2023 11:56
 Operator : MD/SY
 Sample : 03495-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0FA7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	65	71	80	rBV	36485	43485	4.15%	0.579%
2	1.596	88	95	114	rVB	91490	112449	10.73%	1.498%
3	1.908	185	192	215	rVB	90011	139003	13.26%	1.851%
4	2.560	381	395	411	rBV	151322	251139	23.96%	3.345%
5	3.184	575	589	606	rVB2	8412	18573	1.77%	0.247%
6	4.628	1025	1038	1072	rBV	163857	440753	42.06%	5.870%
7	5.059	1156	1172	1190	rVB	161579	354519	33.83%	4.722%
8	5.721	1356	1378	1402	rBV2	312659	823893	78.62%	10.973%
9	6.245	1527	1541	1565	rBV	321601	628951	60.01%	8.377%
10	6.685	1665	1678	1696	rBV	209184	413655	39.47%	5.509%
11	7.563	1936	1951	1967	rBV	99438	181752	17.34%	2.421%
12	7.894	2042	2054	2071	rBV	349919	618328	59.00%	8.236%
13	8.177	2131	2142	2165	rBV	63808	110621	10.56%	1.473%
14	8.550	2246	2258	2271	rVB5	8991	17055	1.63%	0.227%
15	8.631	2271	2283	2317	rBV	545179	1047993	100.00%	13.958%
16	9.415	2513	2527	2552	rBV	454865	775180	73.97%	10.325%
17	10.753	2927	2943	2960	rBV	167170	276014	26.34%	3.676%
18	11.807	3260	3271	3296	rBV	427885	687248	65.58%	9.153%
19	12.190	3378	3390	3411	rBV	340776	567442	54.15%	7.558%




Sum of corrected areas: 7508053

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
Data File : VU054741.D
Acq On : 03 Jul 2023 11:56
Operator : MD/SY
Sample : 03495-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

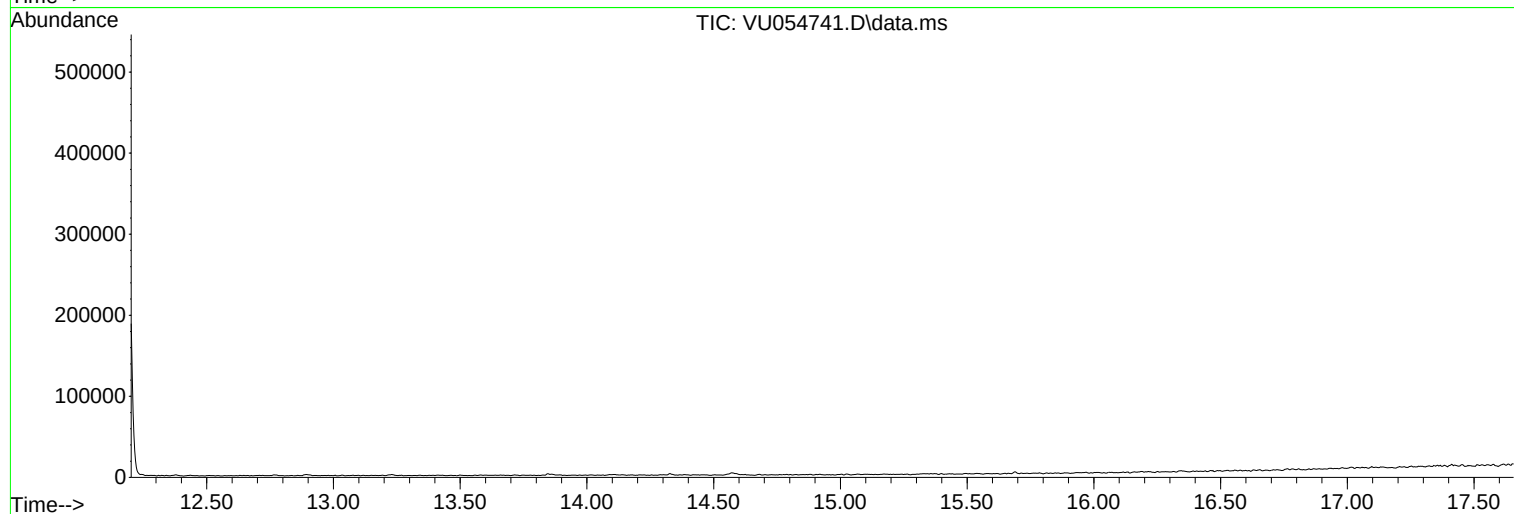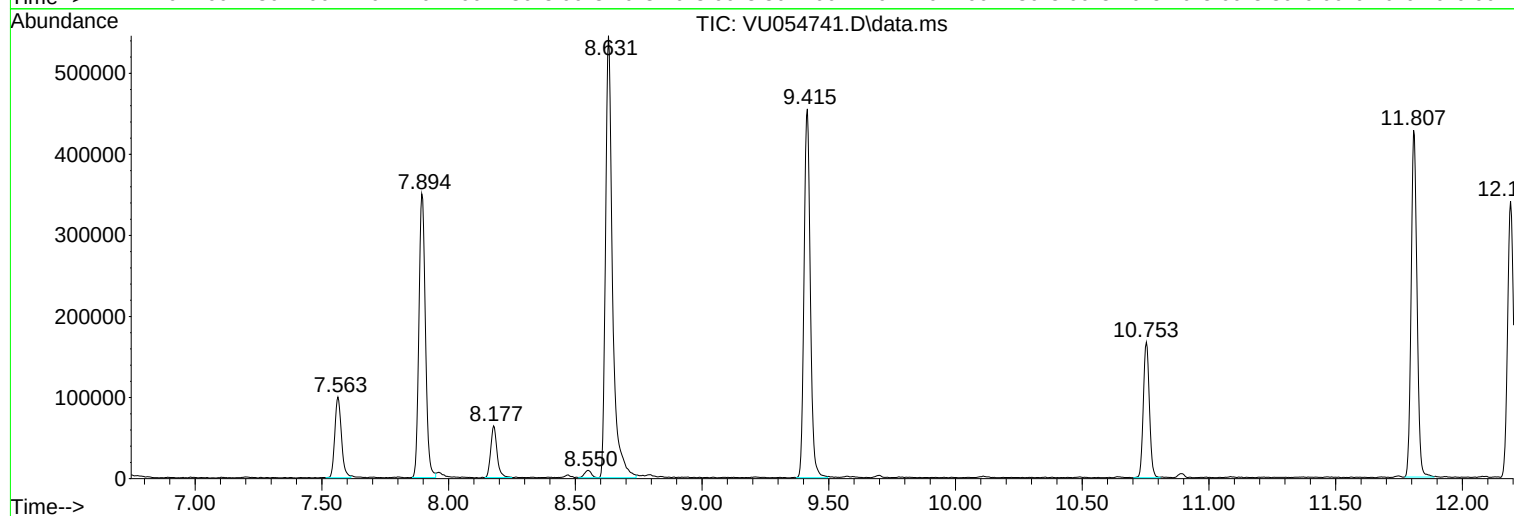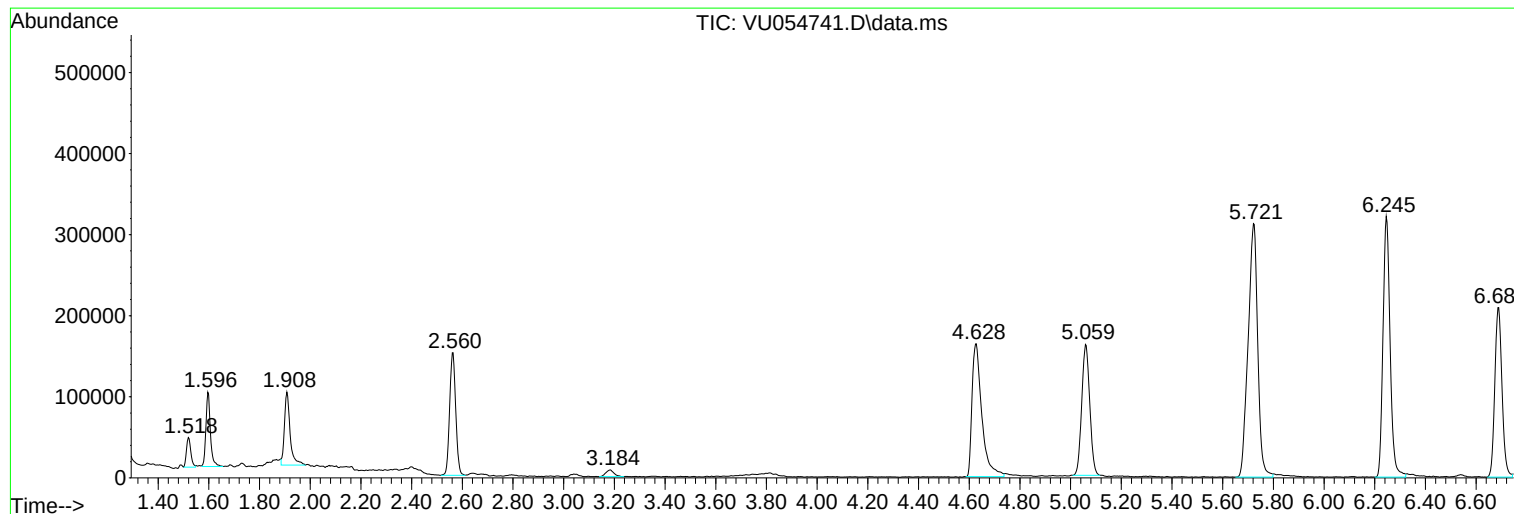

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
Data File : VU054741.D
Acq On : 03 Jul 2023 11:56
Operator : MD/SY
Sample : 03495-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
Data File : VU054741.D
Acq On : 03 Jul 2023 11:56
Operator : MD/SY
Sample : 03495-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------