

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
 Data File : VU054743.D
 Acq On : 03 Jul 2023 12:45
 Operator : MD/SY
 Sample : 03495-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0FB0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054743.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	66	71	79	rBV2	11940	14446	1.43%	0.196%
2	1.595	89	95	112	rVB	89949	107932	10.67%	1.468%
3	1.730	131	137	145	rVB2	10059	12455	1.23%	0.169%
4	1.907	185	192	207	rVB	85359	121806	12.04%	1.657%
5	2.560	384	395	408	rBV	147771	243154	24.03%	3.307%
6	3.177	572	587	604	rBV2	11437	28466	2.81%	0.387%
7	4.624	1026	1037	1071	rBV	163106	428553	42.35%	5.829%
8	5.058	1156	1172	1197	rBV2	166489	410824	40.60%	5.588%
9	5.721	1358	1378	1399	rBV2	304359	791808	78.25%	10.770%
10	6.245	1525	1541	1560	rBV	312269	604143	59.70%	8.217%
11	6.688	1665	1679	1700	rBV	203208	400253	39.55%	5.444%
12	7.563	1937	1951	1970	rBV	98605	180447	17.83%	2.454%
13	7.894	2038	2054	2070	rBV	345795	602114	59.50%	8.190%
14	8.177	2128	2142	2159	rBV	63149	110271	10.90%	1.500%
15	8.553	2246	2259	2269	rVB5	12895	23595	2.33%	0.321%
16	8.631	2271	2283	2320	rBV2	519940	1011909	100.00%	13.763%
17	9.415	2514	2527	2549	rBV	438334	748979	74.02%	10.187%
18	10.753	2929	2943	2959	rBV2	166015	269593	26.64%	3.667%
19	10.891	2975	2986	2996	rVB2	9474	16416	1.62%	0.223%
20	11.807	3260	3271	3294	rBV	417088	671032	66.31%	9.127%
21	12.190	3378	3390	3413	rBV	336166	553998	54.75%	7.535%




Sum of corrected areas: 7352194

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
Data File : VU054743.D
Acq On : 03 Jul 2023 12:45
Operator : MD/SY
Sample : 03495-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

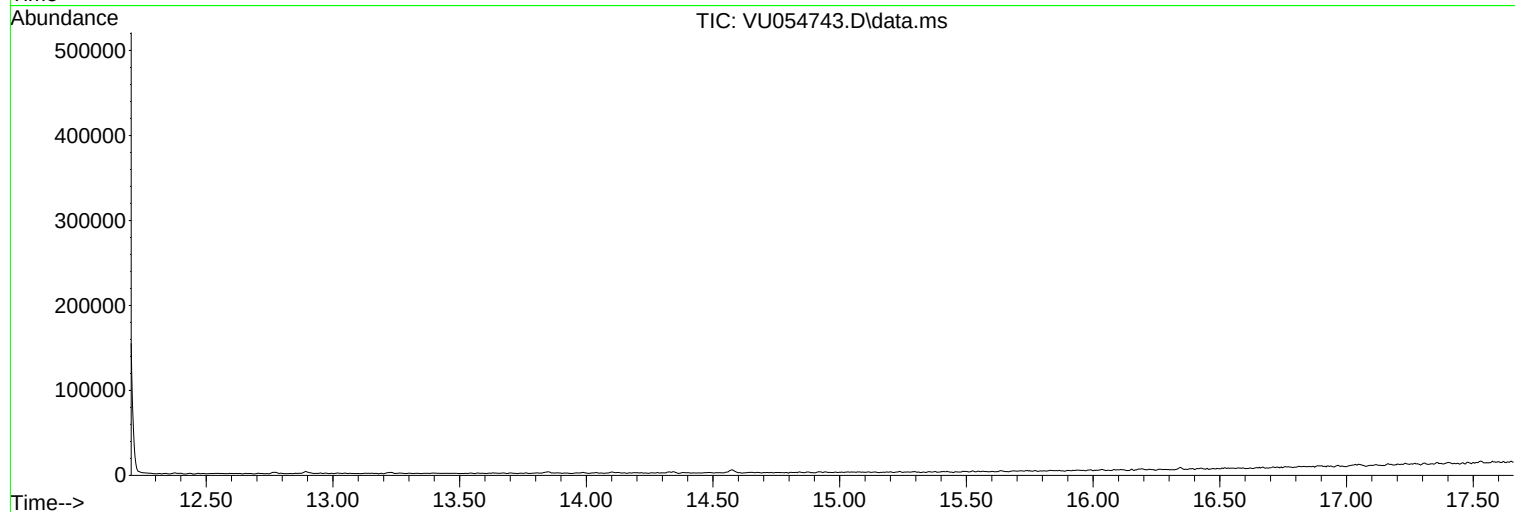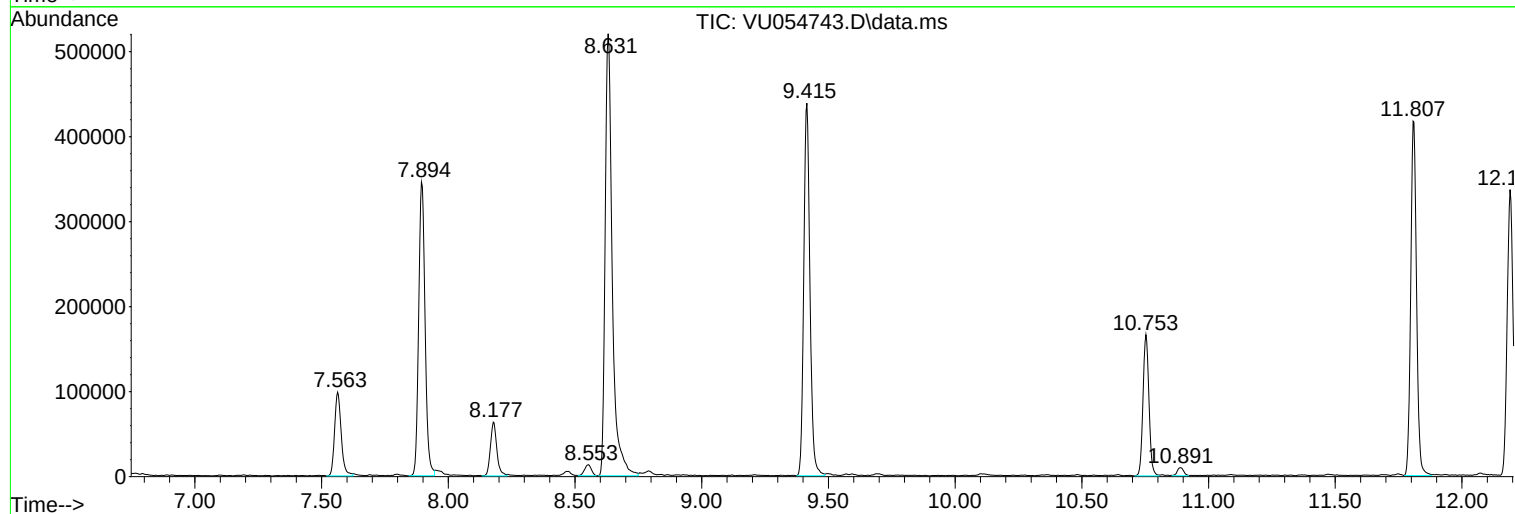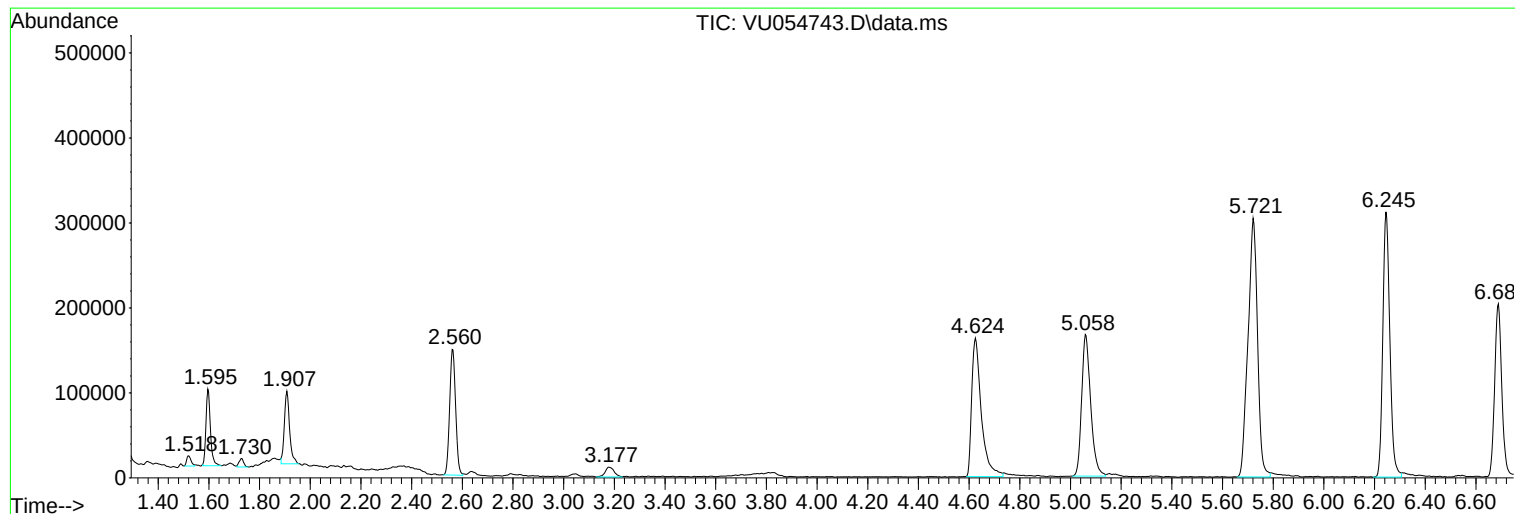

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
Data File : VU054743.D
Acq On : 03 Jul 2023 12:45
Operator : MD/SY
Sample : 03495-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
Data File : VU054743.D
Acq On : 03 Jul 2023 12:45
Operator : MD/SY
Sample : 03495-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc